

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
 Data File : BG056765.D
 Acq On : 1 Mar 2023 15:46
 Operator : CG/JU
 Sample : PB151097BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK097

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.134	98	101	112	rBV	50821	85459	17.27%	1.714%
2	6.343	474	477	480	rBV2	871	1292	0.26%	0.026%
3	6.943	577	579	583	rBV	947	1112	0.22%	0.022%
4	7.536	674	680	687	rBV	62147	107756	21.78%	2.162%
5	7.724	705	712	718	rBV	45547	76616	15.48%	1.537%
6	7.941	742	749	758	rVB	57542	100062	20.22%	2.007%
7	8.417	824	830	837	rBV2	55299	92497	18.69%	1.856%
8	9.105	940	947	954	rBV2	80081	133952	27.07%	2.687%
9	9.592	1020	1030	1037	rBV	62857	115674	23.38%	2.321%
10	10.321	1147	1154	1161	rBV	52393	92366	18.67%	1.853%
11	10.856	1239	1245	1256	rBV	80830	141007	28.50%	2.829%
12	11.255	1306	1313	1321	rBV	83069	145407	29.39%	2.917%
13	11.379	1326	1334	1342	rVB	80027	144409	29.19%	2.897%
14	12.806	1572	1577	1581	rBV4	1197	1715	0.35%	0.034%
15	13.558	1702	1705	1710	rBV	547	746	0.15%	0.015%
16	14.404	1840	1849	1857	rBV	172044	248524	50.23%	4.986%
17	14.722	1896	1903	1909	rBV2	180090	288205	58.25%	5.782%
18	15.021	1947	1954	1960	rVB	152384	237056	47.91%	4.756%
19	15.174	1973	1980	1991	rBV	76381	120839	24.42%	2.424%
20	16.003	2115	2121	2128	rVB	244800	367944	74.36%	7.381%
21	16.102	2132	2138	2144	rBV	67932	97669	19.74%	1.959%
22	16.243	2160	2162	2165	rBV2	1049	820	0.17%	0.016%
23	16.396	2183	2188	2191	rBV	533	707	0.14%	0.014%
24	17.753	2412	2419	2427	rBV	212800	310005	62.65%	6.219%
25	17.853	2429	2436	2446	rBV2	270153	413842	83.64%	8.302%
26	18.118	2476	2481	2484	rVB	797	1220	0.25%	0.024%
27	19.293	2679	2681	2684	rBV	562	809	0.16%	0.016%
28	19.399	2695	2699	2700	rBV2	764	849	0.17%	0.017%
29	19.604	2731	2734	2736	rBV2	684	1055	0.21%	0.021%
30	19.681	2742	2747	2750	rBV2	3958	5164	1.04%	0.104%
31	19.745	2755	2758	2761	rVV2	3057	4234	0.86%	0.085%
32	19.798	2765	2767	2769	rBV	1058	1009	0.20%	0.020%
33	19.845	2773	2775	2778	rVB2	698	782	0.16%	0.016%
34	20.068	2810	2813	2814	rBV	745	866	0.18%	0.017%
35	20.110	2814	2820	2828	rVV	347121	494801	100.00%	9.926%
36	20.233	2839	2841	2843	rBV2	1220	1183	0.24%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
 Data File : BG056765.D
 Acq On : 1 Mar 2023 15:46
 Operator : CG/JU
 Sample : PB151097BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK097

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	20.374	2862	2865	2868	rBV2	1418	1445	0.29%	0.029%
38	20.515	2887	2889	2893	rBV3	1194	1980	0.40%	0.040%
39	20.873	2949	2950	2952	rBV2	1503	1097	0.22%	0.022%
40	21.966	3132	3136	3137	rBV4	1748	1784	0.36%	0.036%
41	22.060	3146	3152	3160	rVB2	197045	333773	67.46%	6.696%
42	22.260	3184	3186	3188	rBV2	1742	998	0.20%	0.020%
43	22.460	3218	3220	3221	rVB2	2143	950	0.19%	0.019%
44	24.428	3553	3555	3556	rBV2	1781	1211	0.24%	0.024%
45	24.510	3567	3569	3570	rBV2	1933	1177	0.24%	0.024%
46	25.339	3700	3710	3722	rVB	159900	467414	94.47%	9.377%
47	25.580	3741	3751	3764	rBV2	102882	323822	65.44%	6.496%
48	26.197	3854	3856	3860	rBV3	1969	2234	0.45%	0.045%
49	27.795	4126	4128	4129	rBV2	1940	1151	0.23%	0.023%
50	27.812	4129	4131	4132	rBV2	1689	883	0.18%	0.018%
51	29.275	4378	4380	4383	rBV4	1675	2042	0.41%	0.041%
52	30.662	4614	4616	4621	rBV5	1654	2510	0.51%	0.050%
53	30.779	4634	4636	4637	rBV2	2098	1225	0.25%	0.025%
54	31.338	4729	4731	4734	rBV2	1704	1484	0.30%	0.030%




Sum of corrected areas: 4984833

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
Data File : BG056765.D
Acq On : 1 Mar 2023 15:46
Operator : CG/JU
Sample : PB151097BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

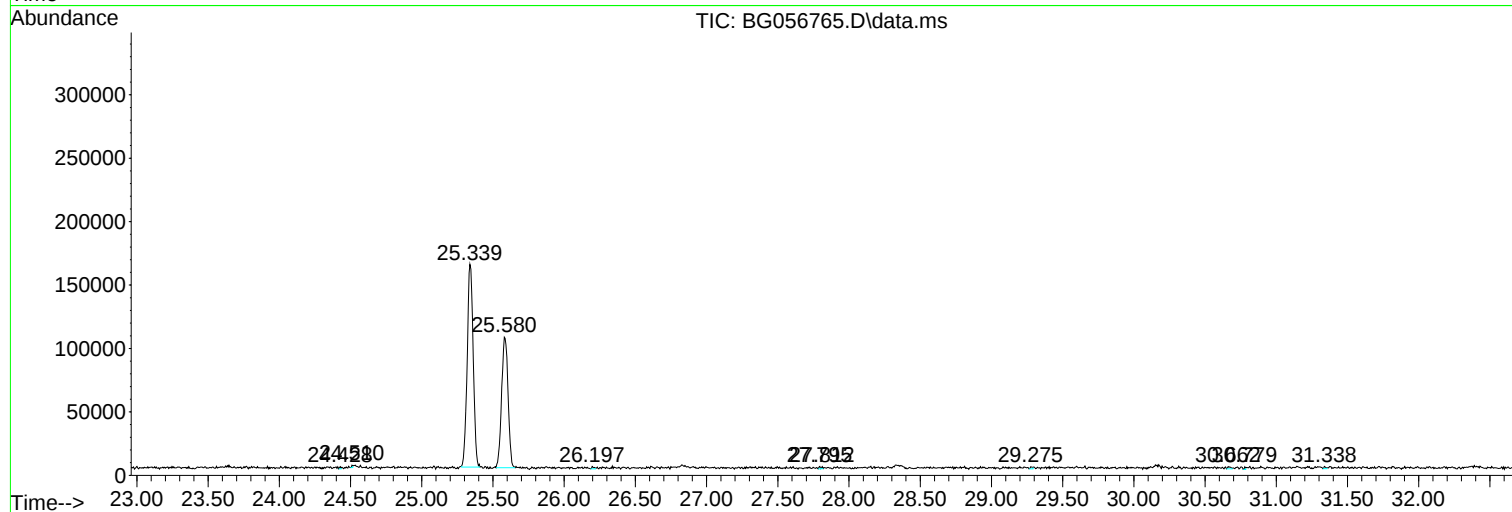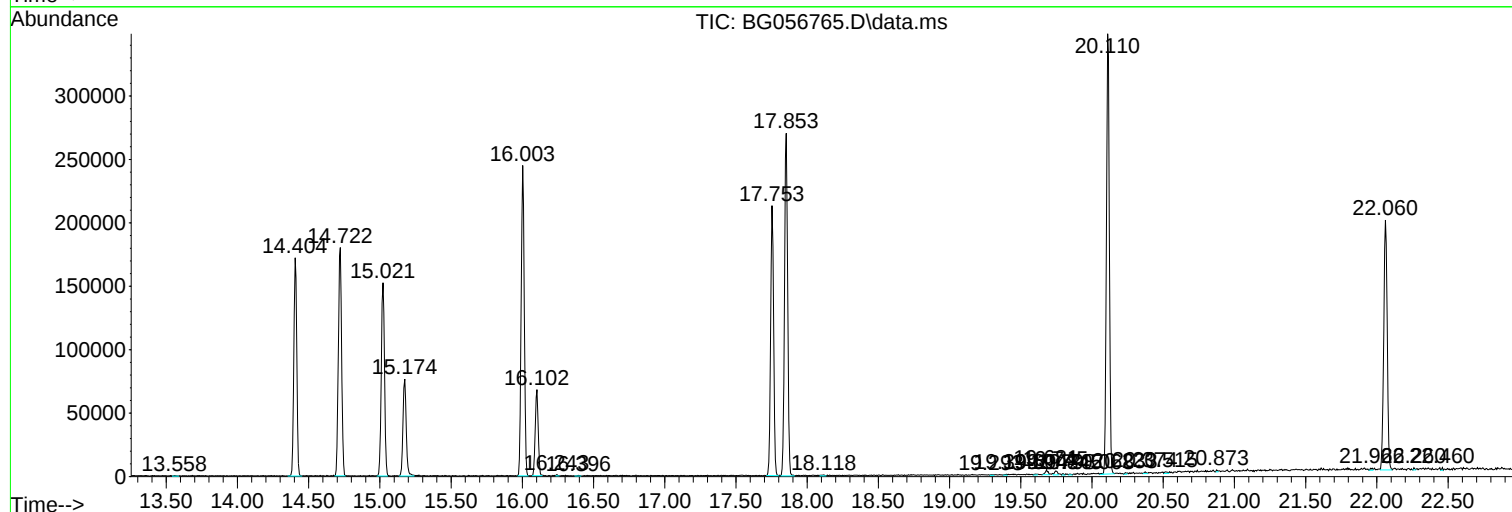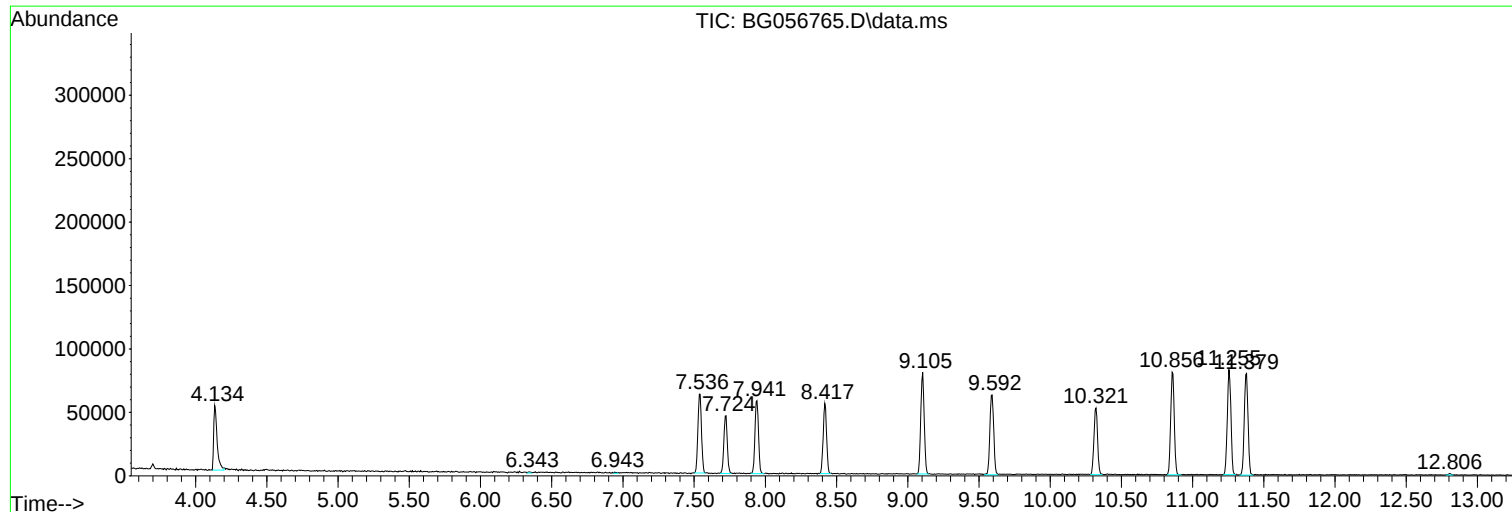

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
Data File : BG056765.D
Acq On : 1 Mar 2023 15:46
Operator : CG/JU
Sample : PB151097BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
Data File : BG056765.D
Acq On : 1 Mar 2023 15:46
Operator : CG/JU
Sample : PB151097BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc