

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
 Data File : BG056779.D
 Acq On : 2 Mar 2023 2:04
 Operator : CG/JU
 Sample : PB151097BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK097

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.698	24	27	32	rBV2	3660	4630	0.91%	0.089%
2	4.133	97	101	114	rBV	52542	89919	17.66%	1.737%
3	4.351	136	138	140	rBV2	1425	1138	0.22%	0.022%
4	5.044	255	256	258	rVB	1651	747	0.15%	0.014%
5	7.541	674	681	688	rVB2	67420	116798	22.94%	2.257%
6	7.723	706	712	721	rVB	47119	80598	15.83%	1.557%
7	7.940	743	749	756	rVB	62673	101880	20.01%	1.968%
8	8.416	824	830	837	rBV	60995	101939	20.03%	1.970%
9	9.104	941	947	955	rBV	84034	140445	27.59%	2.714%
10	9.591	1022	1030	1037	rBV	66313	118763	23.33%	2.295%
11	10.320	1148	1154	1161	rBV2	58967	102284	20.09%	1.976%
12	10.855	1238	1245	1254	rBV	85800	151237	29.71%	2.922%
13	11.254	1306	1313	1320	rBV	85053	151303	29.72%	2.923%
14	11.378	1327	1334	1343	rVB	82927	148721	29.22%	2.873%
15	14.404	1843	1849	1857	rVB	175807	253773	49.85%	4.903%
16	14.721	1895	1903	1910	rBV2	190477	297810	58.50%	5.754%
17	15.020	1948	1954	1962	rVB	154270	241150	47.37%	4.659%
18	15.173	1974	1980	1992	rBV	78197	123900	24.34%	2.394%
19	16.002	2115	2121	2128	rVB	250734	379912	74.63%	7.340%
20	16.102	2133	2138	2147	rBV2	77522	110487	21.70%	2.135%
21	16.243	2158	2162	2163	rBV	863	754	0.15%	0.015%
22	17.541	2379	2383	2386	rVB2	640	889	0.17%	0.017%
23	17.753	2413	2419	2427	rVB	219771	310520	61.00%	6.000%
24	17.852	2430	2436	2444	rVB2	281002	418257	82.17%	8.081%
25	18.223	2496	2499	2504	rVB	545	953	0.19%	0.018%
26	18.540	2550	2553	2556	rBV	630	804	0.16%	0.016%
27	18.969	2622	2626	2627	rBV2	820	848	0.17%	0.016%
28	19.380	2694	2696	2699	rBV2	713	759	0.15%	0.015%
29	19.639	2739	2740	2743	rVB2	691	714	0.14%	0.014%
30	19.680	2743	2747	2751	rBV2	4053	4927	0.97%	0.095%
31	19.750	2755	2759	2766	rBV3	3123	5796	1.14%	0.112%
32	20.109	2814	2820	2827	rBV	362487	509042	100.00%	9.835%
33	20.208	2835	2837	2842	rBV3	808	1314	0.26%	0.025%
34	20.338	2857	2859	2861	rBV2	668	826	0.16%	0.016%
35	20.426	2872	2874	2876	rBV3	863	706	0.14%	0.014%
36	20.743	2926	2928	2930	rBV	1018	824	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
 Data File : BG056779.D
 Acq On : 2 Mar 2023 2:04
 Operator : CG/JU
 Sample : PB151097BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK097

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	20.925	2958	2959	2962	rBV2	2062	1437	0.28%	0.028%
38	21.113	2989	2991	2994	rBV4	1282	1712	0.34%	0.033%
39	21.760	3099	3101	3104	rVB4	1738	1040	0.20%	0.020%
40	21.789	3104	3106	3107	rBV	1454	917	0.18%	0.018%
41	21.877	3119	3121	3122	rBV2	1371	812	0.16%	0.016%
42	22.059	3145	3152	3162	rVB	202005	346657	68.10%	6.698%
43	22.929	3298	3300	3301	rBV2	1637	1105	0.22%	0.021%
44	22.952	3302	3304	3305	rBV	2746	1387	0.27%	0.027%
45	23.910	3465	3467	3468	rBV	1677	1488	0.29%	0.029%
46	24.515	3569	3570	3572	rBV2	2206	1928	0.38%	0.037%
47	24.962	3644	3646	3649	rBV4	1824	2134	0.42%	0.041%
48	25.338	3700	3710	3723	rVB2	155616	486168	95.51%	9.393%
49	25.585	3741	3752	3764	rVB	115096	338675	66.53%	6.544%
50	25.831	3792	3794	3795	rBV2	1608	1573	0.31%	0.030%
51	25.961	3815	3816	3817	rBV	1402	704	0.14%	0.014%
52	26.724	3944	3946	3947	rBV2	1515	1178	0.23%	0.023%
53	27.406	4060	4062	4065	rBV2	2126	2435	0.48%	0.047%
54	27.735	4116	4118	4120	rBV3	1628	1442	0.28%	0.028%
55	27.899	4144	4146	4149	rVB4	1659	1111	0.22%	0.021%
56	28.416	4232	4234	4235	rBV	1458	1055	0.21%	0.020%
57	29.186	4363	4365	4367	rBV3	1545	1238	0.24%	0.024%
58	29.838	4474	4476	4478	rBV3	1437	1003	0.20%	0.019%
59	29.932	4490	4492	4493	rBV2	1607	1150	0.23%	0.022%
60	30.943	4663	4664	4665	rBV	1915	903	0.18%	0.017%
61	31.924	4829	4831	4832	rVB2	1947	1051	0.21%	0.020%




Sum of corrected areas: 5175670

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
Data File : BG056779.D
Acq On : 2 Mar 2023 2:04
Operator : CG/JU
Sample : PB151097BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

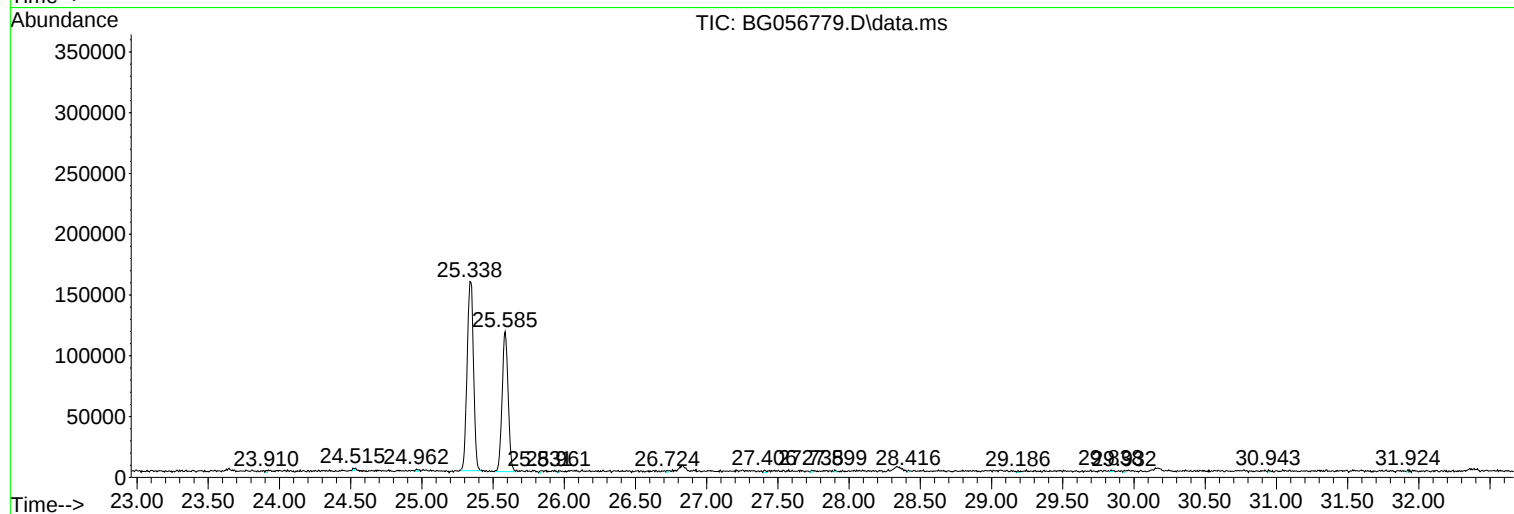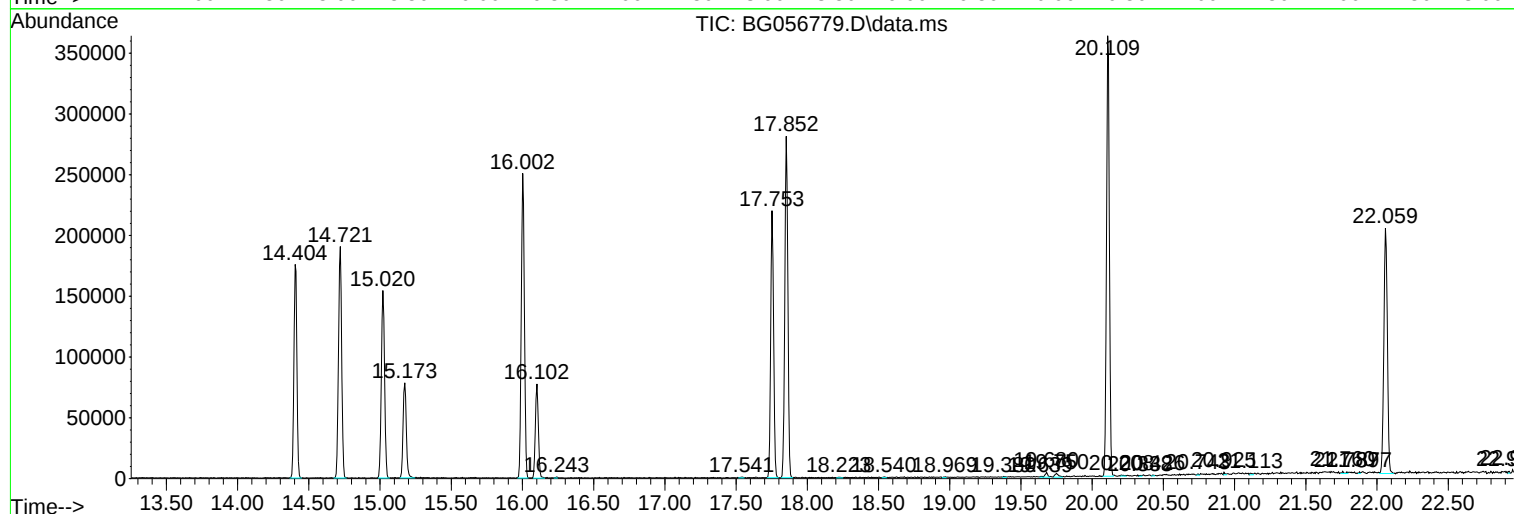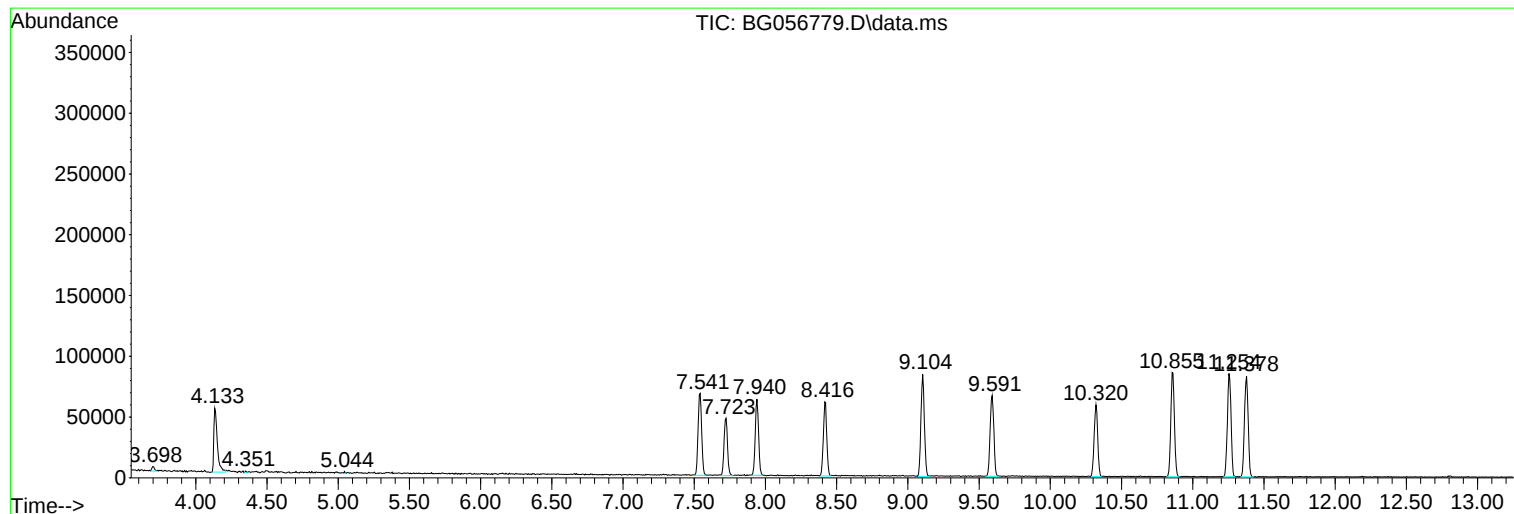

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
Data File : BG056779.D
Acq On : 2 Mar 2023 2:04
Operator : CG/JU
Sample : PB151097BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030123\
Data File : BG056779.D
Acq On : 2 Mar 2023 2:04
Operator : CG/JU
Sample : PB151097BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc