

Data File : BG044632.D

Acq On : 2 Mar 2020 13:13

Operator : CG/JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1



Quant Time: Mar 03 08:35:33 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Feb 24 16:11:23 2020

Response via : Initial Calibration

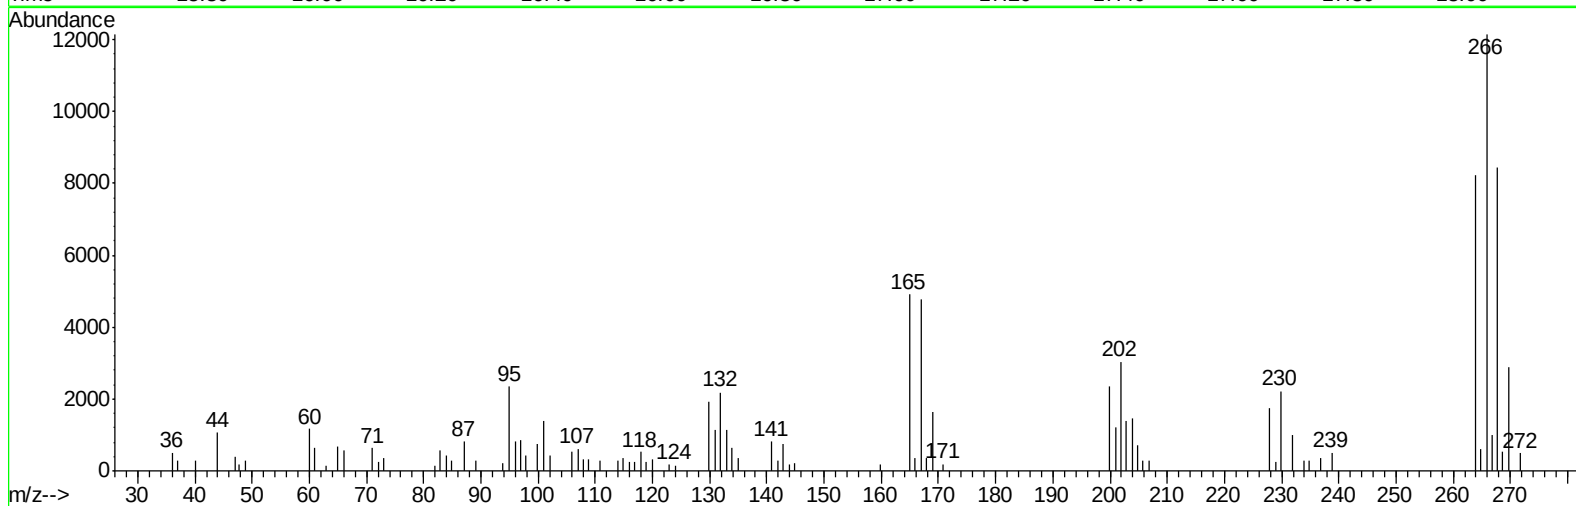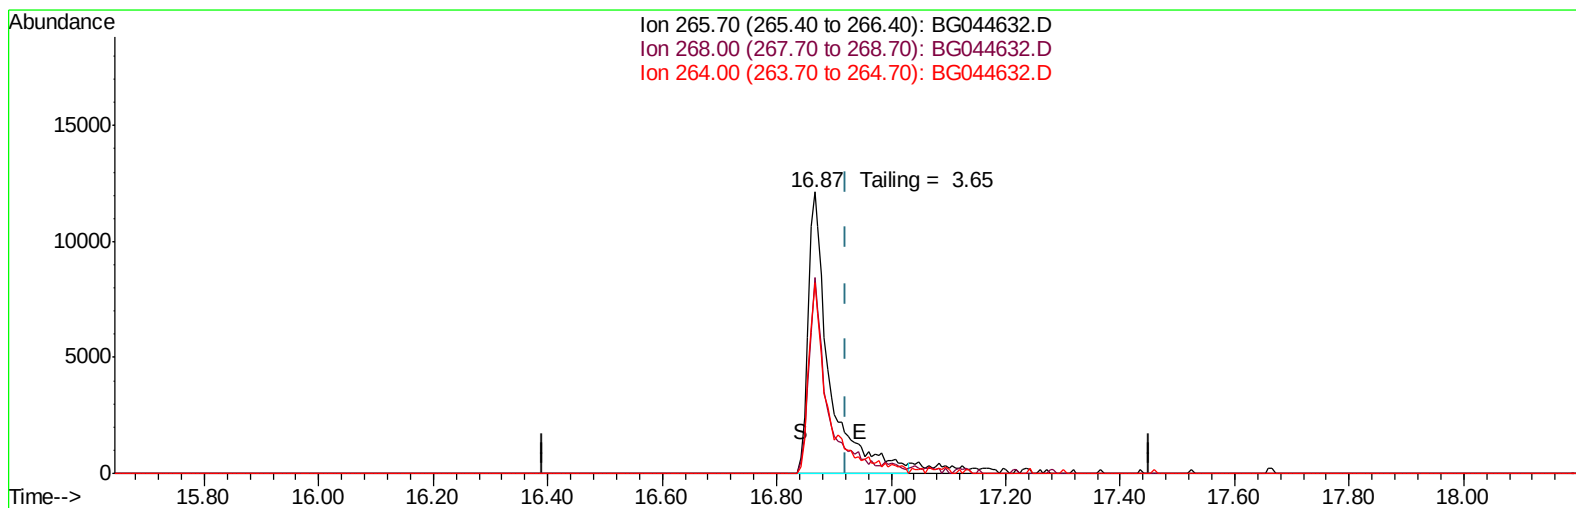

TIC: BG044632.D

(70) Pentachlorophenol (C)



16.866min (-0.055) 21618.14ng

response 29059

Ion	Exp%	Act%
265.70	100	100
268.00	66.70	73.82
264.00	66.20	67.70
0.00	0.00	0.00

Data File : BG044632.D
Acq On : 2 Mar 2020 13:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 08:35:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

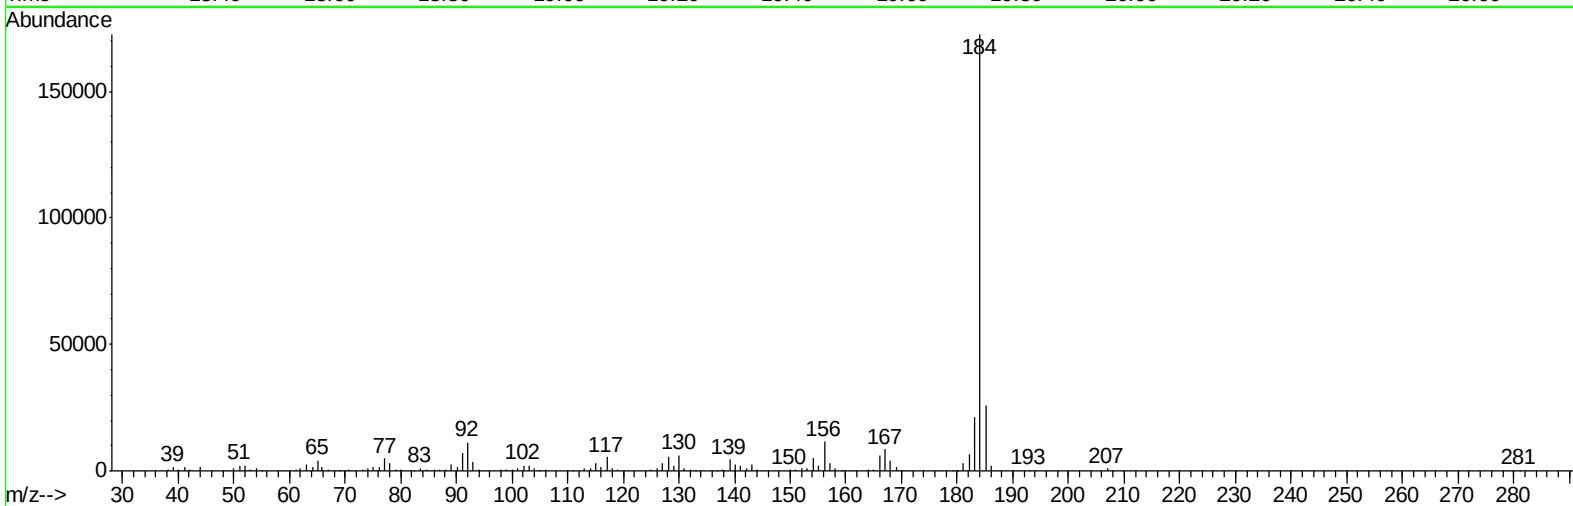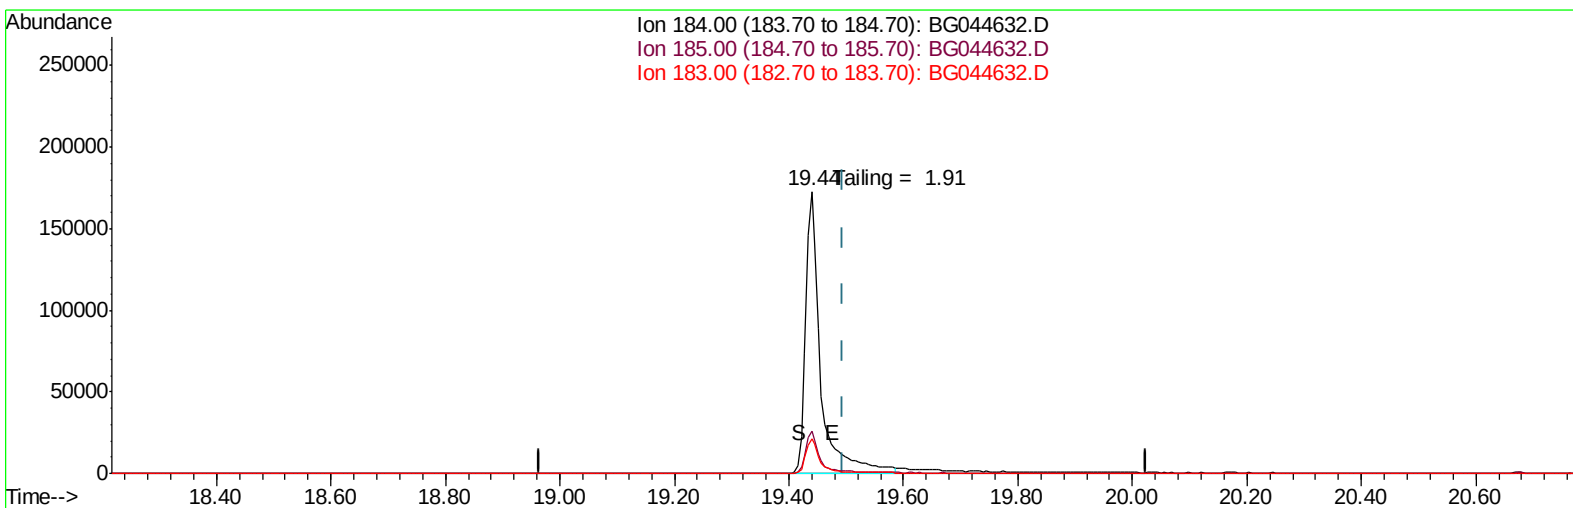

TIC: BG044632.D

(77) Benzidine

19.439min (-0.055) 0.00ng

response 323768

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.94
183.00	12.40	12.19
0.00	0.00	0.00