

Data File : BG044648.D

Acq On : 3 Mar 2020 1:04

Operator : CG/JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1



Quant Time: Mar 03 08:36:30 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Feb 24 16:11:23 2020

Response via : Initial Calibration

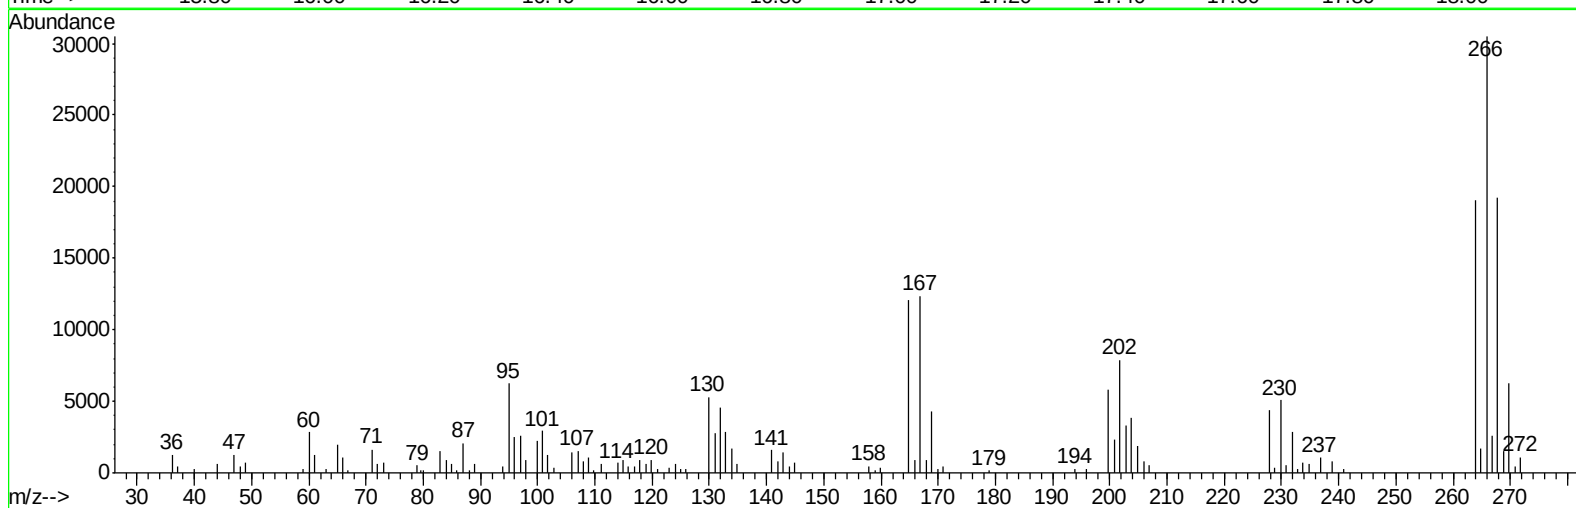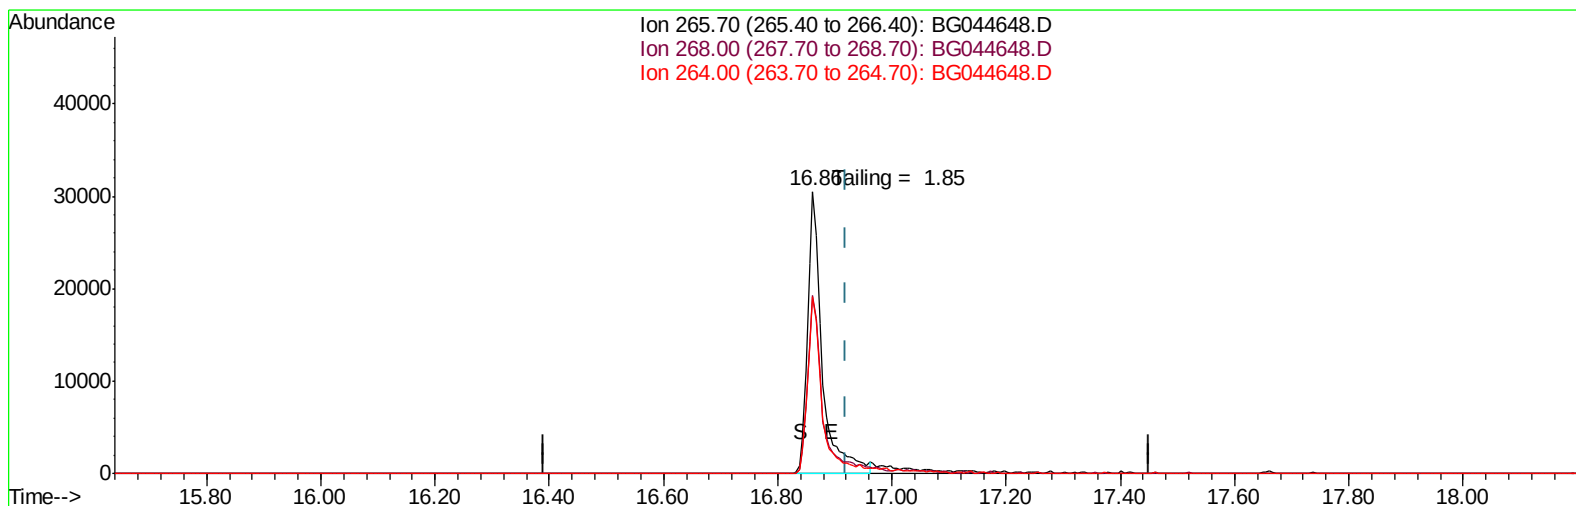

TIC: BG044648.D

(70) Pentachlorophenol (C)



16.861min (-0.060) 21274.60ng

response 53499

Ion	Exp%	Act%
265.70	100	100
268.00	66.70	63.17
264.00	66.20	62.59
0.00	0.00	0.00

Data File : BG044648.D
Acq On : 3 Mar 2020 1:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 08:36:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

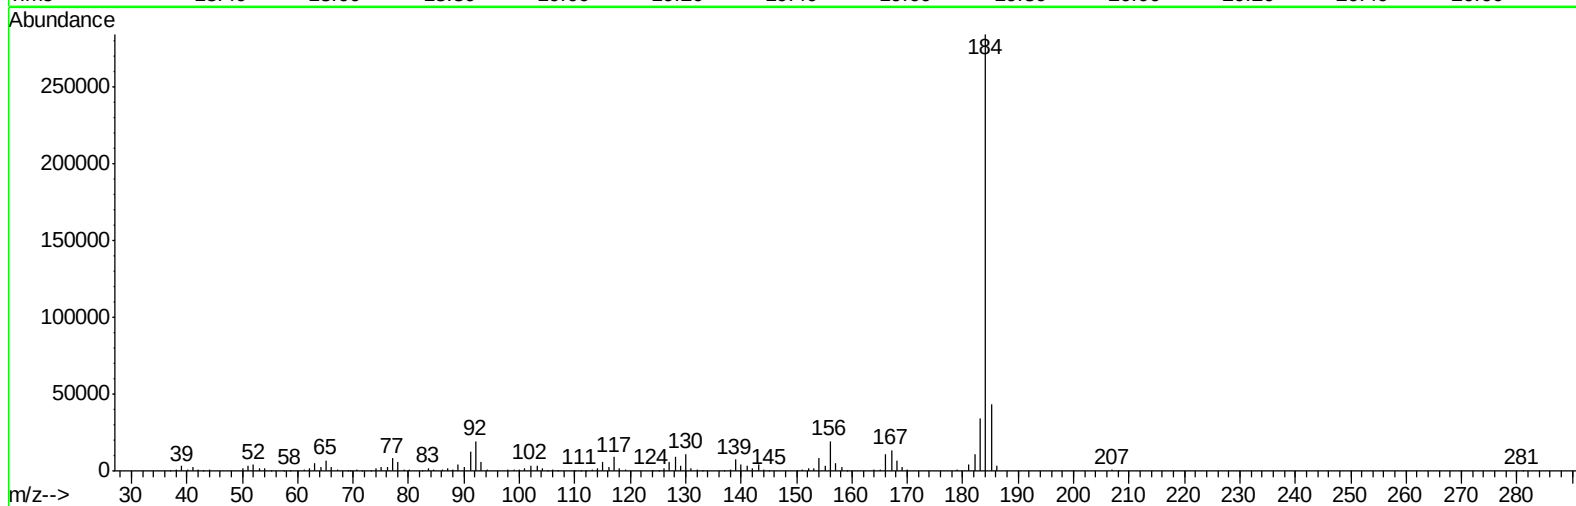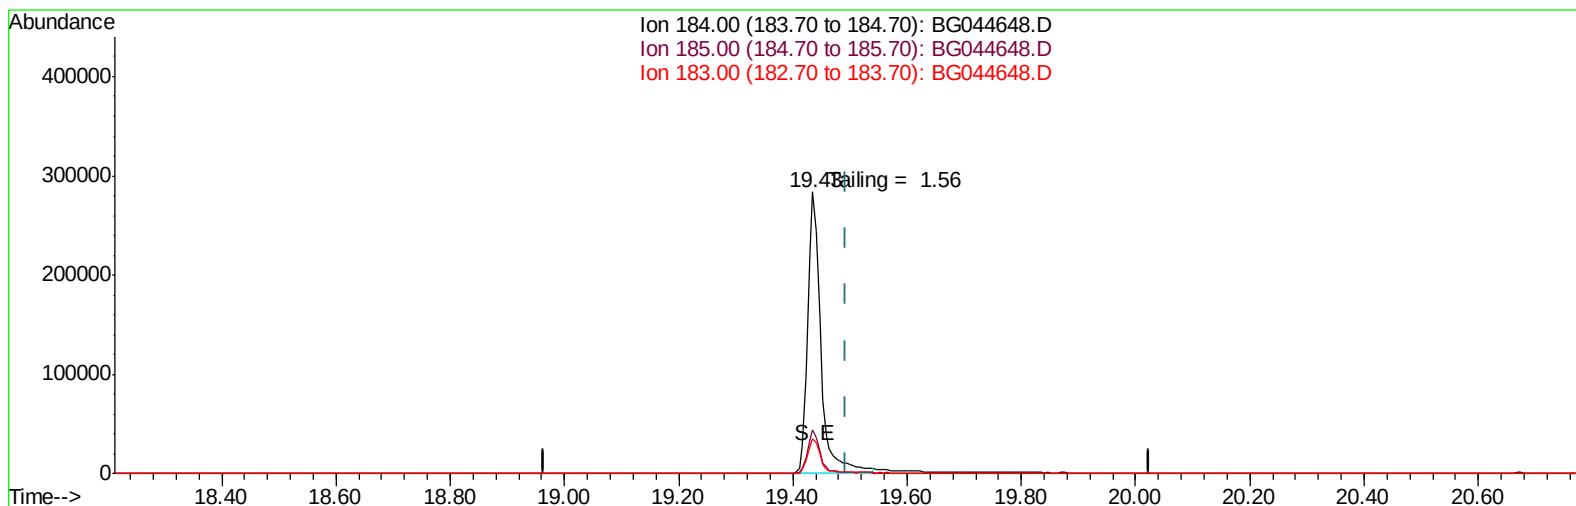

TIC: BG044648.D

(77) Benzidine

19.435min (-0.060) 0.00ng

response 475143

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	15.25
183.00	12.40	12.17
0.00	0.00	0.00