

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030220\
 Data File : BG044660.D
 Acq On : 3 Mar 2020 10:41
 Operator : CG/JU
 Sample : L1743-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C-3

Manual Integrations
 APPROVED

mohammad
 3/4/2020 2:48:28 PM

Quant Time: Mar 03 18:37:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 24 16:11:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	83425	20.00	ng	-0.07
21) Naphthalene-d8	10.60	136	360668	20.00	ng	-0.07
39) Acenaphthene-d10	14.46	164	220409	20.00	ng	-0.06
64) Phenanthrene-d10	17.20	188	436454	20.00	ng	-0.06
76) Chrysene-d12	21.45	240	365319	20.00	ng	-0.05
87) Perylene-d12	24.48	264	432488	20.00	ng	-0.10
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	503197	96.78	ng	-0.07
7) Phenol-d6	6.98	99	662023	93.02	ng	-0.07
23) Nitrobenzene-d5	8.96	82	409991	58.56	ng	-0.07
42) 2,4,6-Tribromophenol	15.95	330	235109	75.23	ng	-0.06
45) 2-Fluorobiphenyl	13.08	172	880685	57.22	ng	-0.06
79) Terphenyl-d14	19.83	244	1113203	57.69	ng	-0.05
Target Compounds						Qvalue
31) Naphthalene	10.65	128	40801	2.073	ng	97
38) 1-Methylnaphthalene	12.49	142	32406	2.345	ng	98
49) Acenaphthylene	14.18	152	102351	4.848	ng	99
50) Dimethylphthalate	13.91	163	99846	5.613	ng	100
52) Acenaphthene	14.52	154	89007	6.613	ng	98
55) Dibenzofuran	14.86	168	97814	4.741	ng	95
58) Fluorene	15.50	166	144908	8.858	ng	100
71) Phenanthrene	17.25	178	2168815m	89.755	ng	
72) Anthracene	17.34	178	546988	22.970	ng	100
73) Carbazole	17.61	167	198141	9.141	ng	98
75) Fluoranthene	19.27	202	3065426	107.165	ng	79
78) Pvrene	19.63	202	2868329	108.162	ng	# 81
80) Butylbenzylphthalate	20.52	149	98189	8.465	ng	95
81) Benzo(a)anthracene	21.43	228	1833680	71.417	ng	92
83) Chrysene	21.49	228	1773944m	71.458	ng	
84) Bis(2-ethylhexyl)phthalate	21.36	149	2512530	157.197	ng	# 81
86) Indeno(1,2,3-cd)pyrene	27.91	276	1246214	39.116	ng	94
88) Benzo(b)fluoranthene	23.54	252	2500817	87.948	ng	# 94
89) Benzo(k)fluoranthene	23.58	252	804856m	29.172	ng	
90) Benzo(a)pyrene	24.35	252	1828472	68.440	ng	96
91) Dibenz(a,h)anthracene	27.94	278	292949	11.087	ng	94
92) Benzo(g,h,i)perylene	28.98	276	1181011	44.613	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030220\
Data File : BG044660.D
Acq On : 3 Mar 2020 10:41
Operator : CG/JU
Sample : L1743-08
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C-3

Manual Integrations
APPROVED

mohammad
3/4/2020 2:48:28 PM

Quant Time: Mar 03 18:37:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

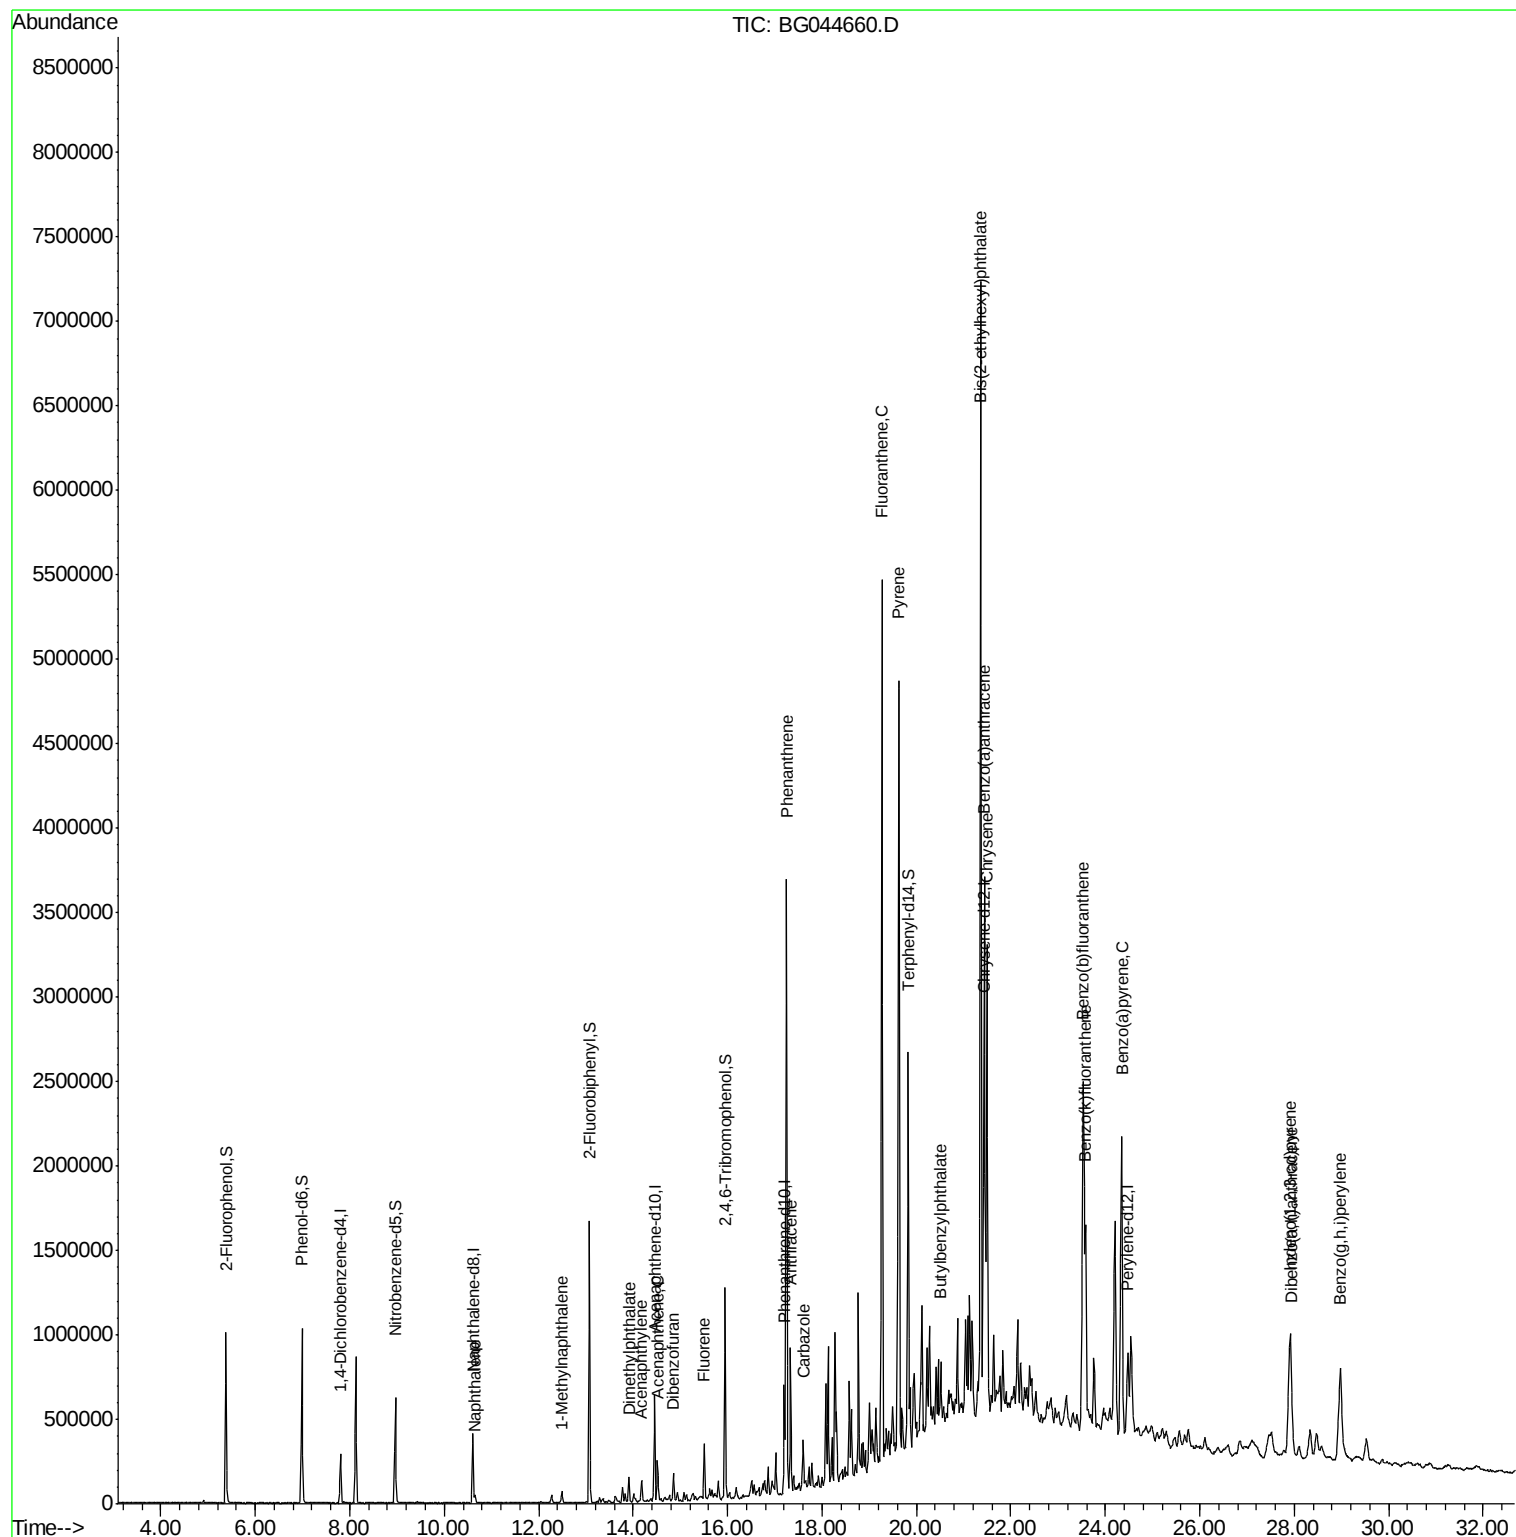



#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.81 min Scan# 803
Delta R.T. -0.07 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Instrument :
BNA_G
ClientSampled :
C-3

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.1	128.9	193.3
115	57.9	47.0	70.4

Manual Integrations
APPROVED

mohammad
3/4/2020 2:48:28 PM

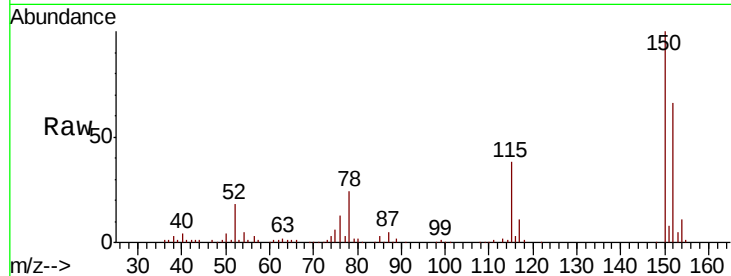



Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E


Time-->

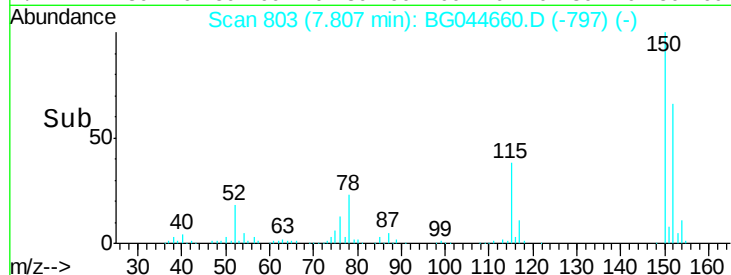

#5

2-Fluorophenol
Concen: 96.777 ng
RT: 5.38 min Scan# 390
Delta R.T. -0.07 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.0	44.8	67.2
63	29.7	22.3	33.5




Abundance


Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

Time-->

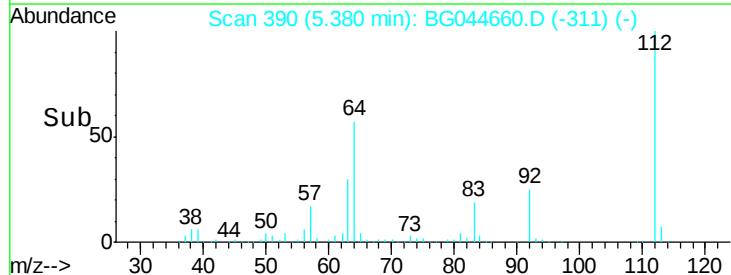



#7

Phenol-d6

Concen: 93.018 ng

RT: 6.98 min Scan# 663

Delta R.T. -0.07 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Instrument :

BNA_G

ClientSampled :

C-3

Tot Ion: 99 Resp: 662023

Ion Ratio Lower Upper

99 100


42 17.3 12.8 19.2

71 32.0 24.4 36.6

Manual Integrations
APPROVED

mohammad

3/4/2020 2:48:28 PM



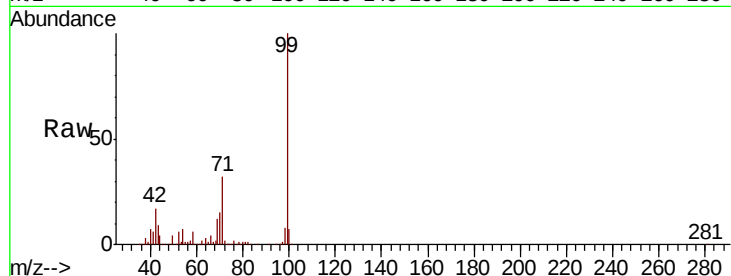


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

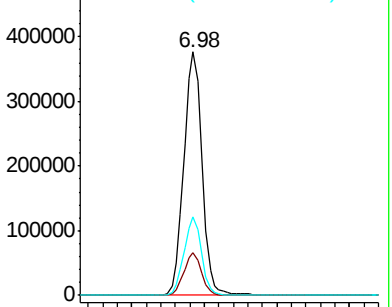

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.60 min Scan# 1279

Delta R.T. -0.07 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Tgt Ion: 136 Resp: 360668


Ion Ratio Lower Upper

136 100

137 11.4 8.8 13.2

54 7.4 5.7 8.5

68 5.7 4.5 6.7





Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

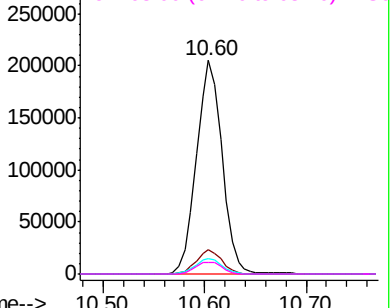







#23
Nitrobenzene-d5
Concen: 58.564 ng
RT: 8.96 min Scan# 1000
Delta R.T. -0.07 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Instrument :
BNA_G
ClientSampled :
C-3

Tot Ion	Ratio	Lower	Upper
82	100		
128	46.1	38.1	57.1
54	46.3	37.5	56.3




Manual Integrations
APPROVED


mohammad
3/4/2020 2:48:28 PM

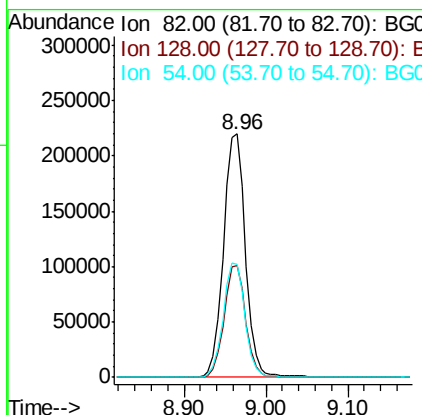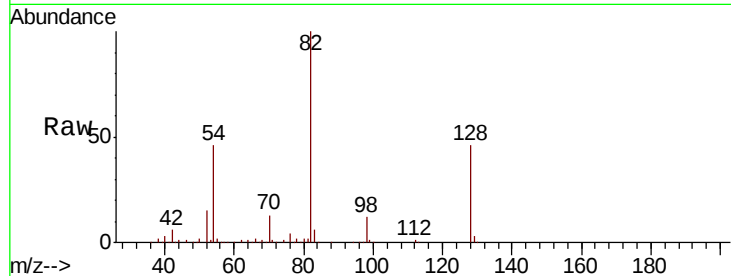

#31
Naphthalene
Concen: 2.073 ng
RT: 10.65 min Scan# 1287
Delta R.T. -0.07 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.4	9.0	13.6
127	12.3	11.0	16.4



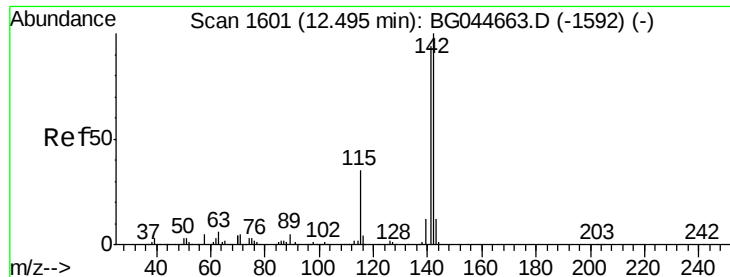





#38
1-Methylnaphthalene
Concen: 2.345 ng
RT: 12.49 min Scan# 1600
Delta R.T. -0.07 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Instrument :
BNA_G
ClientSampled :
C-3

Tot Ion	Ratio	Lower	Upper
142	100		
141	92.0	75.1	112.7
116	3.6	2.6	4.0




Manual Integrations
APPROVED


mohammad
3/4/2020 2:48:28 PM

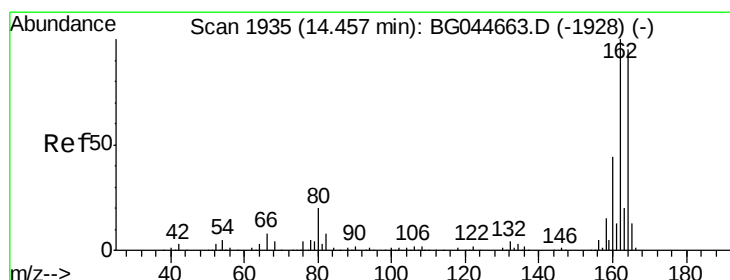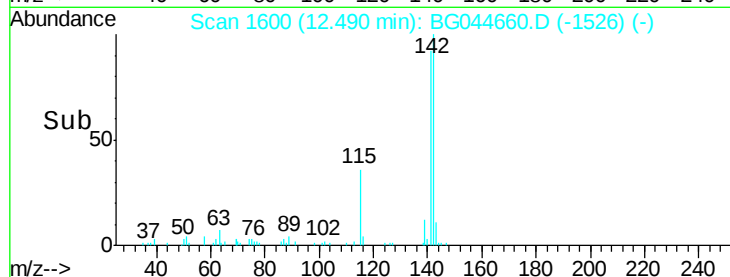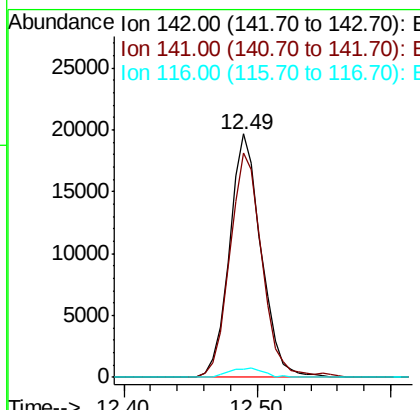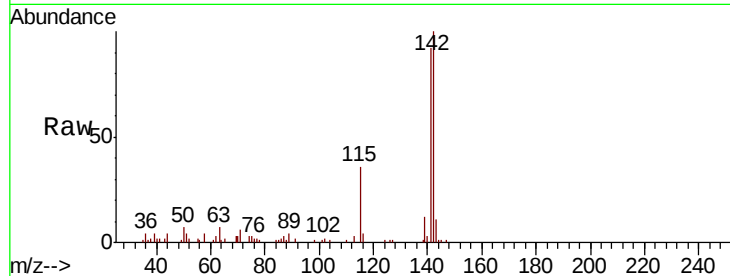

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.46 min Scan# 1935
Delta R.T. -0.06 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
164	100		
162	102.9	83.6	125.4
160	44.8	36.2	54.4

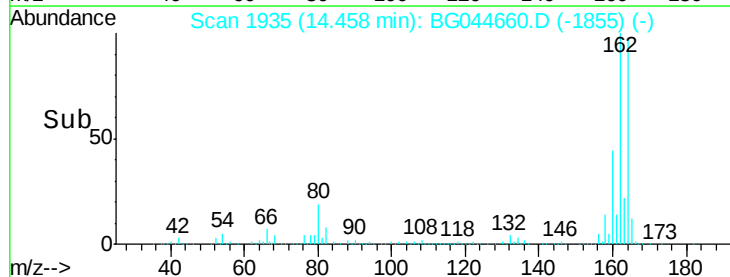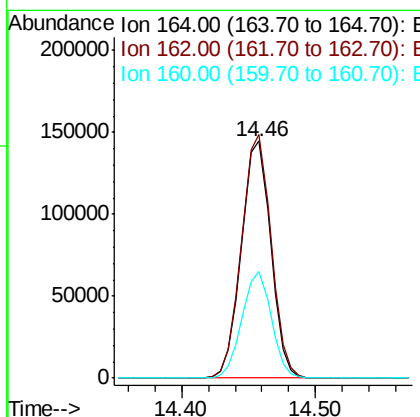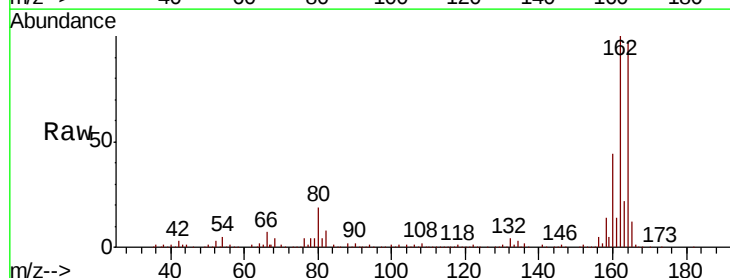







#42
 2,4,6-Tribromophenol
 Concen: 75.229 ng
 RT: 15.95 min Scan# 2189
 Delta R.T. -0.06 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Instrument :
 BNA_G
 ClientSampleId :
 C-3

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.7	77.4	116.0
141	33.8	26.1	39.1




Manual Integrations
 APPROVED


mohammad
 3/4/2020 2:48:28 PM

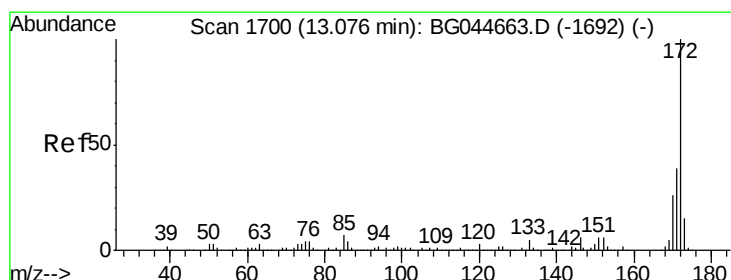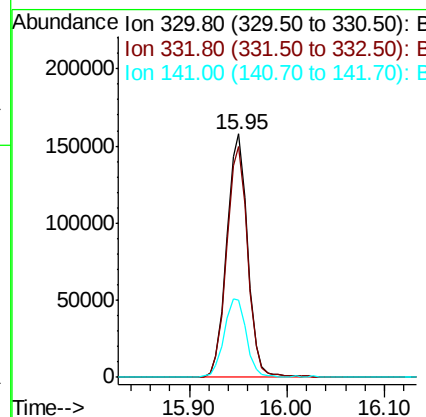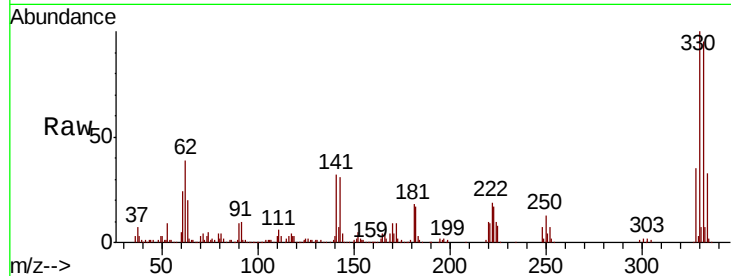

#45
 2-Fluorobiphenyl
 Concen: 57.218 ng
 RT: 13.08 min Scan# 1700
 Delta R.T. -0.06 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.2	31.3	46.9
170	25.1	21.0	31.4

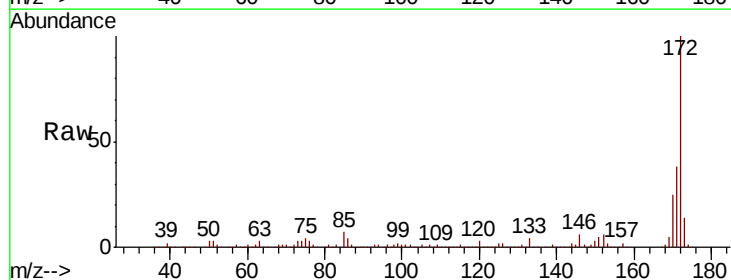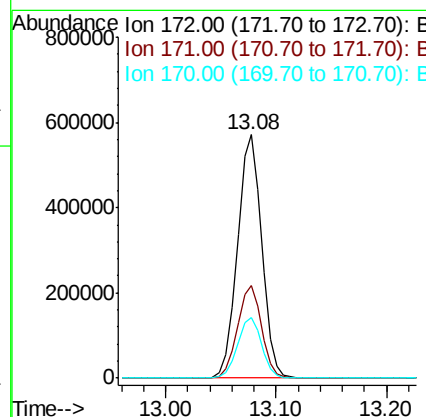



#49

Acenaphthylene

Concen: 4.848 ng

RT: 14.18 min Scan# 1887

Delta R.T. -0.06 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Instrument :

BNA_G





ClientSampleId :

C-3

Tot Ion:	152	Resp:	102351
Ion Ratio		Lower	Upper
152	100		
151	22.7	17.7	26.5
153	14.4	11.3	16.9

Manual Integrations
APPROVED

mohammad
3/4/2020 2:48:28 PM

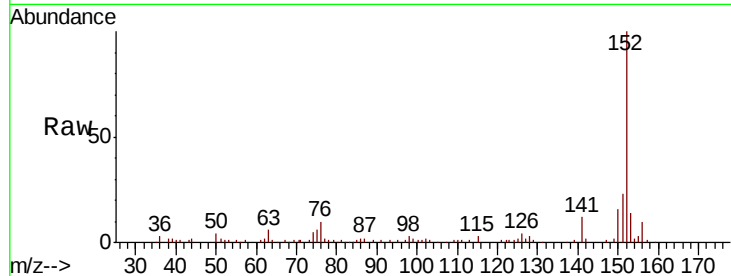

#50

Dimethylphthalate

Concen: 5.613 ng




RT: 13.91 min Scan# 1842


Delta R.T. -0.06 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Tgt Ion:	163	Resp:	99846
Ion Ratio		Lower	Upper
163	100		
194	4.0	3.4	5.0
164	10.9	8.7	13.1





#52

Acenaphthene

Concen: 6.613 ng

RT: 14.52 min Scan# 1945

Delta R.T. -0.07 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Instrument :

BNA_G





ClientSampleId :

C-3

Tot Ion:	154	Resp:	89007
Ion	Ratio	Lower	Upper
154	100		
153	110.1	89.4	134.0
152	51.7	43.0	64.4

Manual Integrations
APPROVED

mohammad
3/4/2020 2:48:28 PM



#55

Dibenzofuran

Concen: 4.741 ng




RT: 14.86 min Scan# 2003


Delta R.T. -0.06 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Tgt Ion:	168	Resp:	97814
Ion	Ratio	Lower	Upper
168	100		
139	33.4	29.2	43.8
169	16.1	11.0	16.6









#58
 Fluorene
 Concen: 8.858 ng
 RT: 15.50 min Scan# 2113
 Delta R.T. -0.06 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Instrument :
 BNA_G
 ClientSampleId :
 C-3

Tot Ion	Ion	Ratio	Lower	Upper
166	100			
165	99.2	79.2	118.8	
167	15.0	11.7	17.5	




Manual Integrations
 APPROVED


mohammad
 3/4/2020 2:48:28 PM

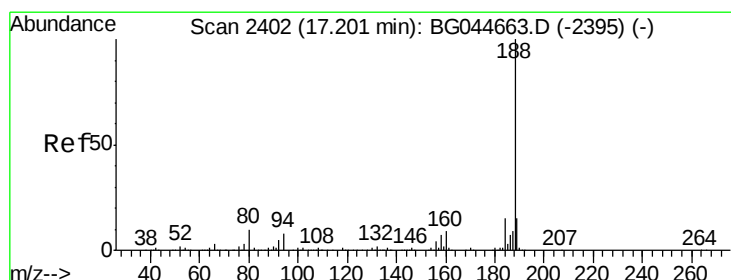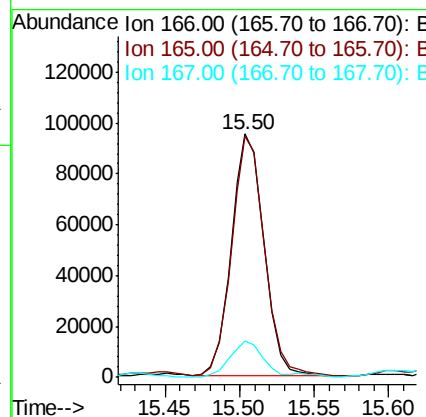

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.20 min Scan# 2402
 Delta R.T. -0.06 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Tgt Ion	Ion	Ratio	Lower	Upper
188	100			
94	8.8	6.7	10.1	
80	9.7	7.6	11.4	

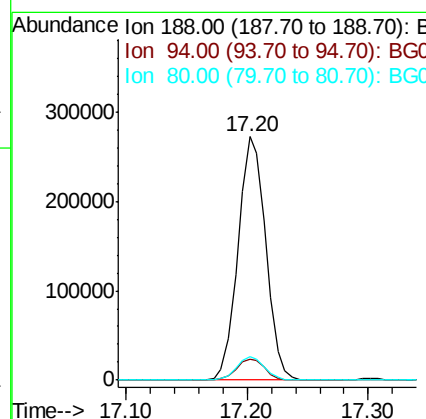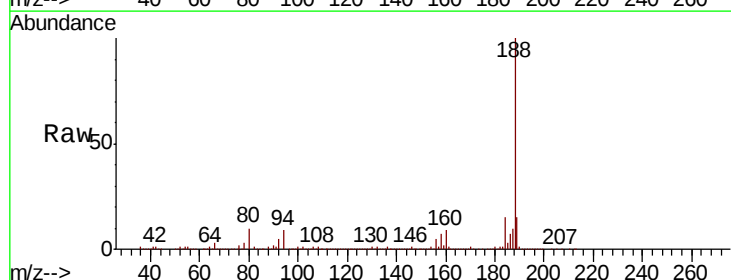

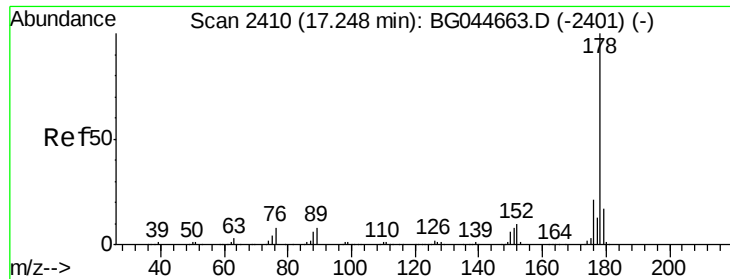





#71
Phenanthrene
Concen: 89.755 ng m
RT: 17.25 min Scan# 2410
Delta R.T. -0.05 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Instrument :
BNA_G
ClientSampleId :
C-3

Tot Ion	Ratio	Lower	Upper
178	100		
176	26.0	16.6	25.0#
179	21.0	13.3	19.9#




Manual Integrations
APPROVED


mohammad
3/4/2020 2:48:28 PM

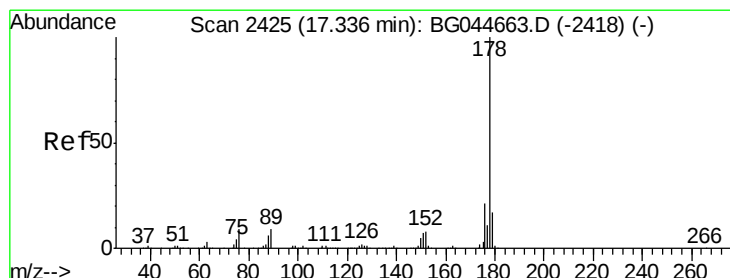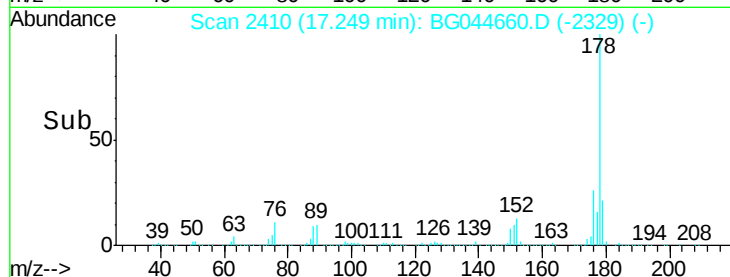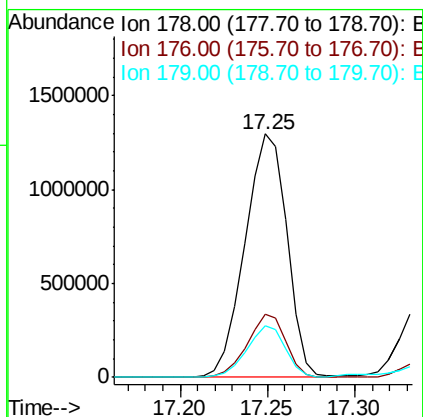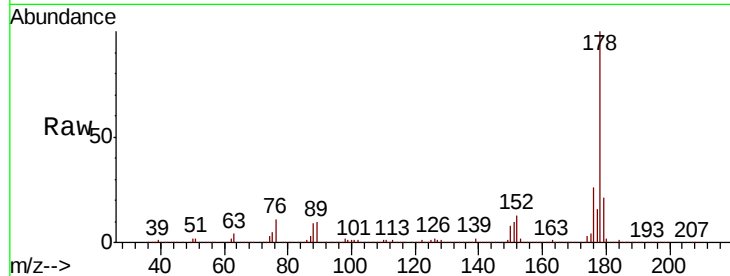

#72
Anthracene
Concen: 22.970 ng
RT: 17.34 min Scan# 2425
Delta R.T. -0.06 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
178	100		
176	20.2	15.9	23.9
179	16.3	13.1	19.7

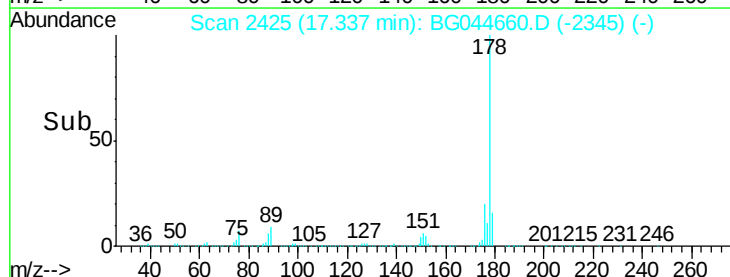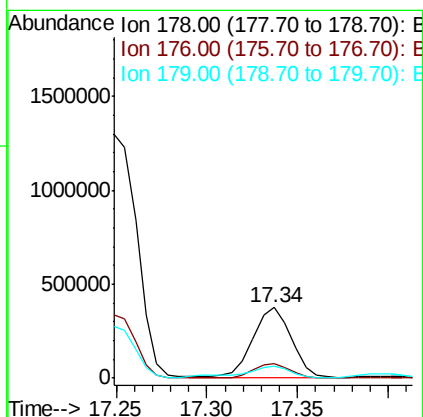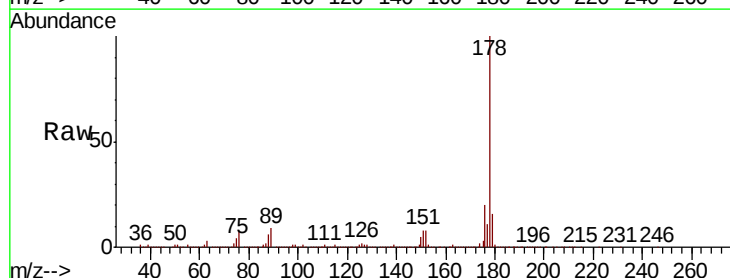







#73
 Carbazole
 Concen: 9.141 ng
 RT: 17.61 min Scan# 2471
 Delta R.T. -0.05 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Instrument :
 BNA_G
 ClientSampleId :
 C-3

Tot Ion	Ion	Ratio	Resp	Lower	Upper
167	100		198141		
166	23.4	19.7	29.5		
139	13.1	10.6	15.8		




Manual Integrations
 APPROVED


mohammad
 3/4/2020 2:48:28 PM

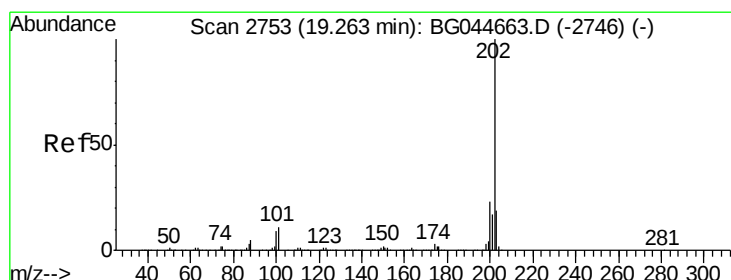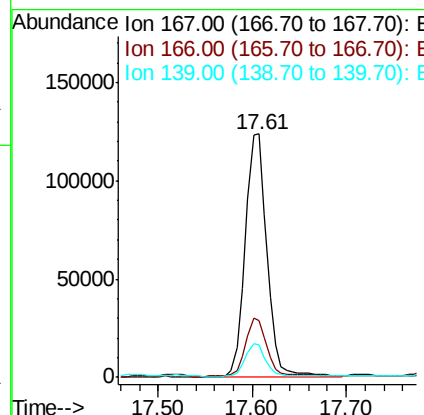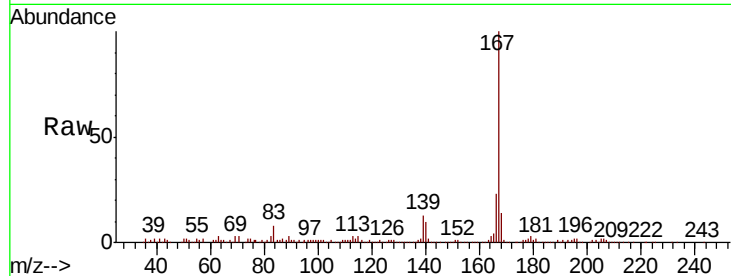

#75
 Fluoranthene
 Concen: 107.165 ng
 RT: 19.27 min Scan# 2754
 Delta R.T. -0.04 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
202	100		3065426		
101	18.0	0.0	31.0		
203	29.4	0.0	39.2		

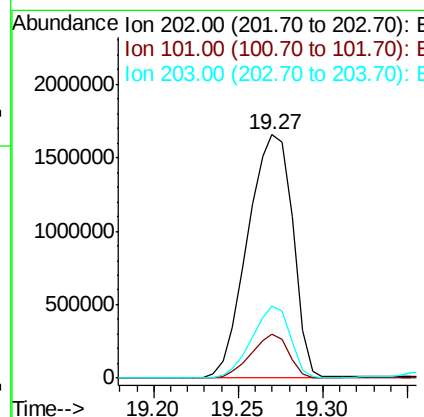







#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.45 min Scan# 3125
Delta R.T. -0.05 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Instrument :
BNA_G
ClientSampleId :
C-3

Tot Ion	Ratio	Lower	Upper
240	100		
120	10.9	8.3	12.5
236	28.2	22.3	33.5




Manual Integrations
APPROVED


mohammad
3/4/2020 2:48:28 PM

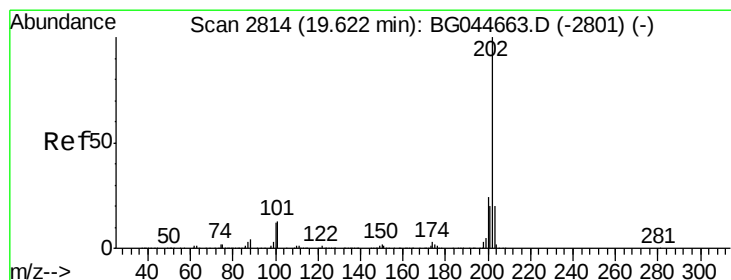

#78
Pyrene
Concen: 108.162 ng
RT: 19.63 min Scan# 2815
Delta R.T. -0.05 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
202	100		
200	32.8	18.6	28.0#
203	27.7	15.3	22.9#

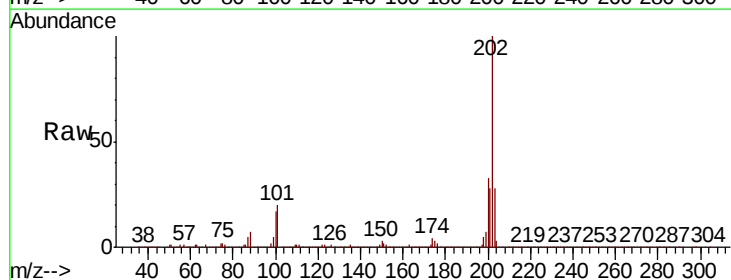







#79
 Terphenyl-d14
 Concen: 57.686 ng
 RT: 19.83 min Scan# 2849
 Delta R.T. -0.05 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Instrument :
 BNA_G
 ClientSampled :
 C-3

Tot Ion	Ratio	Lower	Upper
244	100		
212	8.0	6.5	9.7
122	10.7	8.2	12.4




Manual Integrations
 APPROVED


mohammad
 3/4/2020 2:48:28 PM

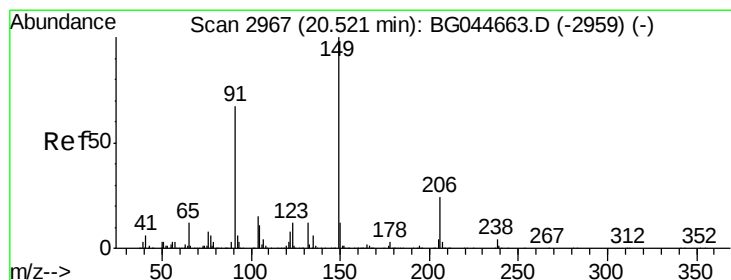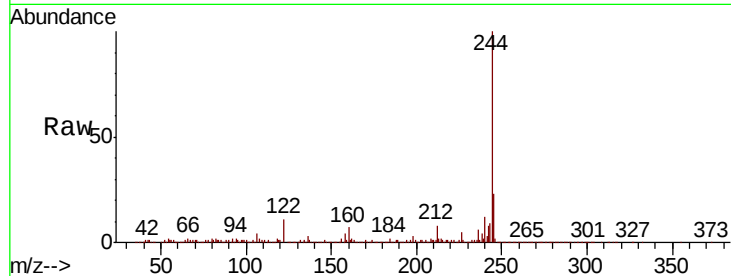

#80
 Butylbenzylphthalate
 Concen: 8.465 ng
 RT: 20.52 min Scan# 2966
 Delta R.T. -0.05 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
149	100		
91	70.0	52.7	79.1
206	21.4	18.6	28.0

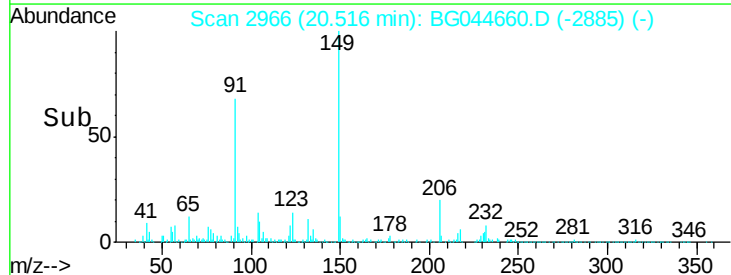



#81

Benzo(a)anthracene

Concen: 71.417 ng

RT: 21.43 min Scan# 3121

Delta R.T. -0.06 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Instrument :

BNA_G

ClientSampleId :

C-3

Tot Ion:228 Resp: 1833680

Ion Ratio Lower Upper

228 100


226 34.0 23.8 35.8

229 25.5 17.2 25.8

Manual Integrations
APPROVED

mohammad




3/4/2020 2:48:28 PM

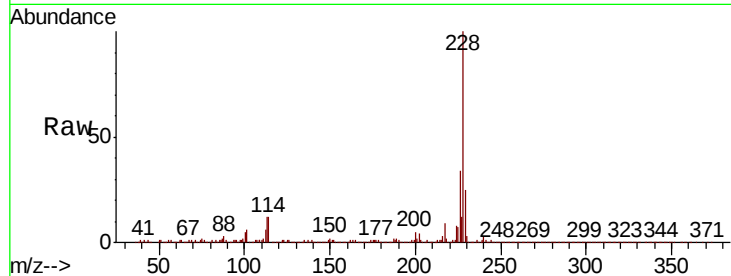

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

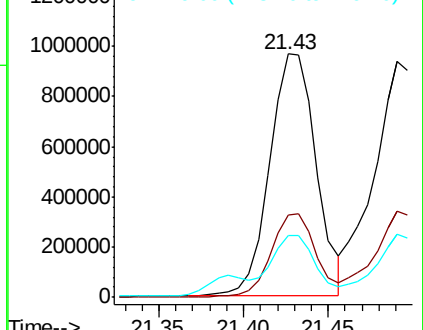

#83

Chrysene

Concen: 71.458 ng m

RT: 21.49 min Scan# 3132

Delta R.T. -0.06 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Tgt Ion:228 Resp: 1773944

Ion Ratio Lower Upper

228 100




226 36.6 26.1 39.1


229 27.0 17.2 25.8#

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

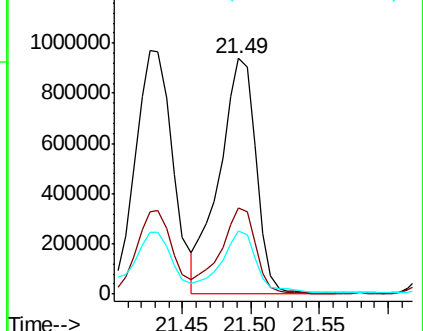

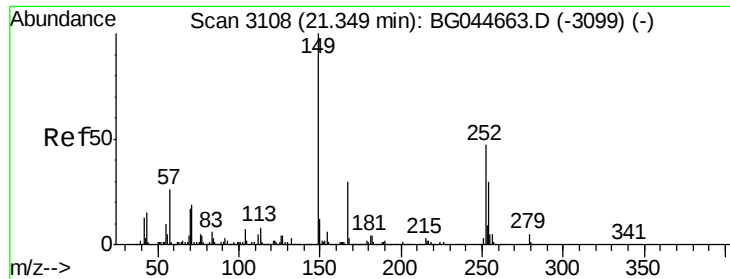





#84
 Bis(2-ethylhexyl)phthalate
 Concen: 157.197 ng
 RT: 21.36 min Scan# 3110
 Delta R.T. -0.05 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Instrument :
 BNA_G
 ClientSampleId :
 C-3

Tot Ion	Ratio	Lower	Upper
149	100		
167	40.4	23.4	35.0#
279	7.4	4.2	6.4#




Manual Integrations
 APPROVED


mohammad
 3/4/2020 2:48:28 PM

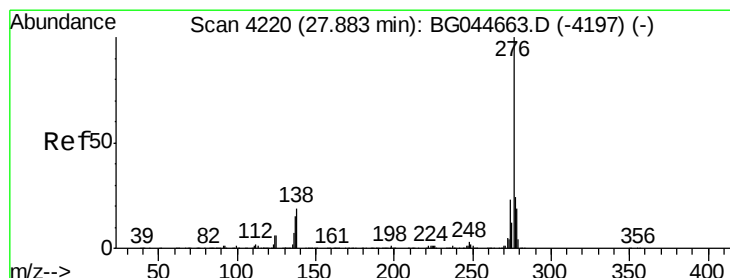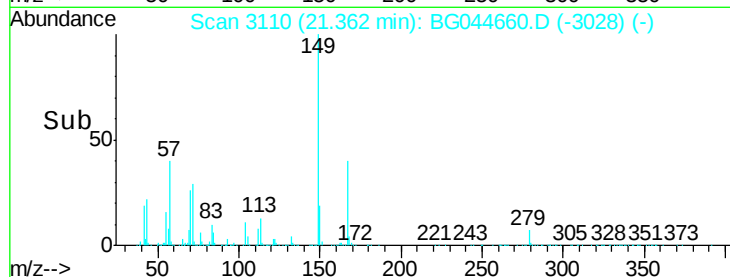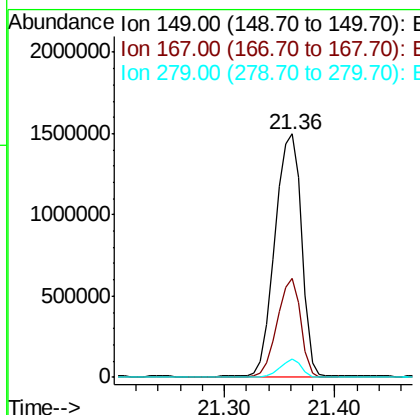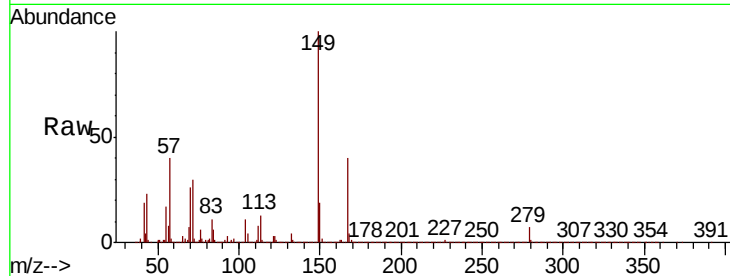

#86
 Indeno(1,2,3-cd)pyrene
 Concen: 39.116 ng
 RT: 27.91 min Scan# 4225
 Delta R.T. -0.14 min
 Lab File: BG044660.D
 Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
276	100		
138	18.7	18.2	27.4
277	24.1	20.7	31.1

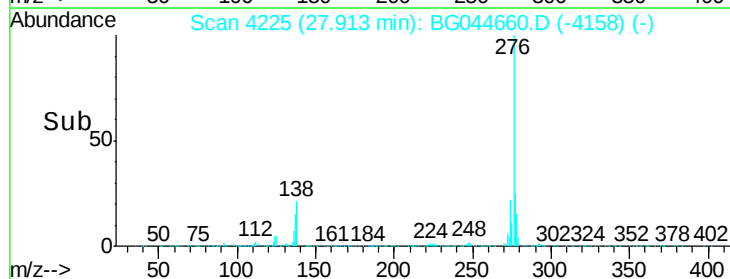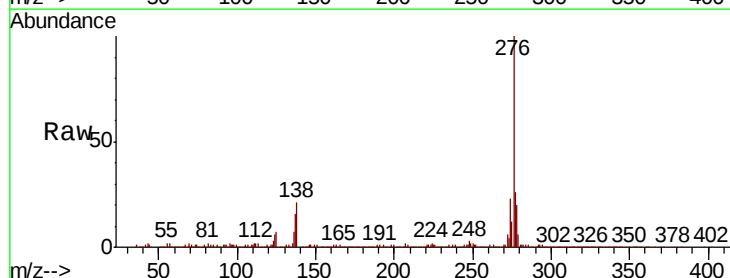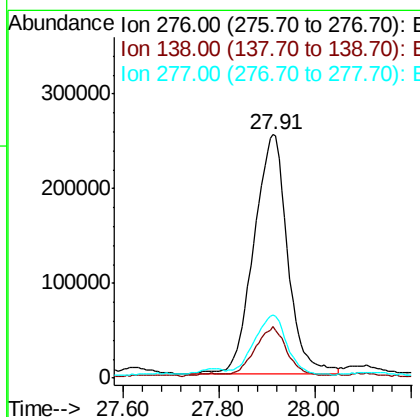

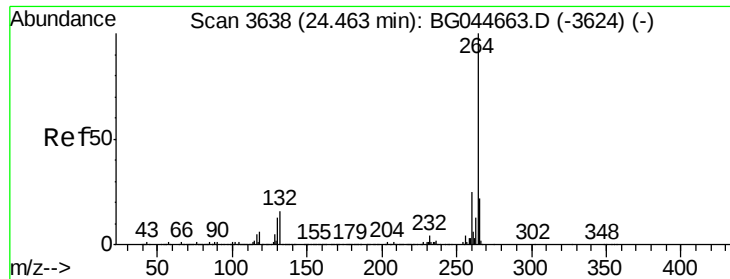





#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.48 min Scan# 3640
Delta R.T. -0.10 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Instrument :
BNA_G
ClientSampleId :
C-3

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.4	19.7	29.5
265	26.1	17.8	26.8




Manual Integrations
APPROVED


mohammad
3/4/2020 2:48:28 PM

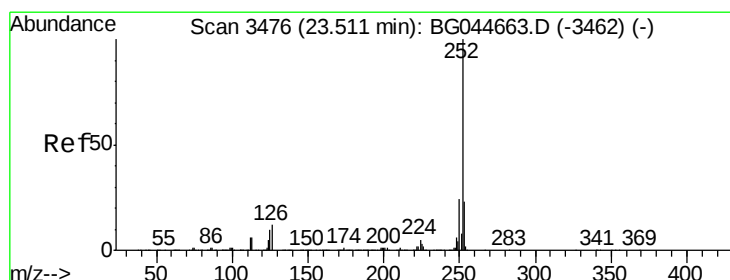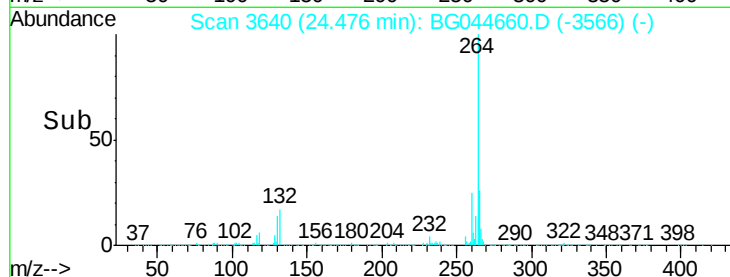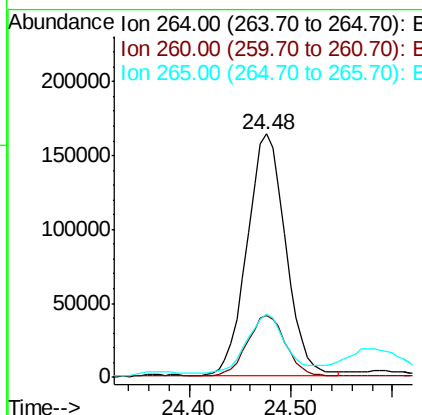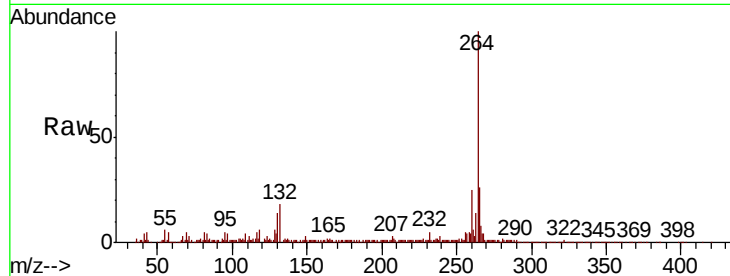

#88
Benzo(b)fluoranthene
Concen: 87.948 ng
RT: 23.54 min Scan# 3480
Delta R.T. -0.07 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
252	100		
253	26.2	18.4	27.6
125	12.2	7.9	11.9

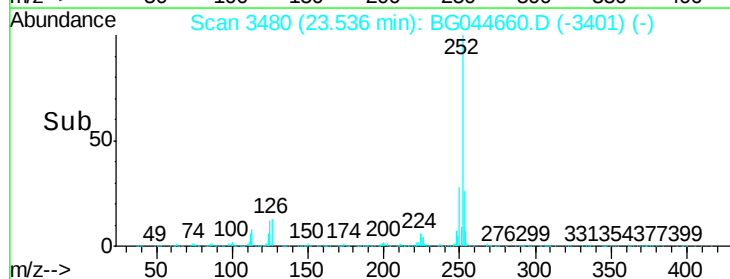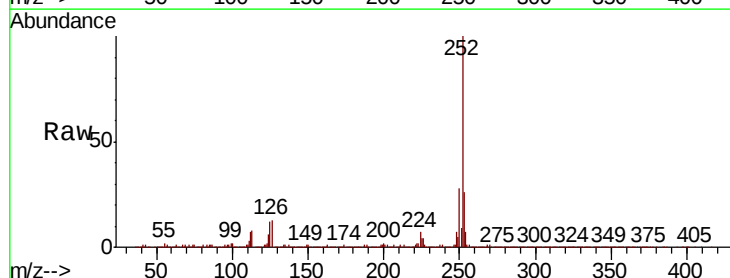



#89

Benzo(k)fluoranthene

Concen: 29.172 ng/mL

RT: 23.58 min Scan# 3488

Delta R.T. -0.08 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Instrument :

BNA_G





ClientSampled :

C-3

Tot Ion:	252	Resp:	804856
Ion Ratio	Lower	Upper	
252	100		
253	25.4	19.0	28.6
125	11.5	7.8	11.8

Manual Integrations
APPROVED

mohammad
3/4/2020 2:48:28 PM

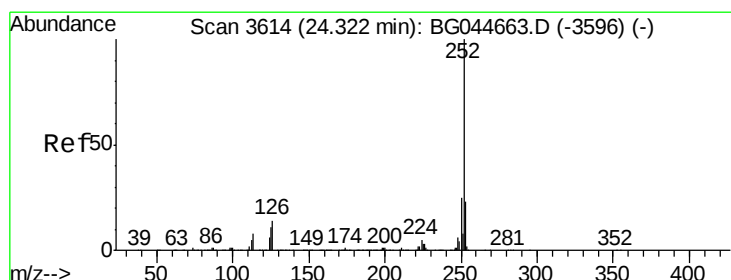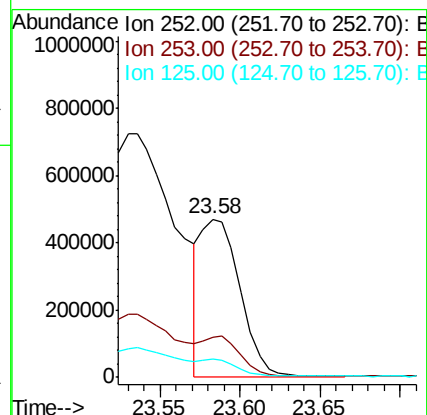

#90

Benzo(a)pyrene

Concen: 68.440 ng/mL




RT: 24.35 min Scan# 3618


Delta R.T. -0.08 min

Lab File: BG044660.D

Acq: 3 Mar 2020 10:41

Tgt Ion:	252	Resp:	1828472
Ion Ratio	Lower	Upper	
252	100		
253	26.2	19.0	28.4
125	11.7	8.5	12.7

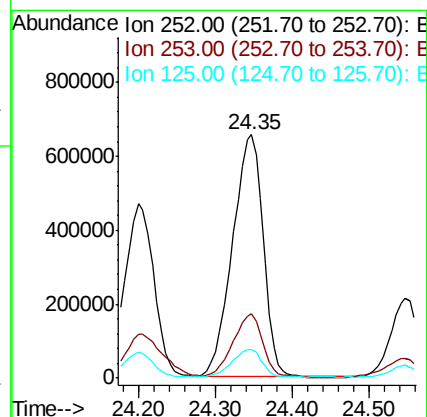

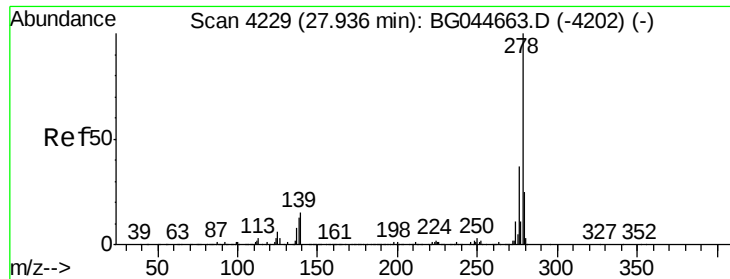


#91
Dibenzo(a,h)anthracene
Concen: 11.087 ng
RT: 27.94 min Scan# 4230
Delta R.T. -0.17 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Instrument :
BNA_G
ClientSampleId :
C-3

Tot Ion	Ratio	Lower	Upper
278	100		
139	17.1	11.7	17.5
279	27.7	19.8	29.6

Manual Integrations
APPROVED

mohammad
3/4/2020 2:48:28 PM



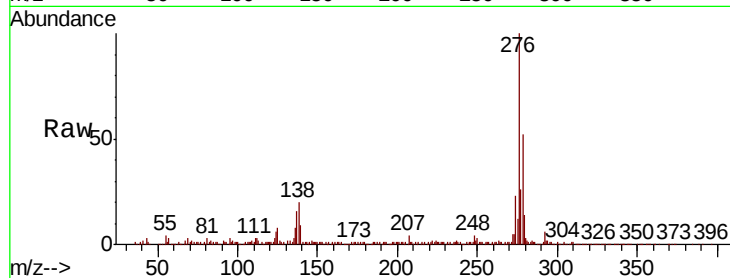


Abundance

Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

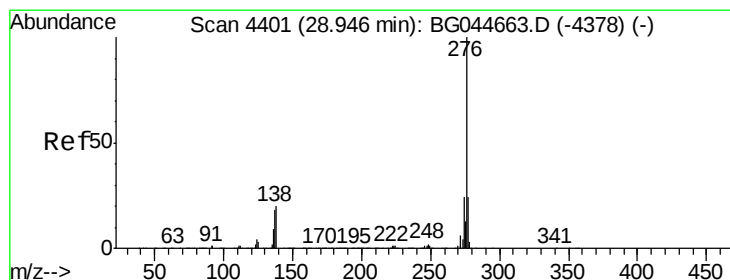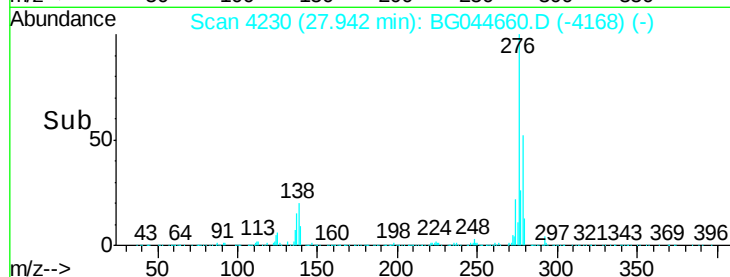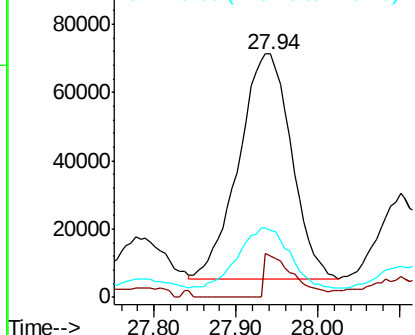

#92
Benzo(g,h,i)perylene
Concen: 44.613 ng
RT: 28.98 min Scan# 4406
Delta R.T. -0.15 min
Lab File: BG044660.D
Acq: 3 Mar 2020 10:41

Tgt Ion	Ratio	Lower	Upper
276	100		
277	24.5	19.5	29.3
138	21.2	16.1	24.1

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

