


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030220\
 Data File : BG044632.D
 Acq On : 2 Mar 2020 13:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 24 16:11:23 2020

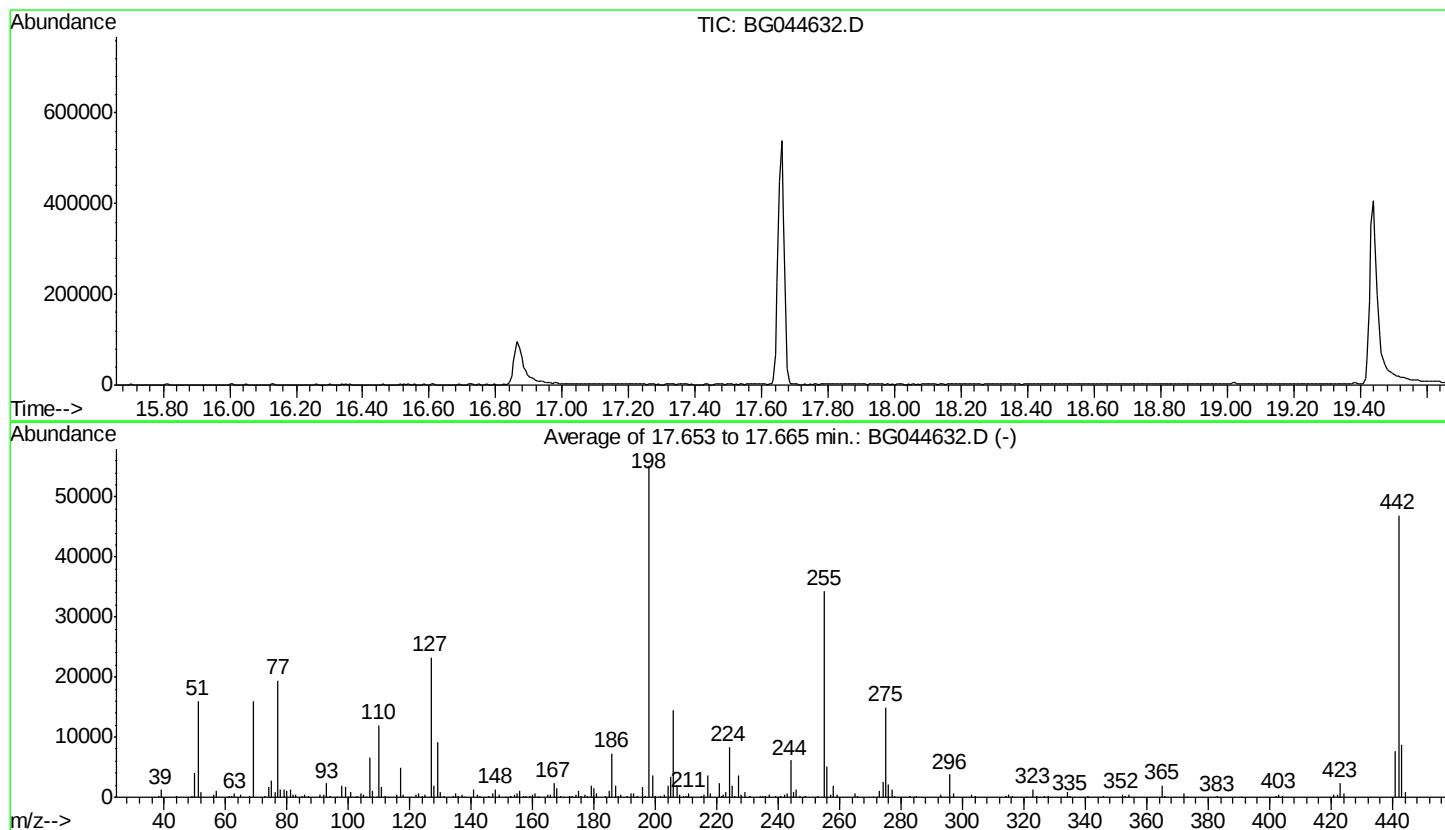

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	16069	PASS
68	69	0.00	2	0.9	143	PASS
69	198	0.00	100	29.0	16004	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	23333	PASS
197	198	0.00	2	0.5	271	PASS
198	198	100	100	100.0	55200	PASS
199	198	5	9	6.7	3721	PASS
275	198	10	60	27.1	14934	PASS
365	198	1	100	3.5	1950	PASS
441	198	0.01	100	13.8	7626	PASS
442	198	50	100	85.1	46981	PASS
443	442	15	24	18.8	8835	PASS