


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030220\
 Data File : BG044648.D
 Acq On : 3 Mar 2020 1:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 24 16:11:23 2020

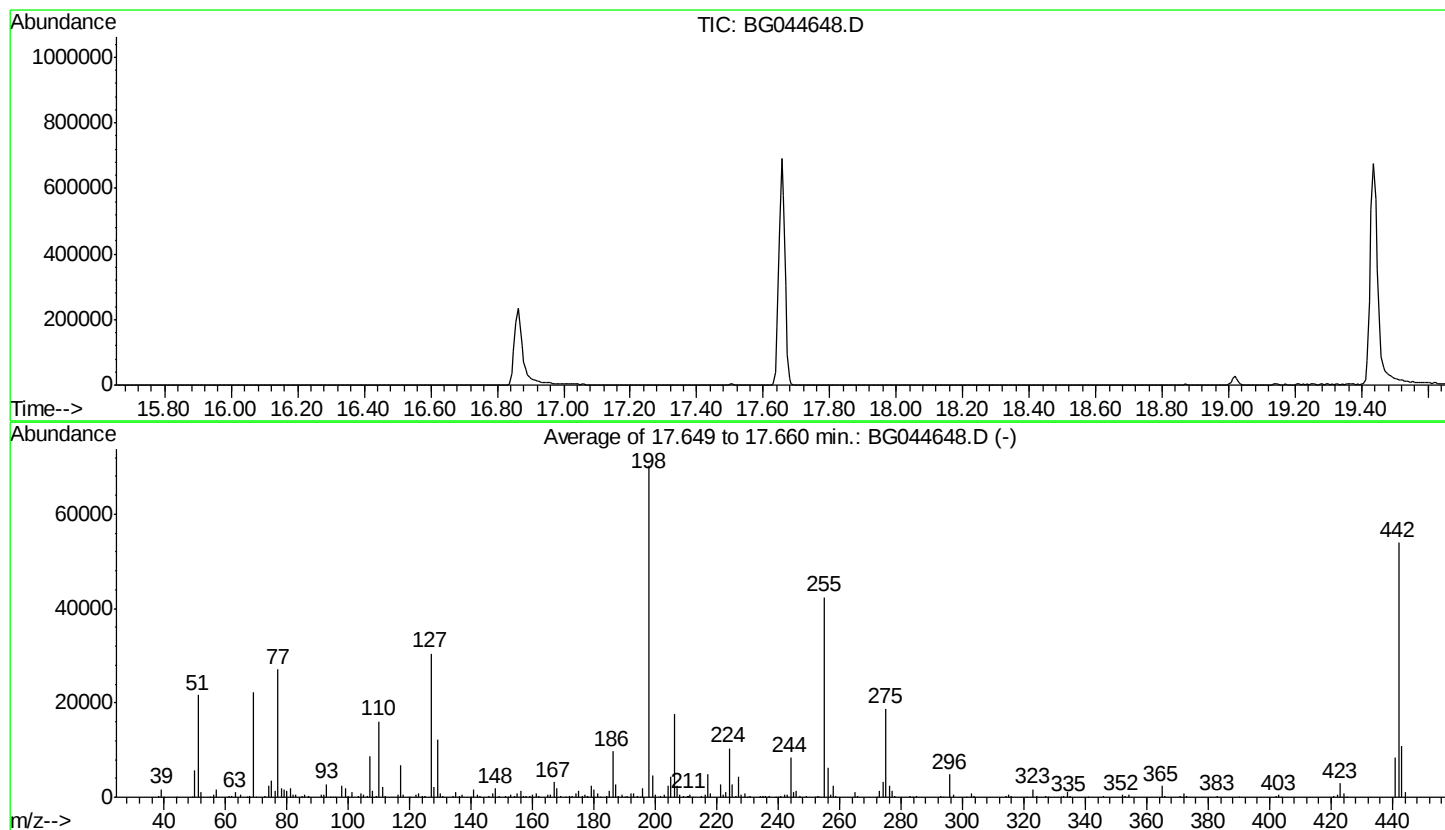

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	21701	PASS
68	69	0.00	2	0.7	162	PASS
69	198	0.00	100	31.6	22229	PASS
70	69	0.00	2	0.2	50	PASS
127	198	10	80	43.3	30461	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70296	PASS
199	198	5	9	6.6	4670	PASS
275	198	10	60	26.8	18836	PASS
365	198	1	100	3.3	2318	PASS
441	198	0.01	100	12.1	8487	PASS
442	198	50	100	76.7	53904	PASS
443	442	15	24	19.9	10748	PASS