

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG030223\  
 Data File : BG056792.D  
 Acq On : 2 Mar 2023 16:03  
 Operator : CG/JU  
 Sample : PB151151BL  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 SBLK151

Quant Time: Mar 03 00:59:28 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG022323.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Mar 02 00:12:28 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min)    |
|-------------------------------|--------|------|----------|--------|--------|-------------|
| -----                         |        |      |          |        |        |             |
| Internal Standards            |        |      |          |        |        |             |
| 1) 1,4-Dichlorobenzene-d4     | 8.420  | 152  | 12335    | 20.000 | ng/ul  | 0.00        |
| 20) Naphthalene-d8            | 11.258 | 136  | 52581    | 20.000 | ng/ul  | 0.00        |
| 38) Acenaphthene-d10          | 15.024 | 164  | 45557    | 20.000 | ng/ul  | 0.00        |
| 64) Phenanthrene-d10          | 17.756 | 188  | 120882   | 20.000 | ng/ul  | 0.00        |
| 79) Chrysene-d12              | 22.063 | 240  | 119656   | 20.000 | ng/ul  | 0.00        |
| 88) Perylene-d12              | 25.588 | 264  | 126738   | 20.000 | ng/ul  | 0.00        |
| System Monitoring Compounds   |        |      |          |        |        |             |
| 3) 1,4-Dioxane-d8             | 3.702  | 96   | 2458     | 11.054 | ng/uL  | 0.00        |
| 4) Pyridine-d5                | 4.137  | 84   | 34587    | 38.535 | ng/ul  | 0.00        |
| 7) Phenol-d5                  | 7.539  | 99   | 40457    | 32.776 | ng/ul  | 0.00        |
| 9) Bis-(2-Chloroethyl)eth...  | 7.721  | 67   | 26785    | 35.574 | ng/ul  | 0.00        |
| 11) 2-Chlorophenol-d4         | 7.939  | 132  | 27260    | 33.256 | ng/ul  | 0.00        |
| 15) 4-Methylphenol-d8         | 9.108  | 113  | 30585    | 32.428 | ng/ul  | 0.00        |
| 21) Nitrobenzene-d5           | 9.595  | 128  | 15674    | 35.570 | ng/ul  | 0.00        |
| 24) 2-Nitrophenol-d4          | 10.324 | 143  | 17885    | 34.097 | ng/ul  | 0.00        |
| 28) 2,4-Dichlorophenol-d3     | 10.859 | 165  | 34017    | 34.425 | ng/ul  | 0.00        |
| 31) 4-Chloroaniline-d4        | 11.376 | 131  | 44883    | 34.824 | ng/ul  | 0.00        |
| 46) Dimethylphthalate-d6      | 14.407 | 166  | 127345   | 34.646 | ng/ul  | 0.00        |
| 49) Acenaphthylene-d8         | 14.719 | 160  | 143106   | 34.256 | ng/ul  | 0.00        |
| 54) 4-Nitrophenol-d4          | 15.177 | 143  | 20187    | 31.855 | ng/ul  | 0.00        |
| 60) Fluorene-d10              | 16.006 | 176  | 117548   | 34.572 | ng/ul  | 0.00        |
| 65) 4,6-Dinitro-2-methylph... | 16.105 | 200  | 23909    | 29.563 | ng/ul  | 0.00        |
| 73) Anthracene-d10            | 17.856 | 188  | 202402   | 34.514 | ng/ul  | 0.00        |
| 81) Pyrene-d10                | 20.113 | 212  | 246823   | 30.484 | ng/ul  | 0.00        |
| 92) Benzo(a)pyrene-d12        | 25.348 | 264  | 236646   | 34.593 | ng/ul  | 0.00        |
| Target Compounds              |        |      |          |        |        |             |
| 17) N-Nitroso-di-n-propyla... | 9.108  | 70   | 996      | 1.075  | ng/ul# | Qvalue<br>1 |
| -----                         |        |      |          |        |        |             |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG030223\  
Data File : BG056792.D  
Acq On : 2 Mar 2023 16:03  
Operator : CG/JU  
Sample : PB151151BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
SBLK151


Quant Time: Mar 03 00:59:28 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG022323.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Mar 02 00:12:28 2023  
Response via : Initial Calibration

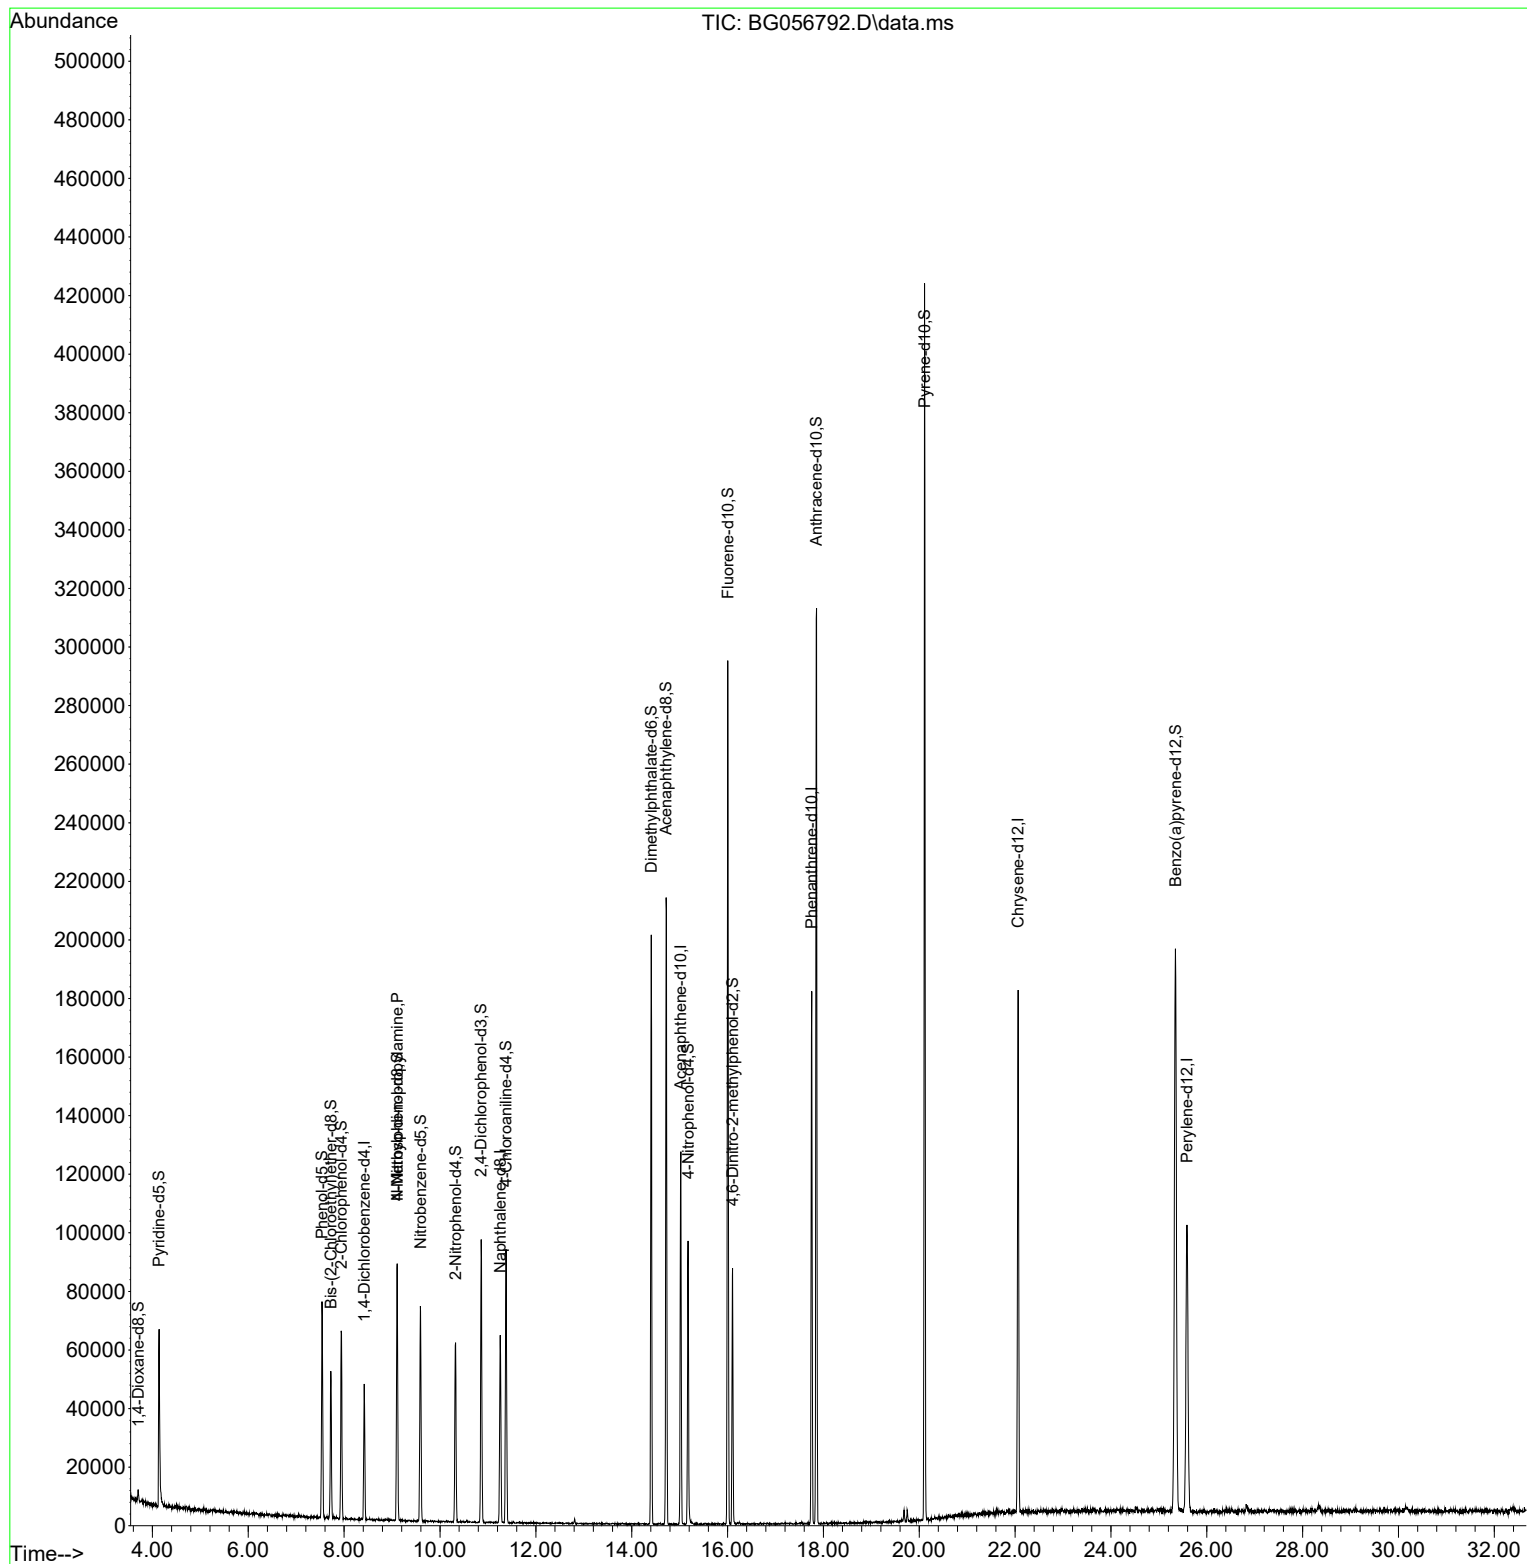

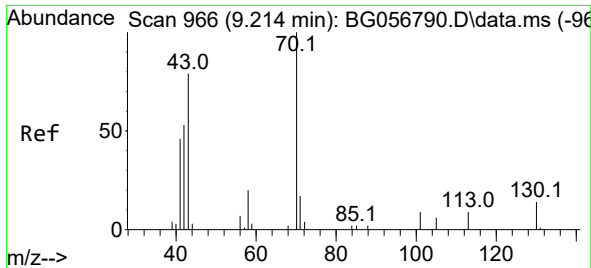

#17  
 N-Nitroso-di-n-propylamine  
 Concen: 1.075 ng/ul  
 RT: 9.108 min Scan# 94  
 Delta R.T. -0.108 min  
 Lab File: BG056792.D  
 Acq: 2 Mar 2023 16:03

Instrument :  
 BNA\_G  
 ClientSampleId :  
 SBLK151

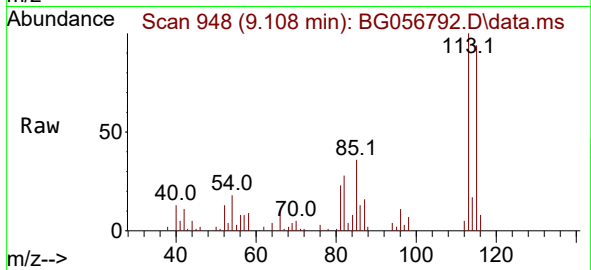

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 70    | Resp: | 996   |
| Ion      | Ratio | Lower | Upper |
| 70       | 100   |       |       |
| 42       | 220.1 | 46.6  | 70.0# |
| 101      | 0.0   | 7.3   | 10.9# |
| 130      | 0.0   | 13.7  | 20.5# |

