

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
 Data File : BG056797.D
 Acq On : 2 Mar 2023 19:31
 Operator : CG/JU
 Sample : 01710-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBAB0

Quant Time: Mar 03 01:00:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.418	152	14651	20.000	ng/ul	0.00
20) Naphthalene-d8	11.256	136	62230	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.022	164	51816	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.754	188	130927	20.000	ng/ul	0.00
79) Chrysene-d12	22.061	240	124200	20.000	ng/ul	0.00
88) Perylene-d12	25.586	264	135137	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.700	96	928	3.514	ng/uL	0.00
4) Pyridine-d5	4.146	84	645	0.605	ng/ul	0.01
7) Phenol-d5	7.542	99	22596	15.412	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.719	67	14593	16.318	ng/ul	0.00
11) 2-Chlorophenol-d4	7.942	132	15429	15.847	ng/ul	0.00
15) 4-Methylphenol-d8	9.099	113	17476	15.600	ng/ul	0.00
21) Nitrobenzene-d5	9.593	128	8461	16.224	ng/ul	0.00
24) 2-Nitrophenol-d4	10.321	143	10458	16.847	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.862	165	20096	17.184	ng/ul	0.00
31) 4-Chloroaniline-d4	11.379	131	14849	9.735	ng/ul	0.00
46) Dimethylphthalate-d6	14.405	166	73095	17.484	ng/ul	0.00
49) Acenaphthylene-d8	14.722	160	81832	17.222	ng/ul	0.00
54) 4-Nitrophenol-d4	15.169	143	10471	14.527	ng/ul	-0.01
60) Fluorene-d10	16.003	176	68381	17.682	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.097	200	13653	15.586	ng/ul	0.00
73) Anthracene-d10	17.854	188	108088	17.017	ng/ul	0.00
81) Pyrene-d10	20.110	212	132442	15.759	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.339	264	125010	17.138	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	9.246	105	3278	1.709	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
Data File : BG056797.D
Acq On : 2 Mar 2023 19:31
Operator : CG/JU
Sample : 01710-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAB0

Quant Time: Mar 03 01:00:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

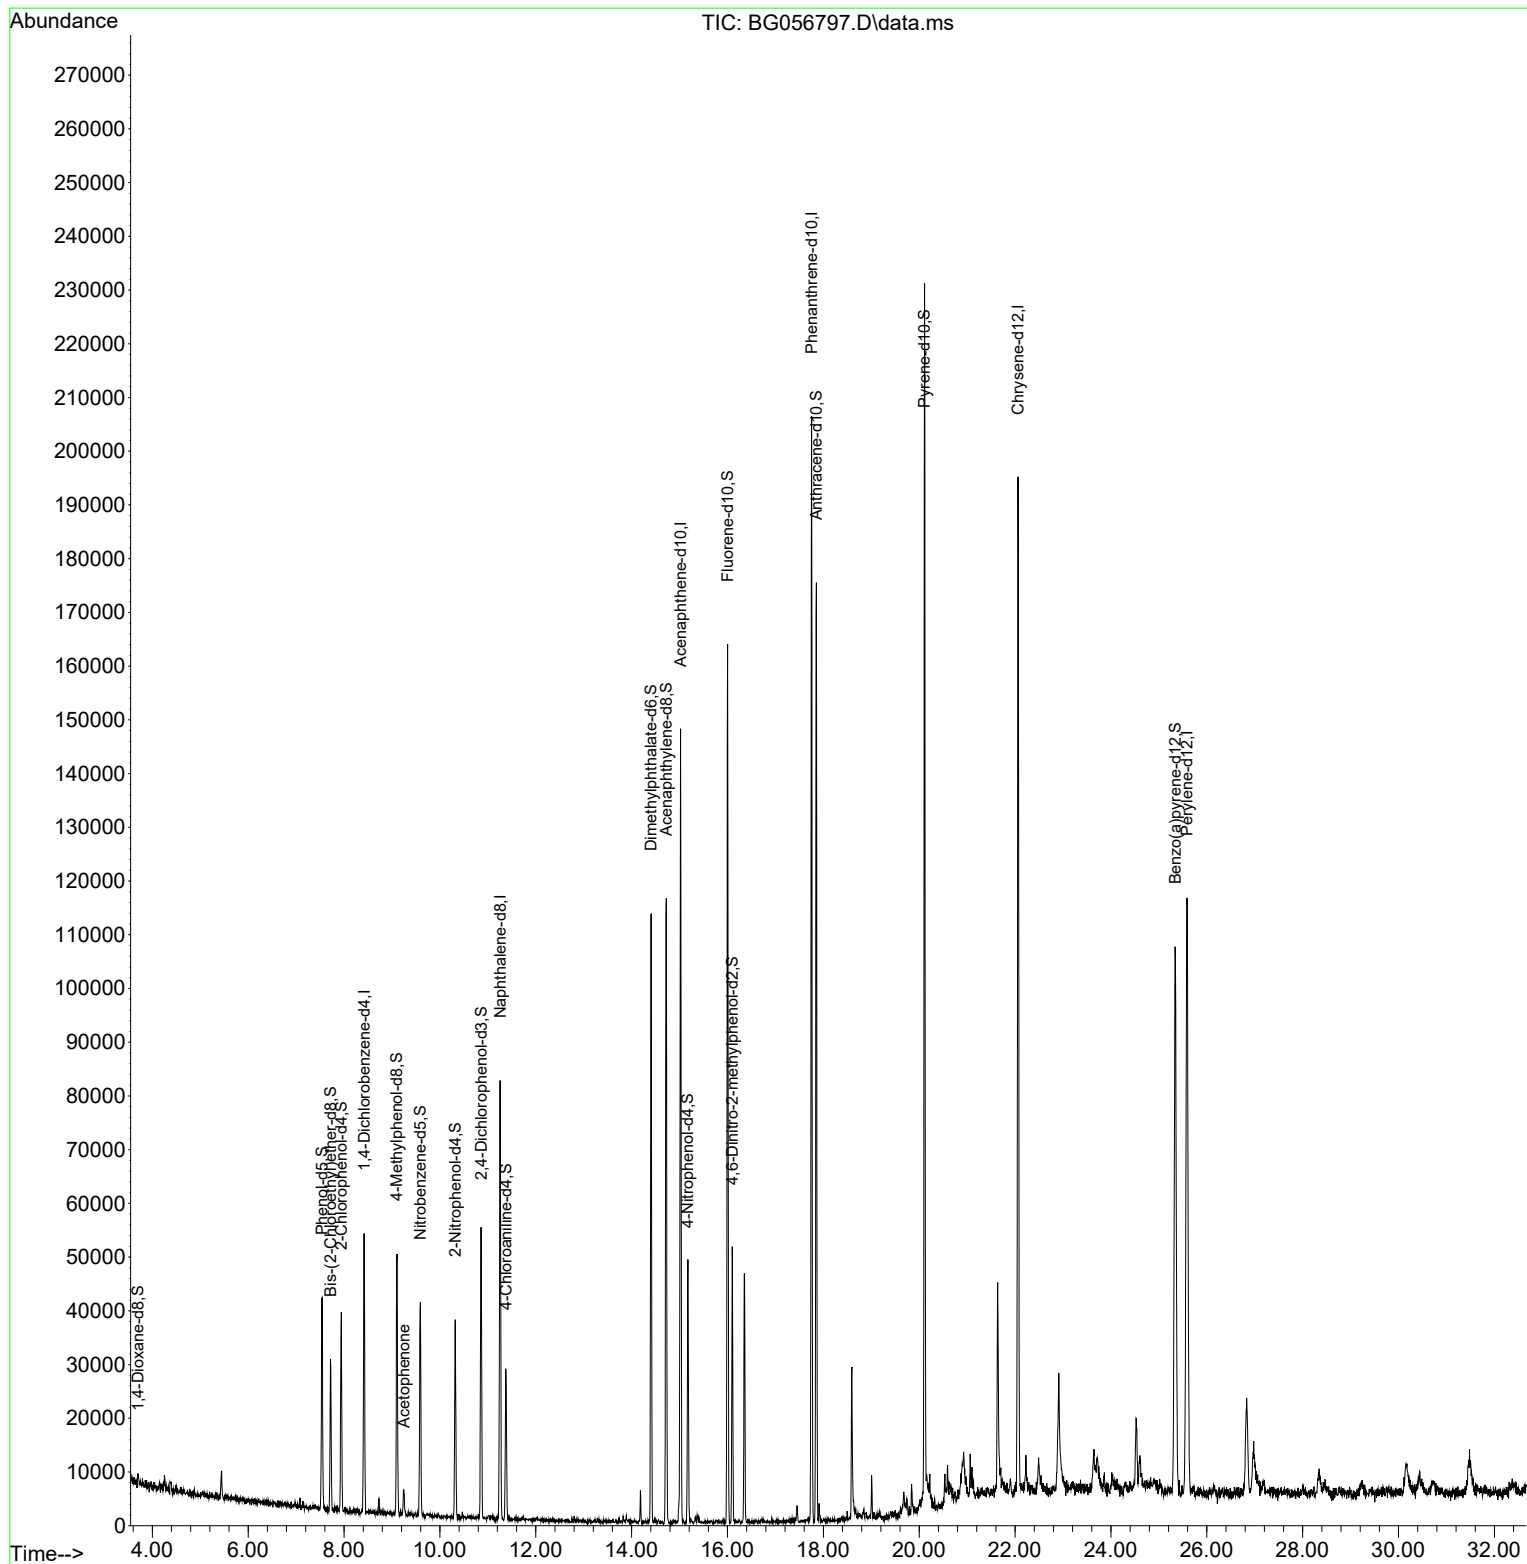

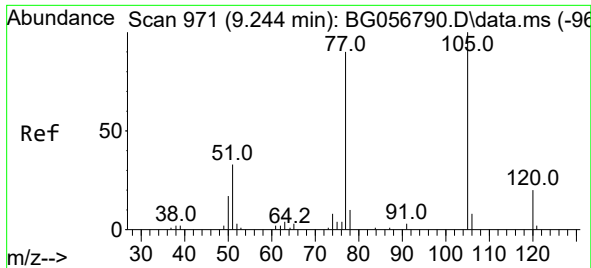

#16
 Acetophenone
 Concen: 1.709 ng/ul
 RT: 9.246 min Scan# 91
 Delta R.T. 0.007 min
 Lab File: BG056797.D
 Acq: 2 Mar 2023 19:31

Instrument :
 BNA_G
 ClientSampleId :
 DBAB0

Tgt Ion:105 Resp: 3278
 Ion Ratio Lower Upper
 105 100
 77 68.5 71.4 107.0#
 51 32.2 23.6 35.4

