

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
 Data File : BG056799.D
 Acq On : 2 Mar 2023 20:53
 Operator : CG/JU
 Sample : 01710-13MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBAB2

Quant Time: Mar 03 01:00:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.418	152	16665	20.000	ng/ul	# 0.00
20) Naphthalene-d8	11.256	136	70587	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.022	164	57975	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.754	188	137782	20.000	ng/ul	0.00
79) Chrysene-d12	22.061	240	129812	20.000	ng/ul	0.00
88) Perylene-d12	25.580	264	139778	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.694	96	1779	5.922	ng/uL	0.00
4) Pyridine-d5	4.147	84	3797	3.131	ng/ul	0.01
7) Phenol-d5	7.537	99	37101	22.247	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.719	67	23650	23.249	ng/ul	0.00
11) 2-Chlorophenol-d4	7.942	132	25424	22.957	ng/ul	0.00
15) 4-Methylphenol-d8	9.105	113	28781	22.587	ng/ul	0.00
21) Nitrobenzene-d5	9.587	128	14000	23.667	ng/ul	0.00
24) 2-Nitrophenol-d4	10.322	143	17533	24.900	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.856	165	32921	24.817	ng/ul	0.00
31) 4-Chloroaniline-d4	11.379	131	22528	13.021	ng/ul	0.00
46) Dimethylphthalate-d6	14.405	166	115347	24.660	ng/ul	0.00
49) Acenaphthylene-d8	14.717	160	129141	24.292	ng/ul	0.00
54) 4-Nitrophenol-d4	15.175	143	15093	18.715	ng/ul	0.00
60) Fluorene-d10	16.003	176	105540	24.392	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.103	200	22420	24.322	ng/ul	0.00
73) Anthracene-d10	17.854	188	165976	24.831	ng/ul	0.00
81) Pyrene-d10	20.110	212	196635	22.385	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.339	264	189634	25.135	ng/ul	-0.01
Target Compounds						
					Qvalue	
13) 2-Methylphenol	8.724	108	5072	3.953	ng/ul#	13
16) Acetophenone	9.246	105	2814	1.290	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
Data File : BG056799.D
Acq On : 2 Mar 2023 20:53
Operator : CG/JU
Sample : 01710-13MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAB2

Quant Time: Mar 03 01:00:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration




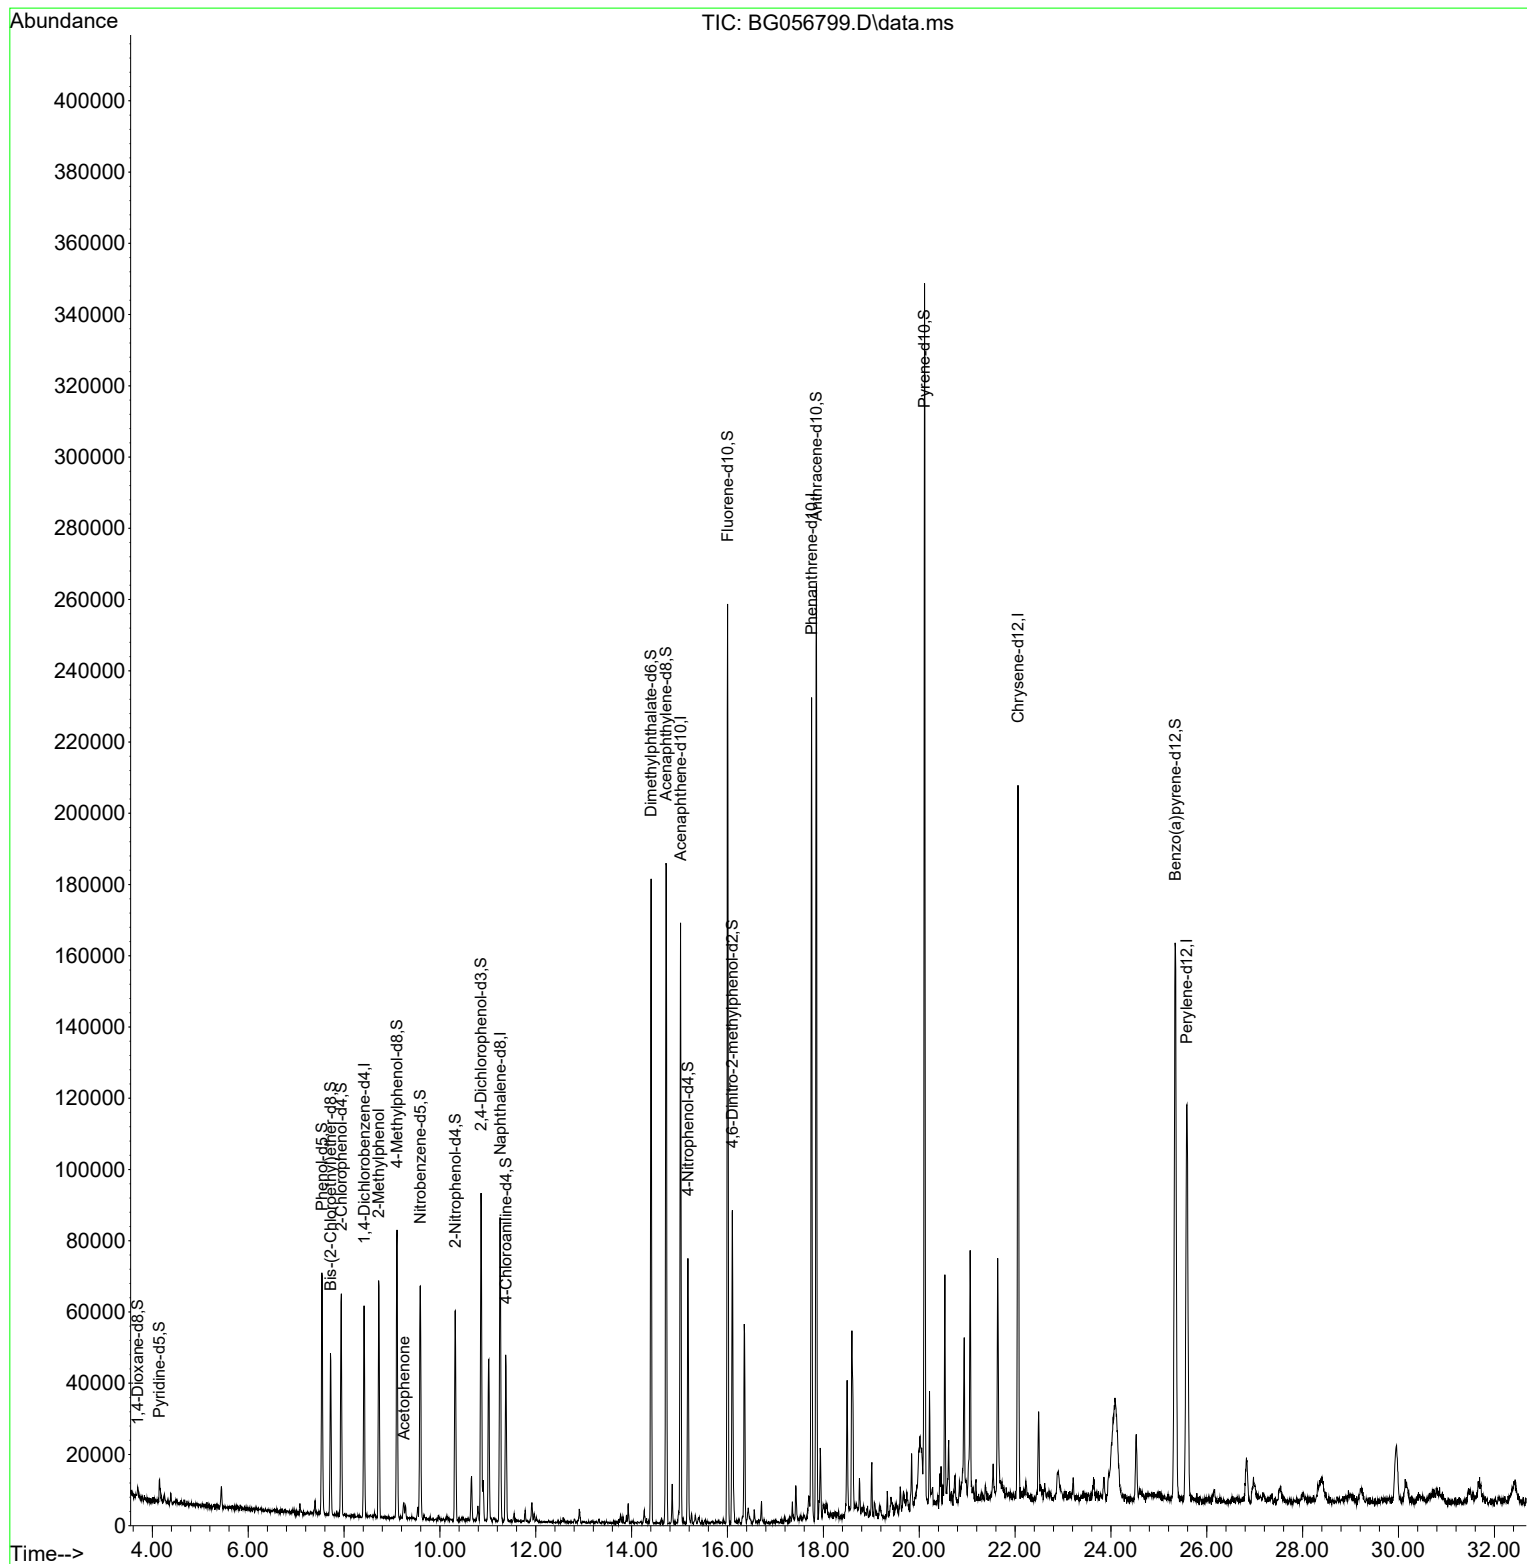


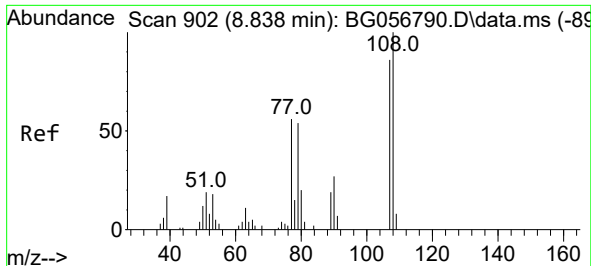

#13
2-Methylphenol
Concen: 3.953 ng/ul
RT: 8.724 min Scan# 811
Delta R.T. -0.117 min
Lab File: BG056799.D
Acq: 2 Mar 2023 20:53

Instrument :
BNA_G
ClientSampleId :
DBAB2

Tgt Ion:108 Resp: 5072
Ion Ratio Lower Upper
108 100
107 9.0 73.4 110.0#

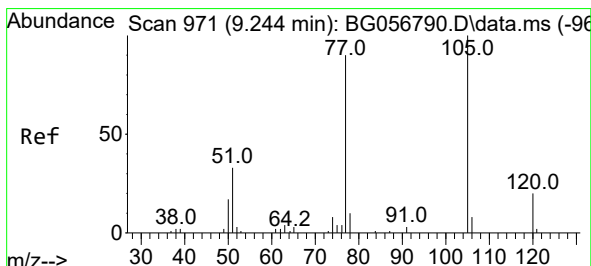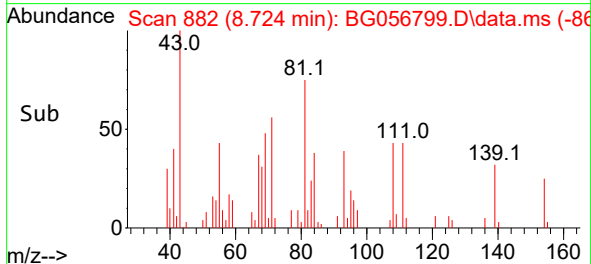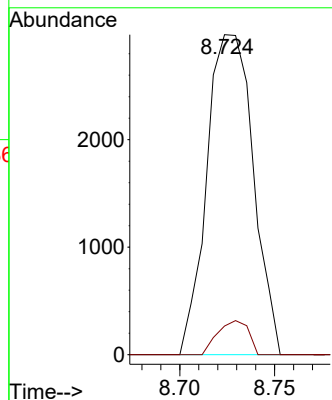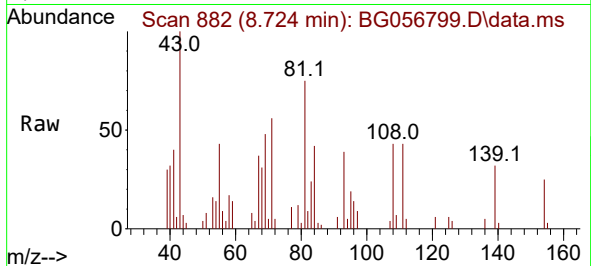

#16
Acetophenone
Concen: 1.290 ng/ul
RT: 9.246 min Scan# 971
Delta R.T. 0.007 min
Lab File: BG056799.D
Acq: 2 Mar 2023 20:53

Tgt Ion:105 Resp: 2814
Ion Ratio Lower Upper
105 100
77 83.3 71.4 107.0
51 36.3 23.6 35.4#

