

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
 Data File : BG056791.D
 Acq On : 2 Mar 2023 15:22
 Operator : CG/JU
 Sample : PB151126BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.134	98	101	116	rVB	49001	81063	16.73%	1.697%
2	5.726	370	372	374	rVB	1525	842	0.17%	0.018%
3	5.744	374	375	377	rBV	1391	666	0.14%	0.014%
4	6.085	431	433	434	rBV	1266	1092	0.23%	0.023%
5	7.042	595	596	598	rBV2	1193	890	0.18%	0.019%
6	7.283	635	637	639	rBV	1022	744	0.15%	0.016%
7	7.542	675	681	688	rBV	60745	102247	21.10%	2.140%
8	7.718	706	711	719	rVB	41685	69145	14.27%	1.447%
9	7.941	742	749	755	rBV	55932	94341	19.47%	1.975%
10	8.165	786	787	789	rBV	754	701	0.14%	0.015%
11	8.417	824	830	838	rVB	50736	81508	16.82%	1.706%
12	8.688	874	876	878	rBV2	971	807	0.17%	0.017%
13	8.975	923	925	928	rBV	835	689	0.14%	0.014%
14	9.064	936	940	941	rBV2	826	1057	0.22%	0.022%
15	9.105	941	947	954	rVB2	75739	126450	26.09%	2.647%
16	9.369	990	992	995	rBV2	1031	773	0.16%	0.016%
17	9.410	998	999	1003	rVB2	877	668	0.14%	0.014%
18	9.498	1013	1014	1017	rBV	669	767	0.16%	0.016%
19	9.592	1023	1030	1037	rVB	62495	110593	22.82%	2.315%
20	9.921	1085	1086	1090	rBV	653	791	0.16%	0.017%
21	10.010	1097	1101	1104	rBV2	696	925	0.19%	0.019%
22	10.321	1147	1154	1160	rVB	53588	91762	18.93%	1.921%
23	10.856	1236	1245	1253	rBV2	76852	137311	28.33%	2.874%
24	11.255	1305	1313	1321	rBV	72907	128776	26.57%	2.696%
25	11.379	1327	1334	1344	rVB	76201	135445	27.95%	2.835%
26	12.689	1554	1557	1561	rBV2	427	669	0.14%	0.014%
27	12.806	1573	1577	1582	rVB2	1533	1956	0.40%	0.041%
28	13.182	1636	1641	1644	rBV2	544	740	0.15%	0.015%
29	13.881	1759	1760	1764	rVB2	868	1074	0.22%	0.022%
30	14.404	1843	1849	1856	rBV	161405	235961	48.69%	4.939%
31	14.722	1895	1903	1910	rBV	174120	276366	57.03%	5.785%
32	15.021	1947	1954	1962	rVB	139854	215911	44.55%	4.520%
33	15.174	1974	1980	1988	rBV	76770	118452	24.44%	2.480%
34	16.003	2115	2121	2132	rVB	235004	353242	72.89%	7.394%
35	16.102	2132	2138	2147	rBV2	69656	104953	21.66%	2.197%
36	16.238	2159	2161	2164	rVB	595	675	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
 Data File : BG056791.D
 Acq On : 2 Mar 2023 15:22
 Operator : CG/JU
 Sample : PB151126BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	17.753	2413	2419	2428	rVB	188474	282545	58.30%	5.915%
38	17.853	2428	2436	2442	rBV	273602	398598	82.25%	8.344%
39	18.106	2476	2479	2482	rBV	589	721	0.15%	0.015%
40	18.400	2526	2529	2534	rVB	432	673	0.14%	0.014%
41	18.588	2557	2561	2562	rBV	582	682	0.14%	0.014%
42	19.070	2639	2643	2644	rBV	749	726	0.15%	0.015%
43	19.410	2698	2701	2705	rBV	578	771	0.16%	0.016%
44	19.681	2743	2747	2752	rVB4	3149	4343	0.90%	0.091%
45	19.751	2754	2759	2762	rBV3	2889	4046	0.83%	0.085%
46	19.851	2774	2776	2778	rVB	922	770	0.16%	0.016%
47	20.109	2814	2820	2829	rBV	343357	484633	100.00%	10.145%
48	20.327	2855	2857	2858	rBV2	936	671	0.14%	0.014%
49	20.356	2860	2862	2865	rBV2	1289	1261	0.26%	0.026%
50	20.521	2884	2890	2892	rBV3	1187	2433	0.50%	0.051%
51	20.544	2892	2894	2897	rVB2	853	870	0.18%	0.018%
52	21.097	2986	2988	2990	rBV2	1412	1449	0.30%	0.030%
53	22.060	3145	3152	3161	rVB2	181371	316095	65.22%	6.617%
54	23.476	3392	3393	3395	rBV2	1953	1557	0.32%	0.033%
55	23.635	3419	3420	3425	rBV4	2496	3584	0.74%	0.075%
56	24.399	3548	3550	3553	rVB2	1728	1196	0.25%	0.025%
57	24.769	3611	3613	3615	rBV2	1874	1464	0.30%	0.031%
58	25.345	3698	3711	3723	rBV	164200	472767	97.55%	9.896%
59	25.585	3741	3752	3767	rBV2	99462	304911	62.92%	6.383%
60	27.090	4007	4008	4009	rBV	1981	793	0.16%	0.017%
61	27.231	4030	4032	4033	rBV2	1903	951	0.20%	0.020%
62	27.372	4054	4056	4058	rBV3	1973	1667	0.34%	0.035%
63	27.988	4160	4161	4163	rBV2	1760	1099	0.23%	0.023%
64	29.863	4478	4480	4482	rBV2	1703	1378	0.28%	0.029%
65	30.016	4504	4506	4507	rVB	1736	919	0.19%	0.019%
66	30.726	4625	4627	4629	rBV3	2073	999	0.21%	0.021%
67	31.420	4743	4745	4747	rBV2	1322	1320	0.27%	0.028%
68	32.454	4919	4921	4922	rBV2	1767	1177	0.24%	0.025%




Sum of corrected areas: 4777121

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
Data File : BG056791.D
Acq On : 2 Mar 2023 15:22
Operator : CG/JU
Sample : PB151126BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

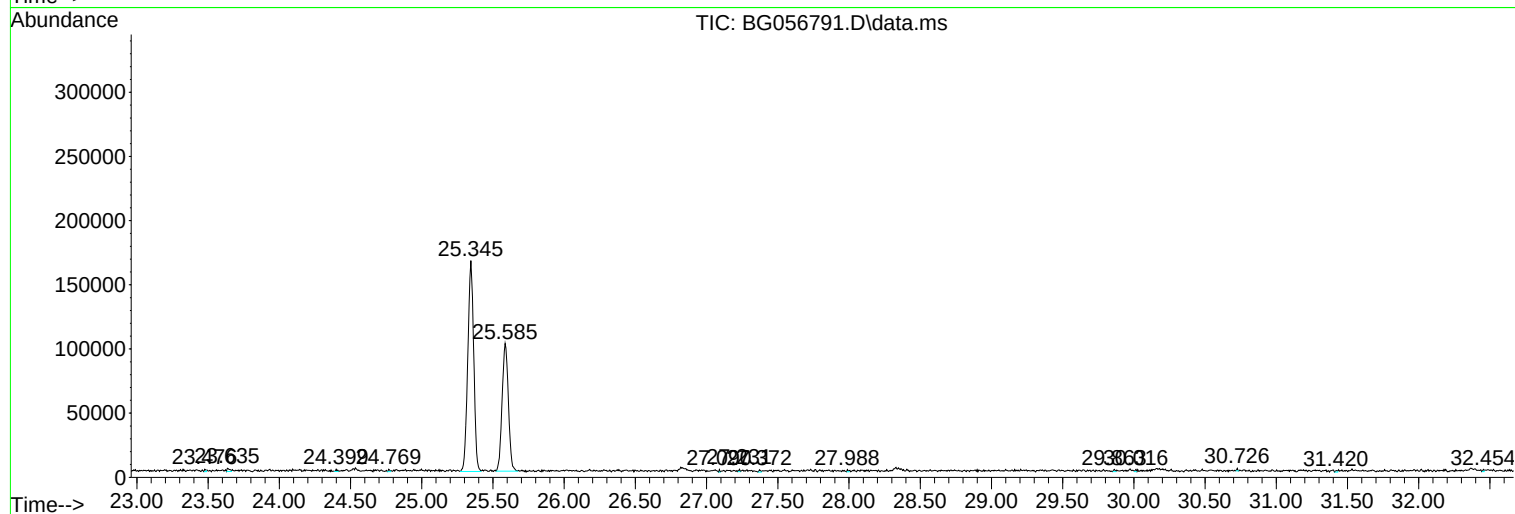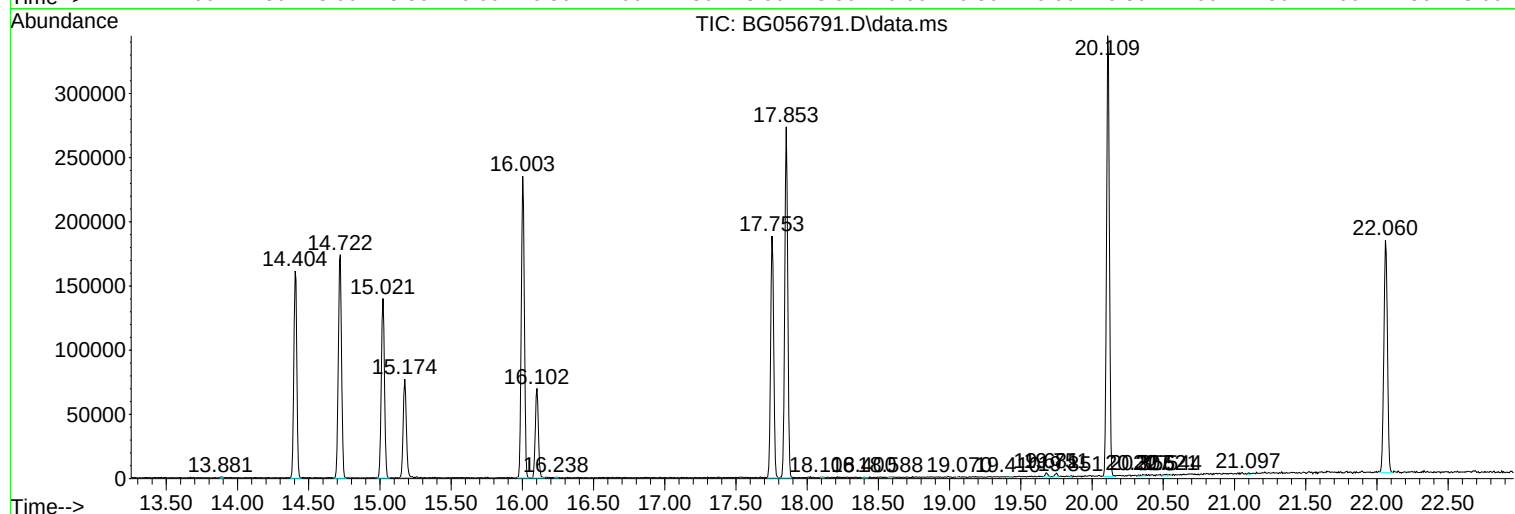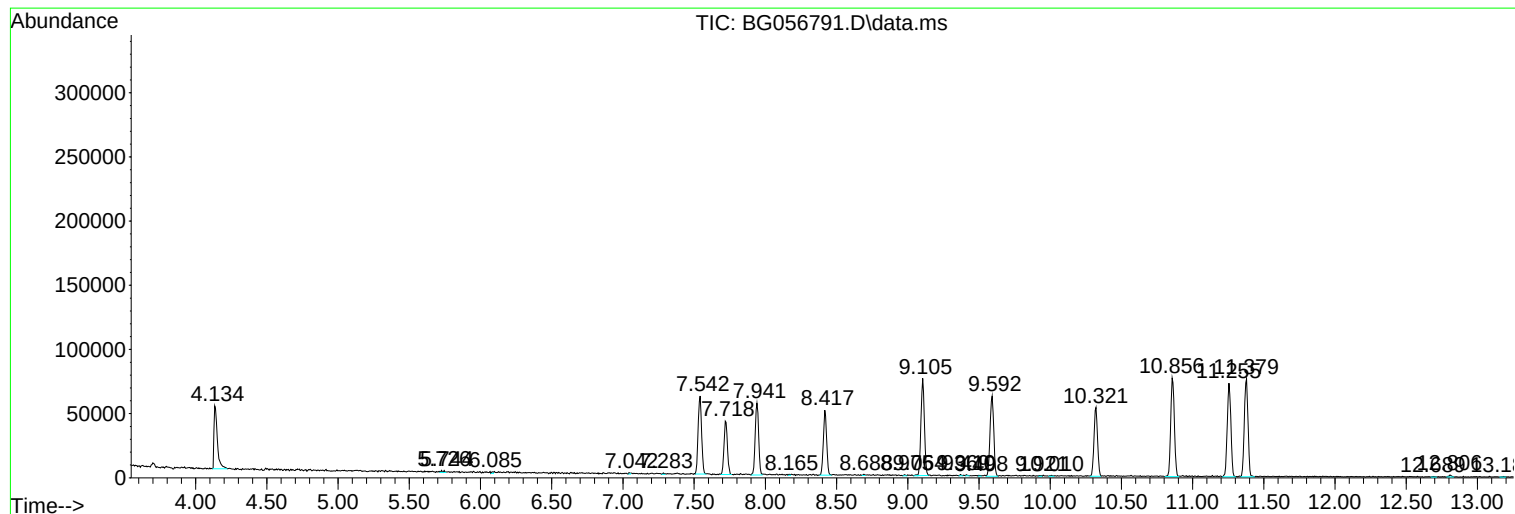

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
Data File : BG056791.D
Acq On : 2 Mar 2023 15:22
Operator : CG/JU
Sample : PB151126BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
Data File : BG056791.D
Acq On : 2 Mar 2023 15:22
Operator : CG/JU
Sample : PB151126BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc