

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
 Data File : BG056792.D
 Acq On : 2 Mar 2023 16:03
 Operator : CG/JU
 Sample : PB151151BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK151

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.137	98	102	112	rBV	60626	99549	16.89%	1.834%
2	7.539	675	681	689	rVB	74021	124763	21.17%	2.299%
3	7.721	706	712	719	rVB	50390	85033	14.43%	1.567%
4	7.939	743	749	756	rVB	64503	110788	18.80%	2.041%
5	8.420	825	831	837	rVB	46607	76353	12.96%	1.407%
6	9.108	941	948	955	rVB	87671	150419	25.53%	2.771%
7	9.590	1023	1030	1039	rVB	73712	132763	22.53%	2.446%
8	10.324	1148	1155	1160	rBV	60920	107868	18.31%	1.987%
9	10.859	1239	1246	1255	rVB2	96672	163454	27.74%	3.011%
10	11.258	1306	1314	1321	rBV2	64026	116799	19.82%	2.152%
11	11.376	1328	1334	1342	rBV	93437	163275	27.71%	3.008%
12	12.809	1574	1578	1584	rVB3	1836	2480	0.42%	0.046%
13	14.407	1844	1850	1856	rBV	201077	287639	48.82%	5.299%
14	14.719	1895	1903	1912	rVB	214110	334856	56.83%	6.169%
15	15.024	1948	1955	1961	rBV	127095	198354	33.66%	3.654%
16	15.177	1972	1981	1990	rBV	96899	150387	25.52%	2.771%
17	16.006	2115	2122	2130	rVB	294857	429422	72.88%	7.911%
18	16.105	2133	2139	2147	rBV	87378	130477	22.14%	2.404%
19	16.246	2160	2163	2167	rVB	815	941	0.16%	0.017%
20	17.756	2414	2420	2429	rVB	181784	275050	46.68%	5.067%
21	17.856	2430	2437	2446	rVB	312705	488978	82.98%	9.008%
22	18.062	2469	2472	2475	rVB2	732	822	0.14%	0.015%
23	18.162	2485	2489	2492	rVB	766	1029	0.17%	0.019%
24	18.309	2513	2514	2518	rBV	883	893	0.15%	0.016%
25	18.967	2622	2626	2628	rVB	822	1040	0.18%	0.019%
26	19.684	2743	2748	2752	rVB5	3977	5380	0.91%	0.099%
27	19.748	2755	2759	2764	rBV2	4371	6487	1.10%	0.120%
28	19.960	2792	2795	2797	rBV	916	1127	0.19%	0.021%
29	20.113	2814	2821	2828	rBV	422303	589240	100.00%	10.856%
30	20.588	2900	2902	2904	rBV2	1111	968	0.16%	0.018%
31	20.618	2904	2907	2911	rVV3	1318	1820	0.31%	0.034%
32	20.747	2927	2929	2931	rBV3	1376	1404	0.24%	0.026%
33	20.941	2960	2962	2965	rBV4	1204	1403	0.24%	0.026%
34	21.552	3064	3066	3069	rVB3	1519	1327	0.23%	0.024%
35	21.605	3073	3075	3076	rBV3	1701	1232	0.21%	0.023%
36	22.063	3146	3153	3160	rVB2	178354	300929	51.07%	5.544%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
 Data File : BG056792.D
 Acq On : 2 Mar 2023 16:03
 Operator : CG/JU
 Sample : PB151151BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK151

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	25.077	3664	3666	3668	rBV2	2089	1741	0.30%	0.032%
38	25.348	3701	3712	3725	rVB3	191990	566832	96.20%	10.443%
39	25.588	3743	3753	3765	rVB	98129	298598	50.68%	5.501%
40	26.382	3886	3888	3891	rBV2	1503	1667	0.28%	0.031%
41	26.405	3891	3892	3894	rVB	1918	1222	0.21%	0.023%
42	26.822	3961	3963	3967	rBV4	1933	1920	0.33%	0.035%
43	27.945	4153	4154	4155	rBV	1710	813	0.14%	0.015%
44	28.174	4192	4193	4196	rVB3	1751	1056	0.18%	0.019%
45	28.485	4244	4246	4248	rBV2	1329	1064	0.18%	0.020%
46	28.732	4286	4288	4292	rVB3	1534	995	0.17%	0.018%
47	29.701	4451	4453	4455	rVB3	1774	1075	0.18%	0.020%
48	30.818	4641	4643	4646	rVB3	1632	1633	0.28%	0.030%
49	30.847	4646	4648	4649	rBV	1340	868	0.15%	0.016%
50	32.292	4893	4894	4897	rBV2	1879	1368	0.23%	0.025%
51	32.533	4933	4935	4938	rBV2	1461	1491	0.25%	0.027%
52	32.627	4949	4951	4952	rBV	1646	920	0.16%	0.017%




Sum of corrected areas: 5428012

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
Data File : BG056792.D
Acq On : 2 Mar 2023 16:03
Operator : CG/JU
Sample : PB151151BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK151

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

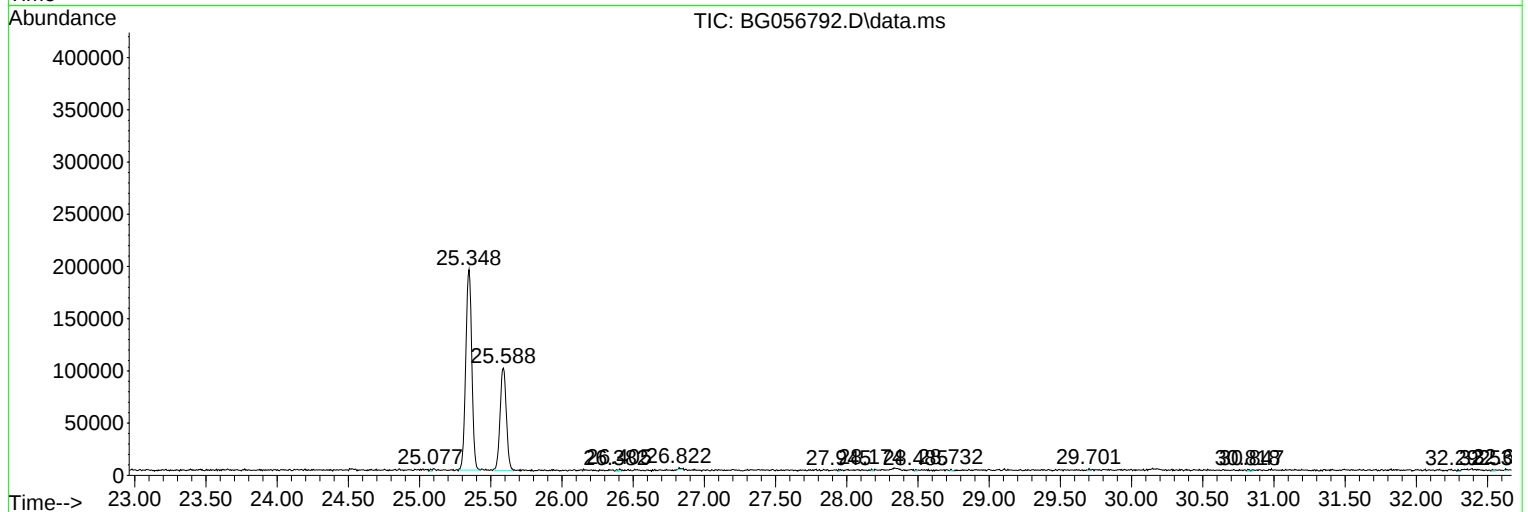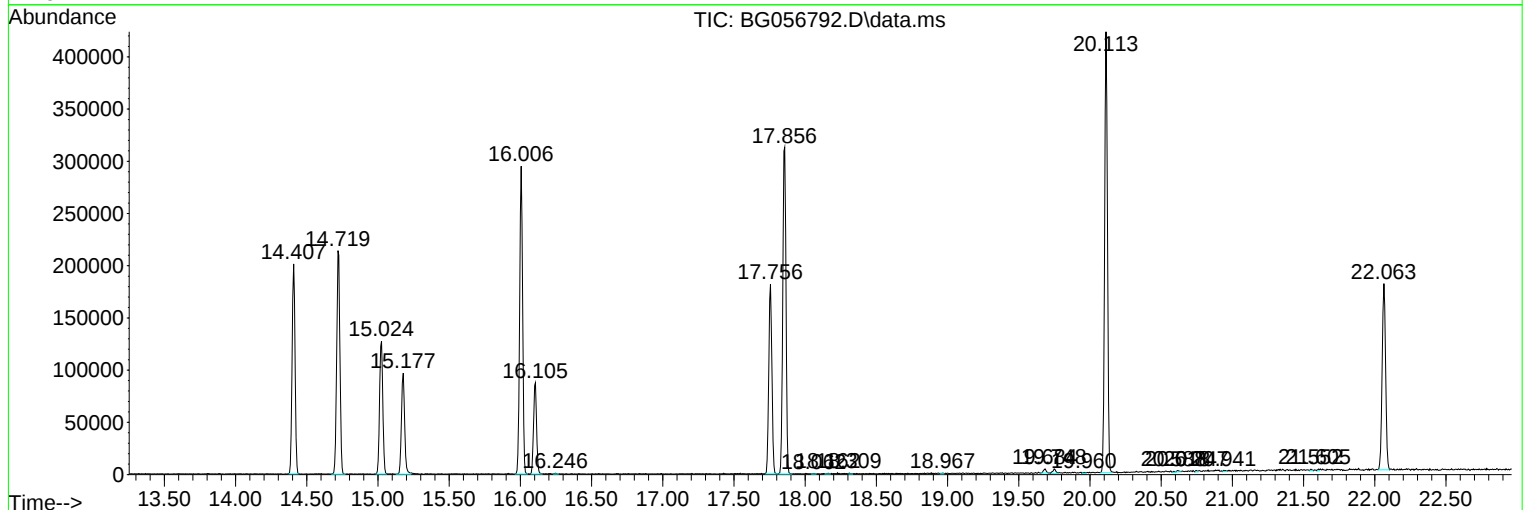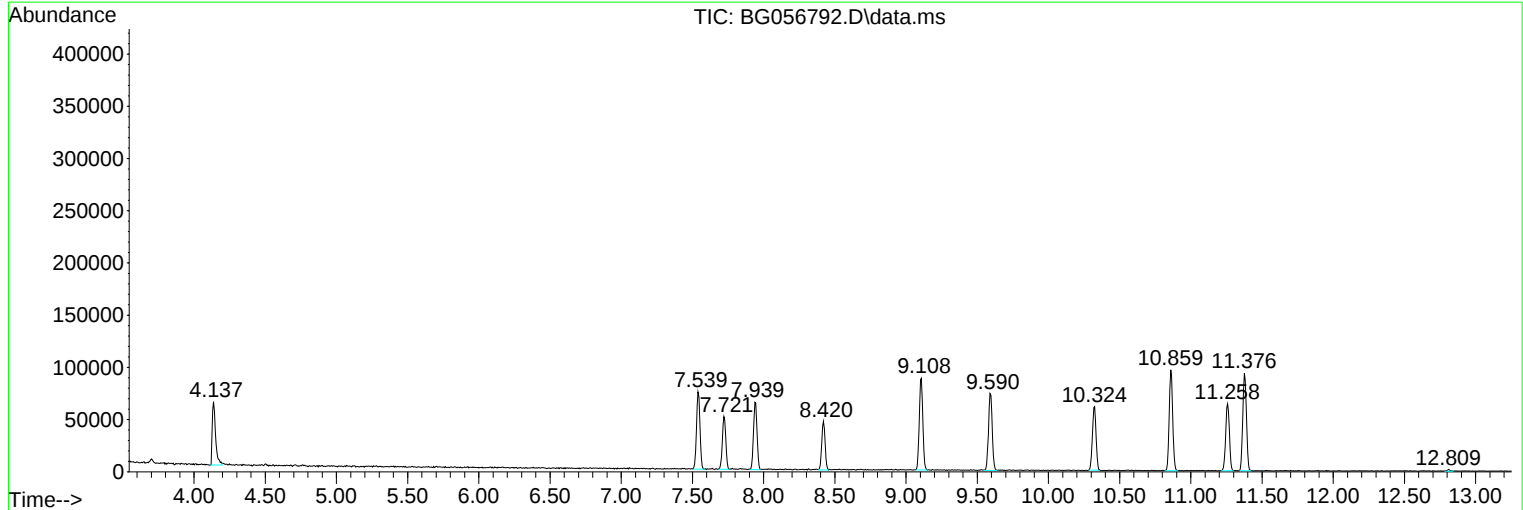

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
Data File : BG056792.D
Acq On : 2 Mar 2023 16:03
Operator : CG/JU
Sample : PB151151BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK151

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030223\
Data File : BG056792.D
Acq On : 2 Mar 2023 16:03
Operator : CG/JU
Sample : PB151151BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK151

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc