

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
 Data File : BG056824.D
 Acq On : 4 Mar 2023 5:32
 Operator : CG/JU
 Sample : 01711-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBAC9

Quant Time: Mar 05 23:55:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.422	152	15160	20.000	ng/ul	0.00
20) Naphthalene-d8	11.254	136	67186	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.020	164	54291	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.752	188	132736	20.000	ng/ul	0.00
79) Chrysene-d12	22.065	240	129193	20.000	ng/ul	0.00
88) Perylene-d12	25.584	264	138952	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.698	96	629	2.302	ng/uL	0.00
4) Pyridine-d5	4.145	84	156	0.141	ng/ul	0.01
7) Phenol-d5	7.541	99	23590	15.550	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.717	67	15455	16.701	ng/ul	0.00
11) 2-Chlorophenol-d4	7.934	132	15225	15.112	ng/ul	0.00
15) 4-Methylphenol-d8	9.104	113	17171	14.813	ng/ul	0.00
21) Nitrobenzene-d5	9.591	128	9276	16.475	ng/ul	0.00
24) 2-Nitrophenol-d4	10.320	143	10721	15.996	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.860	165	20980	16.616	ng/ul	0.00
31) 4-Chloroaniline-d4	11.378	131	1572	0.955	ng/ul	0.00
46) Dimethylphthalate-d6	14.403	166	62386	14.242	ng/ul	0.00
49) Acenaphthylene-d8	14.721	160	83297	16.731	ng/ul	0.00
54) 4-Nitrophenol-d4	15.173	143	7775	10.295	ng/ul	0.00
60) Fluorene-d10	16.002	176	68166	16.823	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.101	200	10635	11.976	ng/ul	0.00
73) Anthracene-d10	17.852	188	106161	16.486	ng/ul	0.00
81) Pyrene-d10	20.108	212	131963	15.095	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.338	264	124208	16.561	ng/ul	-0.01
Target Compounds						
					Qvalue	
10) Bis(2-Chloroethyl)ether	7.846	93	4960	4.511	ng/ul#	17
16) Acetophenone	9.245	105	3719	1.874	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056824.D
Acq On : 4 Mar 2023 5:32
Operator : CG/JU
Sample : 01711-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAC9

Quant Time: Mar 05 23:55:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

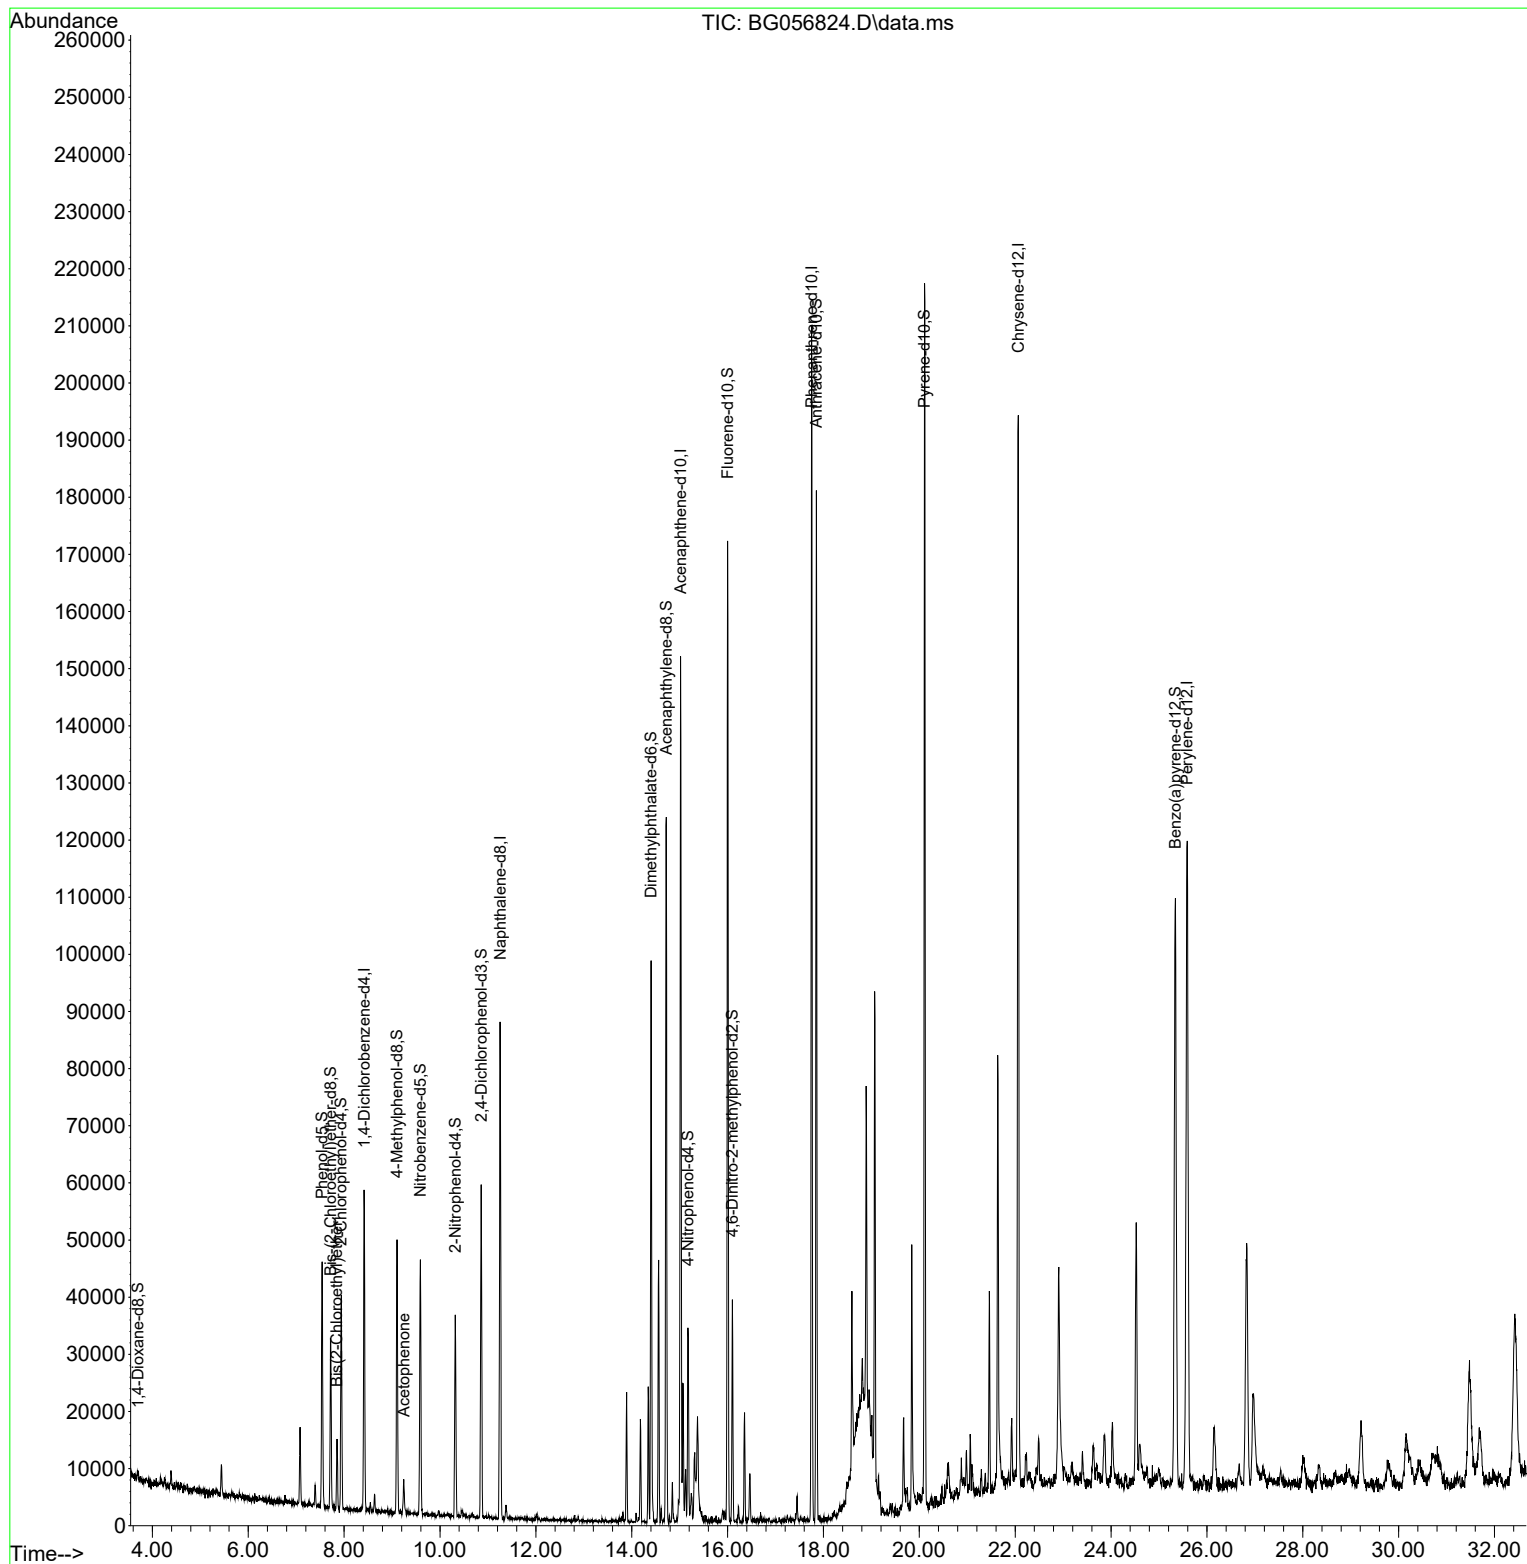

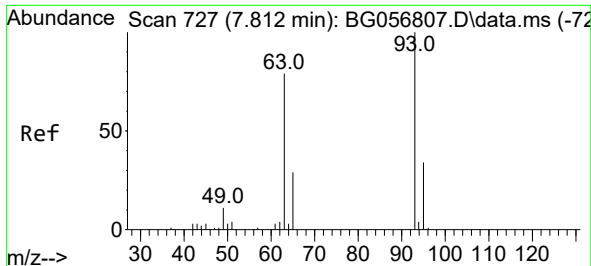

#10

Bis(2-Chloroethyl)ether

Concen: 4.511 ng/ul

RT: 7.846 min Scan# 71

Delta R.T. 0.028 min

Lab File: BG056824.D

Acq: 4 Mar 2023 5:32

Instrument :

BNA_G

ClientSampleId :

DBAC9





Tgt Ion: 93 Resp: 4960

Ion Ratio Lower Upper

93 100

63 0.0 66.6 100.0#

95 0.0 25.0 37.4#

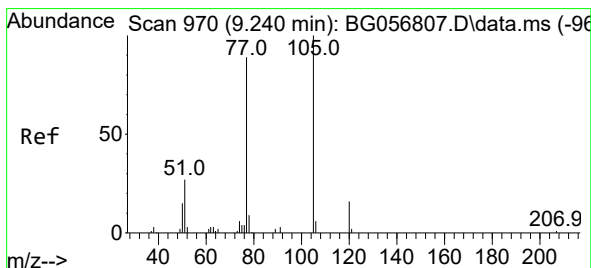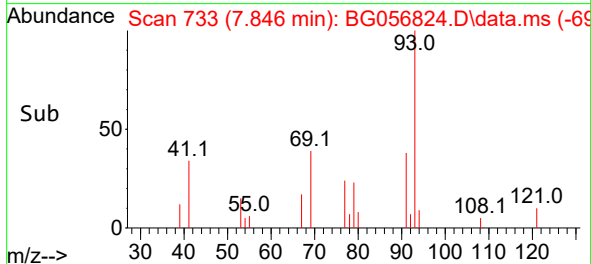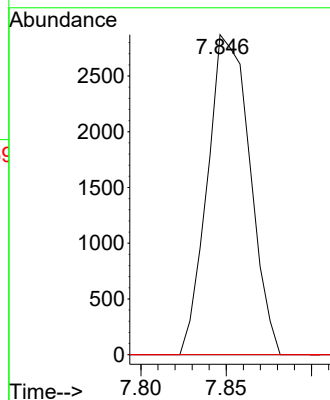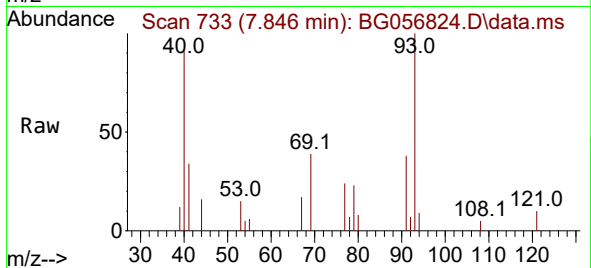

#16

Acetophenone

Concen: 1.874 ng/ul

RT: 9.245 min Scan# 971

Delta R.T. 0.005 min

Lab File: BG056824.D

Acq: 4 Mar 2023 5:32

Tgt Ion:105 Resp: 3719

Ion Ratio Lower Upper

105 100

77 82.3 71.4 107.0

51 22.3 23.6 35.4#

