

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
 Data File : BG056832.D
 Acq On : 4 Mar 2023 11:05
 Operator : CG/JU
 Sample : 01711-21
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBAD5

Quant Time: Mar 05 23:57:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.414	152	14169	20.000	ng/ul	0.00
20) Naphthalene-d8	11.252	136	61202	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.018	164	50506	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.756	188	128001	20.000	ng/ul	0.00
79) Chrysene-d12	22.057	240	120303	20.000	ng/ul	0.00
88) Perylene-d12	25.582	264	133175	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.702	96	2475	9.690	ng/uL	0.00
4) Pyridine-d5	4.137	84	41502	40.254	ng/ul	0.00
7) Phenol-d5	7.539	99	56474	39.830	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.721	67	35311	40.827	ng/ul	0.00
11) 2-Chlorophenol-d4	7.938	132	35455	37.654	ng/ul	0.00
15) 4-Methylphenol-d8	9.108	113	43206	39.880	ng/ul	0.00
21) Nitrobenzene-d5	9.589	128	20628	40.219	ng/ul	0.00
24) 2-Nitrophenol-d4	10.318	143	25609	41.946	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.858	165	47962	41.700	ng/ul	0.00
31) 4-Chloroaniline-d4	11.375	131	56361	37.570	ng/ul	0.00
46) Dimethylphthalate-d6	14.407	166	163504	40.124	ng/ul	0.00
49) Acenaphthylene-d8	14.719	160	191210	41.286	ng/ul	0.00
54) 4-Nitrophenol-d4	15.177	143	27312	38.875	ng/ul	0.00
60) Fluorene-d10	16.005	176	152054	40.339	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.099	200	33228	38.801	ng/ul	0.00
73) Anthracene-d10	17.850	188	251907	40.566	ng/ul	0.00
81) Pyrene-d10	20.112	212	299727	36.818	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.341	264	286748	39.891	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	9.108	70	1479	1.389 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056832.D
Acq On : 4 Mar 2023 11:05
Operator : CG/JU
Sample : 01711-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAD5

Quant Time: Mar 05 23:57:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

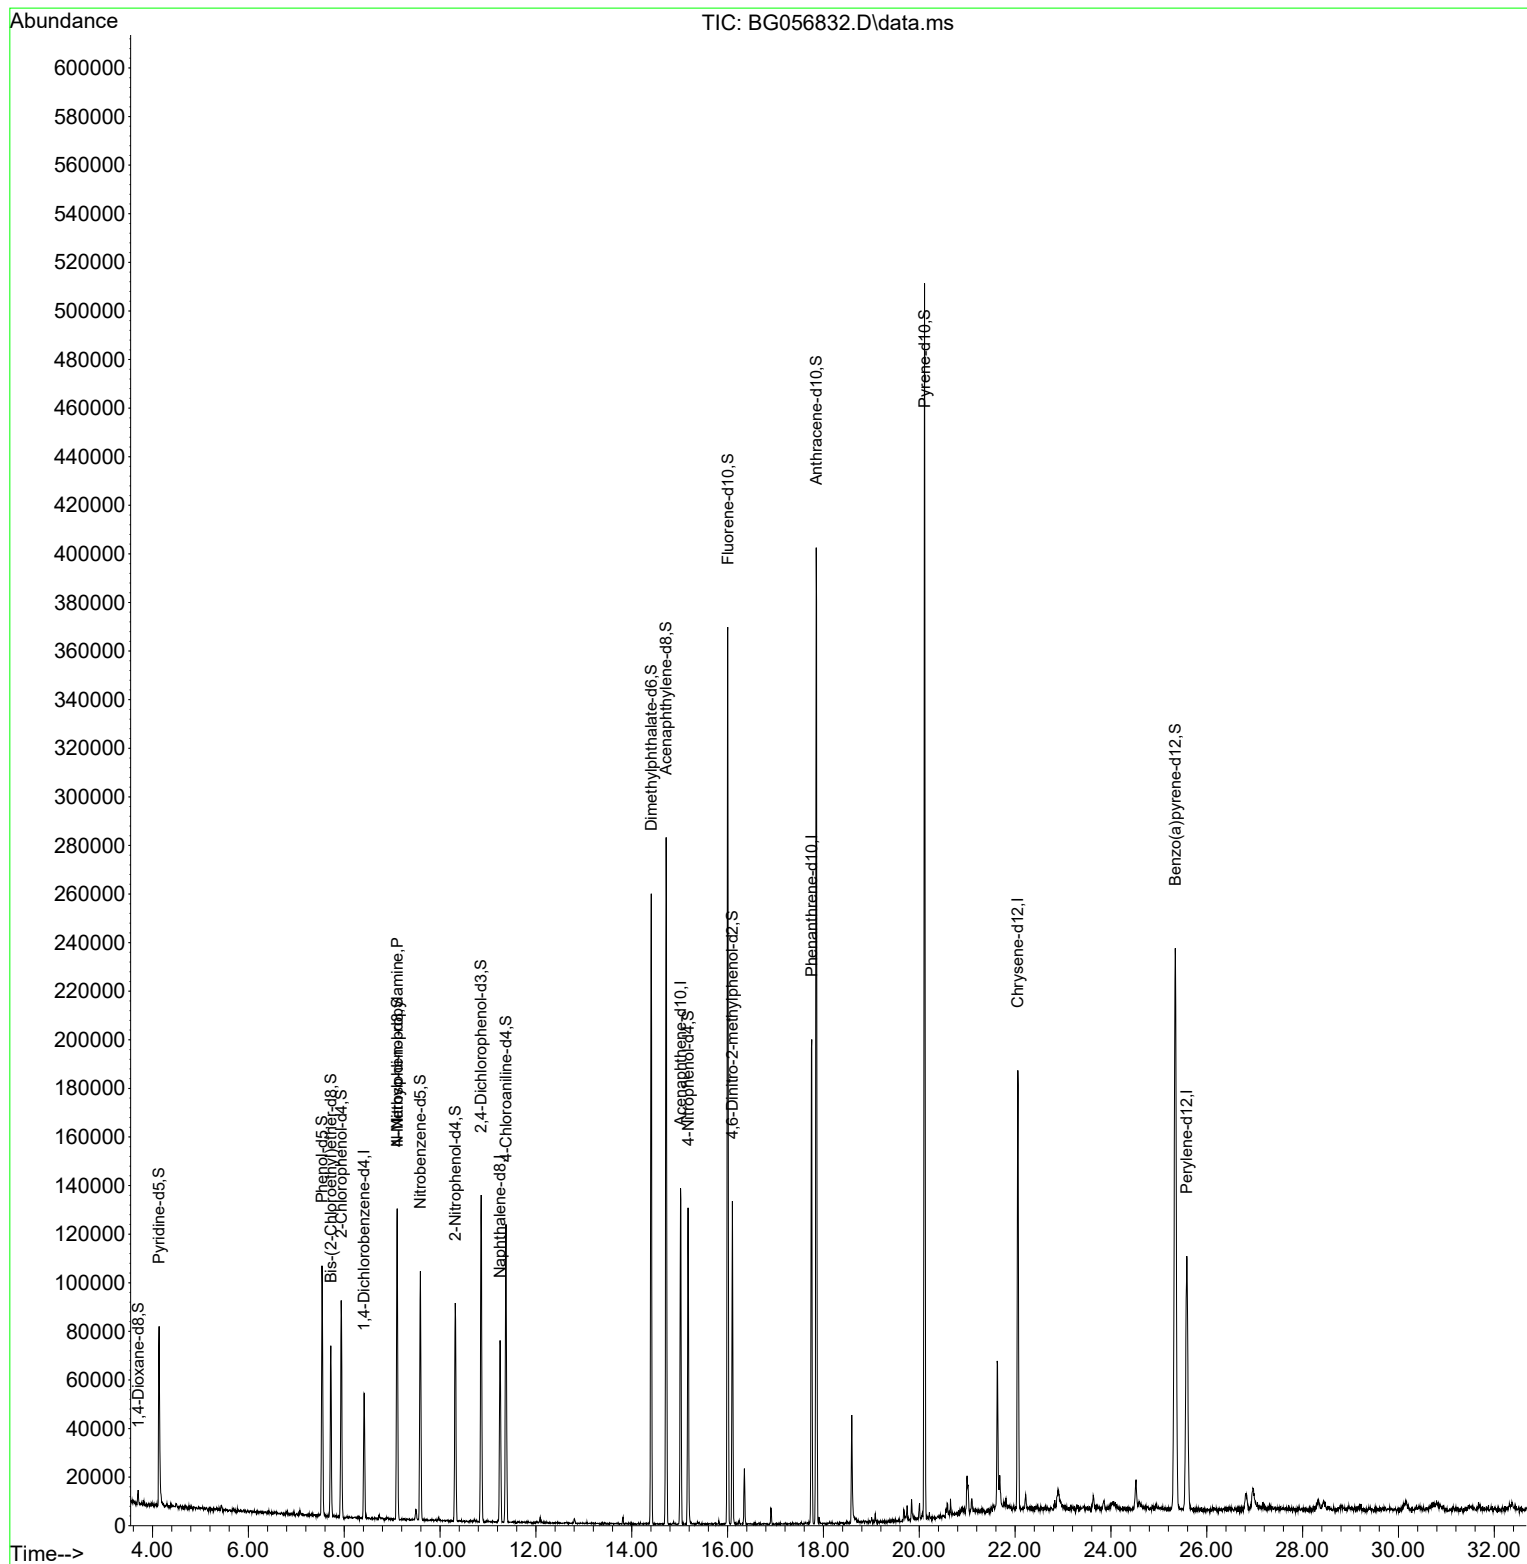

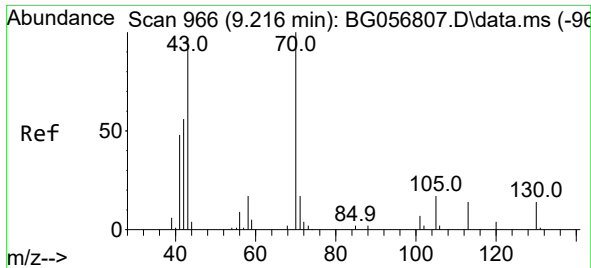

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.389 ng/ul
 RT: 9.108 min Scan# 94
 Delta R.T. -0.109 min
 Lab File: BG056832.D
 Acq: 4 Mar 2023 11:05

Instrument :
 BNA_G
 ClientSampleId :
 DBAD5

Tgt Ion: 70 Resp: 1479
 Ion Ratio Lower Upper
 70 100
 42 308.5 46.6 70.0#
 101 0.0 7.3 10.9#
 130 0.0 13.7 20.5#

