




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056817.D
Acq On : 4 Mar 2023 00:01
Operator : CG/JU
Sample : 01711-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAC4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/06/2023
Supervised By :Jagrut Upadhyay 03/06/2023

Quant Time: Mar 04 00:37:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

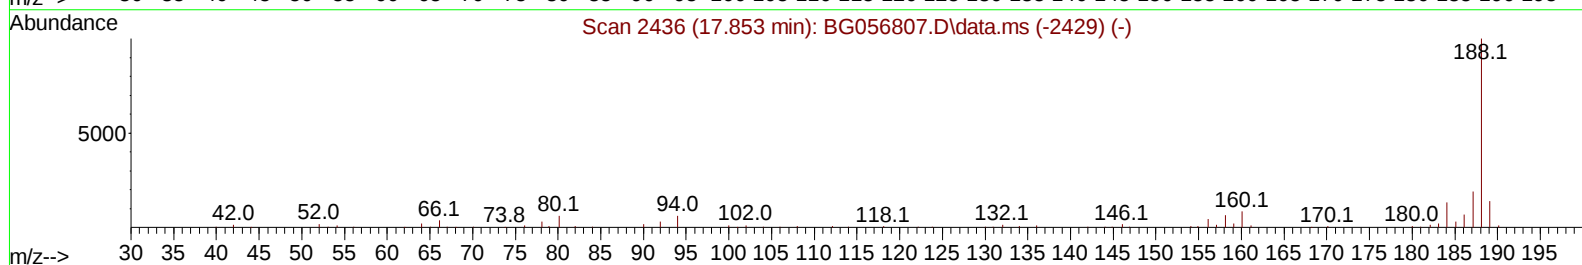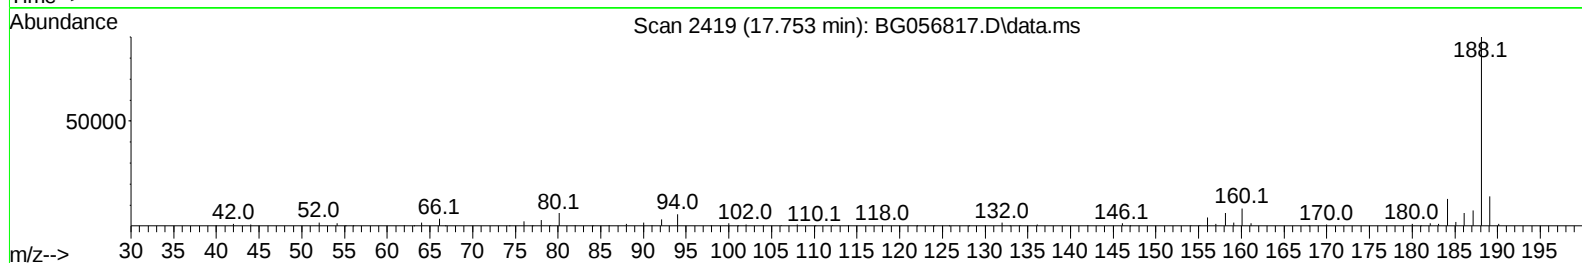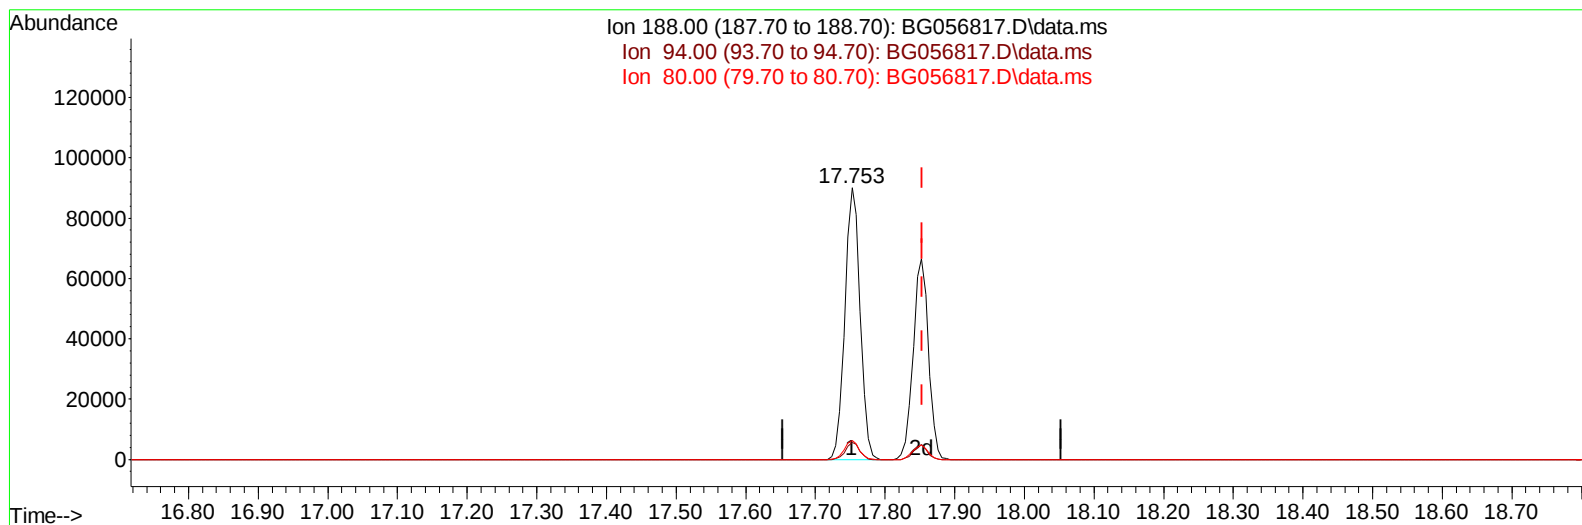

TIC: BG056817.D\data.ms

(73) Anthracene-d10 (S)

17.753min (-0.101) 20.61 ng/u1

response 136215

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	5.90	6.33
80.00	7.20	6.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
 Data File : BG056817.D
 Acq On : 4 Mar 2023 00:01
 Operator : CG/JU
 Sample : 01711-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBAC4

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:37:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/06/2023
 Supervised By :Jagrut Upadhyay 03/06/2023

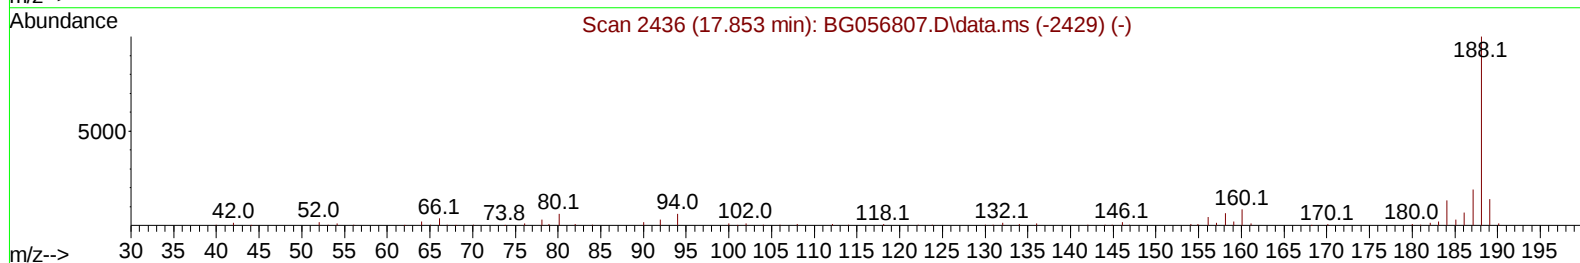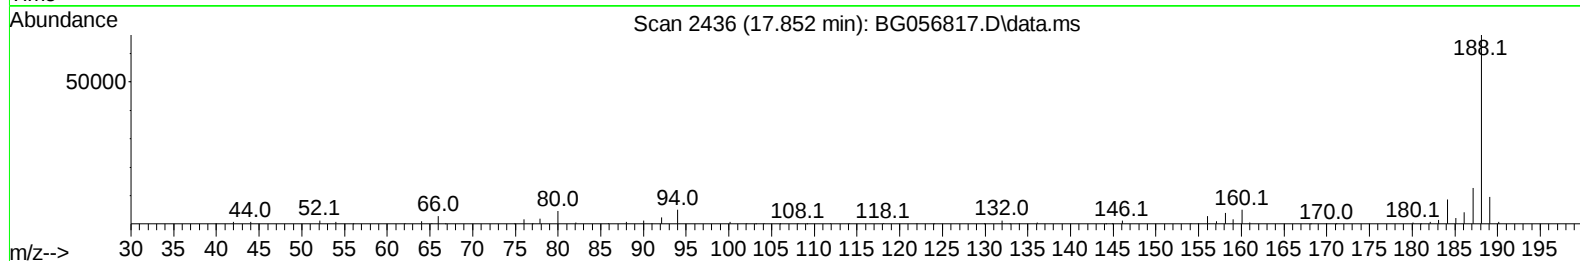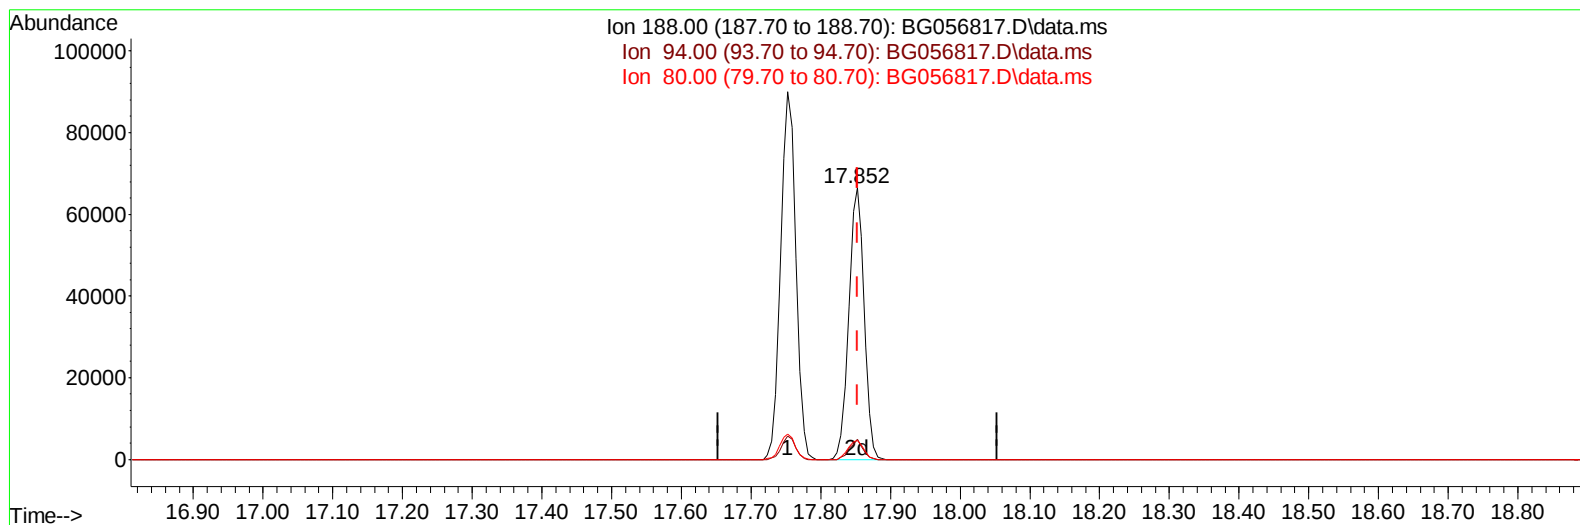

TIC: BG056817.D\data.ms

(73) Anthracene-d10 (S)

17.852min (-0.001) 15.35 ng/ul m

response 101435

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	5.90	7.53#
80.00	7.20	7.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
 Data File : BG056817.D
 Acq On : 4 Mar 2023 00:01
 Operator : CG/JU
 Sample : 01711-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBAC4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/06/2023
 Supervised By :Jagrut Upadhyay 03/06/2023

Quant Time: Mar 04 00:37:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.422	152	14343	20.000	ng/ul	0.00
20) Naphthalene-d8	11.254	136	63406	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.021	164	54459	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.753	188	136215	20.000	ng/ul	0.00
79) Chrysene-d12	22.059	240	130576	20.000	ng/ul	0.00
88) Perylene-d12	25.585	264	140260	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.704	96	731	2.827	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.535	99	20989	14.623	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.723	67	13147	15.016	ng/ul	0.00
11) 2-Chlorophenol-d4	7.941	132	13277	13.930	ng/ul	0.00
15) 4-Methylphenol-d8	9.104	113	15366	14.011	ng/ul	0.00
21) Nitrobenzene-d5	9.592	128	7642	14.382	ng/ul	0.00
24) 2-Nitrophenol-d4	10.320	143	9388	14.842	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.855	165	17209	14.442	ng/ul	0.00
31) 4-Chloroaniline-d4	11.372	131	18911	12.168	ng/ul	0.00
46) Dimethylphthalate-d6	14.404	166	64274	14.628	ng/ul	0.00
49) Acenaphthylene-d8	14.715	160	73413	14.701	ng/ul	0.00
54) 4-Nitrophenol-d4	15.173	143	9368	12.366	ng/ul	0.00
60) Fluorene-d10	16.002	176	59244	14.576	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.102	200	12171	13.355	ng/ul	0.00
73) Anthracene-d10	17.852	188	101435m	15.350	ng/ul	0.00
81) Pyrene-d10	20.109	212	123045	13.926	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.344	264	115307	15.231	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056817.D
Acq On : 4 Mar 2023 00:01
Operator : CG/JU
Sample : 01711-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAC4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/06/2023
Supervised By :Jagrut Upadhyay 03/06/2023

Quant Time: Mar 04 00:37:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

