

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
 Data File : BG056808.D
 Acq On : 3 Mar 2023 17:49
 Operator : CG/JU
 Sample : PB151148BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK148

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.132	98	101	115	rBV	53996	90656	17.74%	1.814%
2	5.078	260	262	264	rBV	1638	1108	0.22%	0.022%
3	6.864	564	566	569	rBV2	1046	1183	0.23%	0.024%
4	7.534	674	680	690	rVB	66554	108149	21.17%	2.164%
5	7.716	705	711	719	rVB	47695	74561	14.59%	1.492%
6	7.933	742	748	754	rVB	55143	94182	18.43%	1.884%
7	8.409	823	829	839	rVB	51122	85950	16.82%	1.720%
8	8.544	850	852	855	rBV	730	727	0.14%	0.015%
9	9.103	940	947	954	rVB	78722	132589	25.95%	2.653%
10	9.584	1023	1029	1037	rBV	66540	115046	22.52%	2.302%
11	9.949	1088	1091	1092	rBV	821	744	0.15%	0.015%
12	10.025	1102	1104	1107	rVB2	797	714	0.14%	0.014%
13	10.319	1147	1154	1160	rVB	50262	88497	17.32%	1.771%
14	10.765	1227	1230	1233	rBV2	471	699	0.14%	0.014%
15	10.853	1239	1245	1253	rVB2	80882	142234	27.84%	2.846%
16	11.253	1306	1313	1320	rBV	78908	133752	26.18%	2.676%
17	11.370	1327	1333	1341	rBV	80735	145309	28.44%	2.907%
18	12.804	1573	1577	1582	rVB3	1029	1839	0.36%	0.037%
19	14.402	1843	1849	1856	rVB	168032	246271	48.20%	4.927%
20	14.496	1863	1865	1869	rBV	513	704	0.14%	0.014%
21	14.719	1896	1903	1911	rVB	184415	288943	56.55%	5.781%
22	15.019	1947	1954	1961	rVB	143684	224060	43.85%	4.483%
23	15.172	1974	1980	1993	rBV	75611	122346	23.94%	2.448%
24	15.495	2030	2035	2038	rBV2	613	1224	0.24%	0.024%
25	16.000	2115	2121	2129	rVB	251027	377750	73.93%	7.558%
26	16.100	2133	2138	2145	rVB	67605	95620	18.71%	1.913%
27	16.300	2170	2172	2176	rVB	538	681	0.13%	0.014%
28	17.622	2394	2397	2400	rBV	453	792	0.15%	0.016%
29	17.751	2413	2419	2427	rVB	202517	302588	59.22%	6.054%
30	17.851	2430	2436	2445	rVB2	292333	423911	82.96%	8.481%
31	18.210	2494	2497	2502	rVB	968	1322	0.26%	0.026%
32	18.403	2528	2530	2533	rVB	737	775	0.15%	0.016%
33	19.144	2654	2656	2658	rBV2	698	792	0.15%	0.016%
34	19.355	2690	2692	2695	rVB	828	739	0.14%	0.015%
35	19.631	2737	2739	2742	rBV	892	847	0.17%	0.017%
36	19.684	2744	2748	2755	rVV4	3707	5476	1.07%	0.110%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
 Data File : BG056808.D
 Acq On : 3 Mar 2023 17:49
 Operator : CG/JU
 Sample : PB151148BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK148

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	19.749	2755	2759	2763	rVB	2978	4029	0.79%	0.081%
38	20.107	2814	2820	2827	rBV	352463	510968	100.00%	10.223%
39	20.201	2833	2836	2838	rBV2	1074	1352	0.26%	0.027%
40	20.342	2858	2860	2861	rVB	1274	715	0.14%	0.014%
41	20.354	2861	2862	2864	rBV2	849	736	0.14%	0.015%
42	20.524	2890	2891	2894	rBV2	1137	744	0.15%	0.015%
43	21.600	3072	3074	3075	rVB	1925	902	0.18%	0.018%
44	21.617	3075	3077	3079	rVV3	1984	2276	0.45%	0.046%
45	21.641	3079	3081	3084	rVB3	2940	2854	0.56%	0.057%
46	22.058	3146	3152	3164	rVB2	199245	338218	66.19%	6.767%
47	23.586	3410	3412	3413	rBV	1739	1362	0.27%	0.027%
48	25.342	3699	3711	3725	rBV2	161818	485634	95.04%	9.716%
49	25.583	3742	3752	3765	rVB3	107520	326544	63.91%	6.533%
50	26.500	3906	3908	3912	rBV4	1709	2437	0.48%	0.049%
51	27.475	4073	4074	4075	rBV	1804	773	0.15%	0.015%
52	28.304	4213	4215	4216	rBV2	2449	2386	0.47%	0.048%
53	30.295	4552	4554	4555	rBV	1602	1117	0.22%	0.022%
54	30.724	4625	4627	4630	rBV3	1779	2374	0.46%	0.047%




Sum of corrected areas: 4998201

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056808.D
Acq On : 3 Mar 2023 17:49
Operator : CG/JU
Sample : PB151148BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK148

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

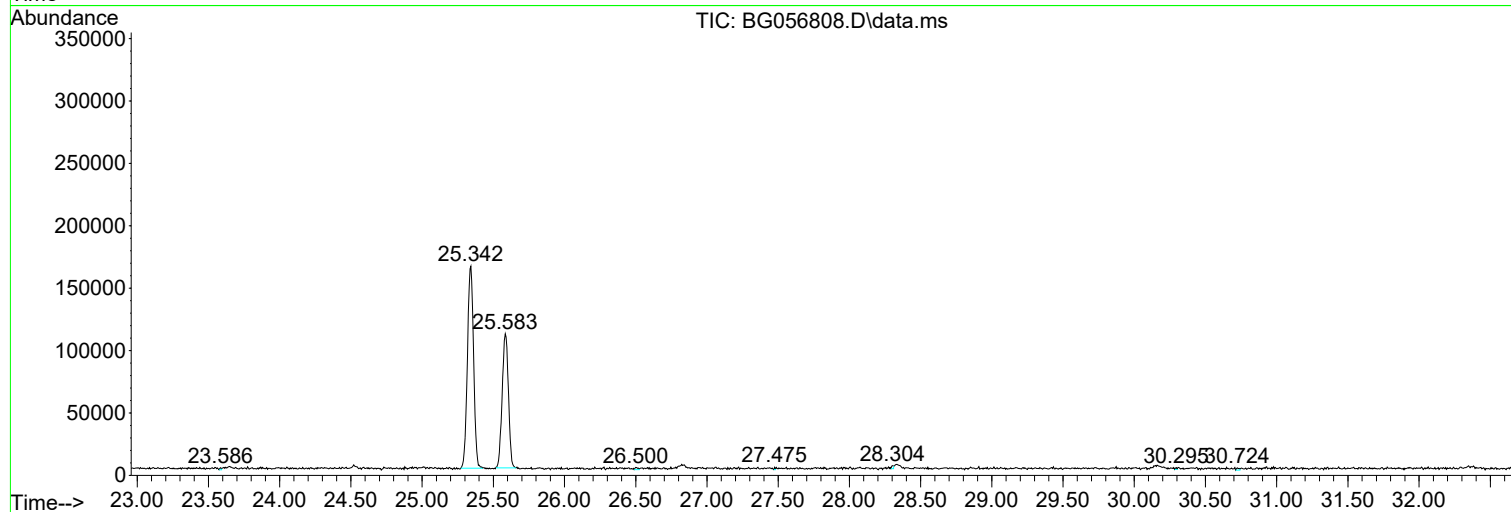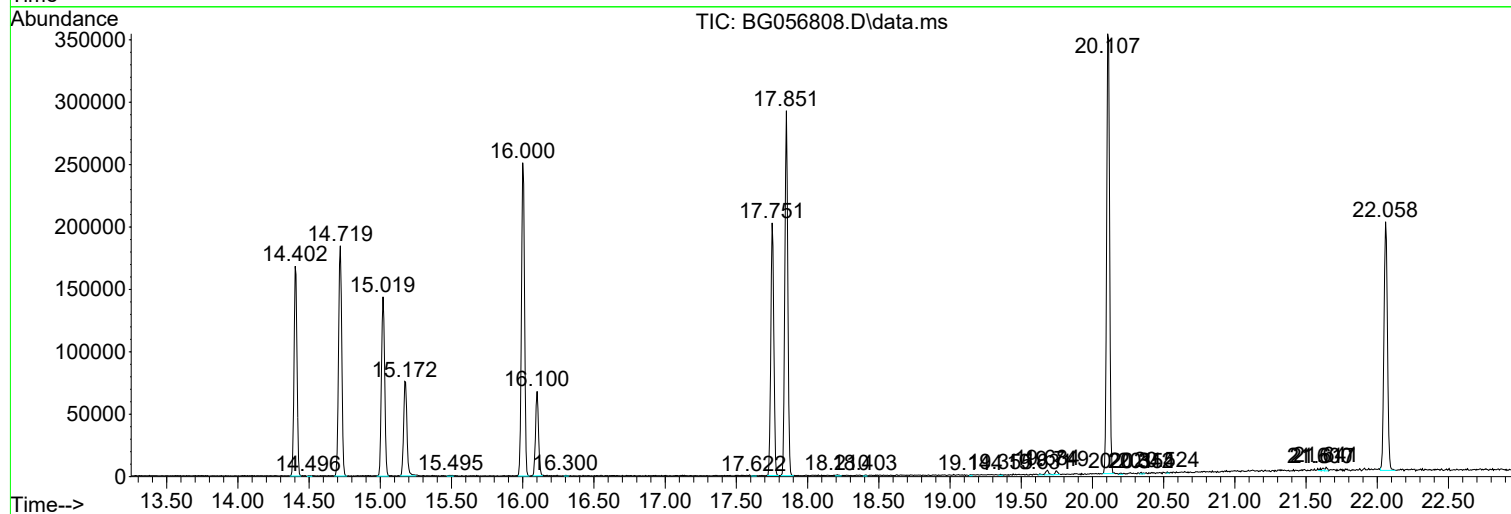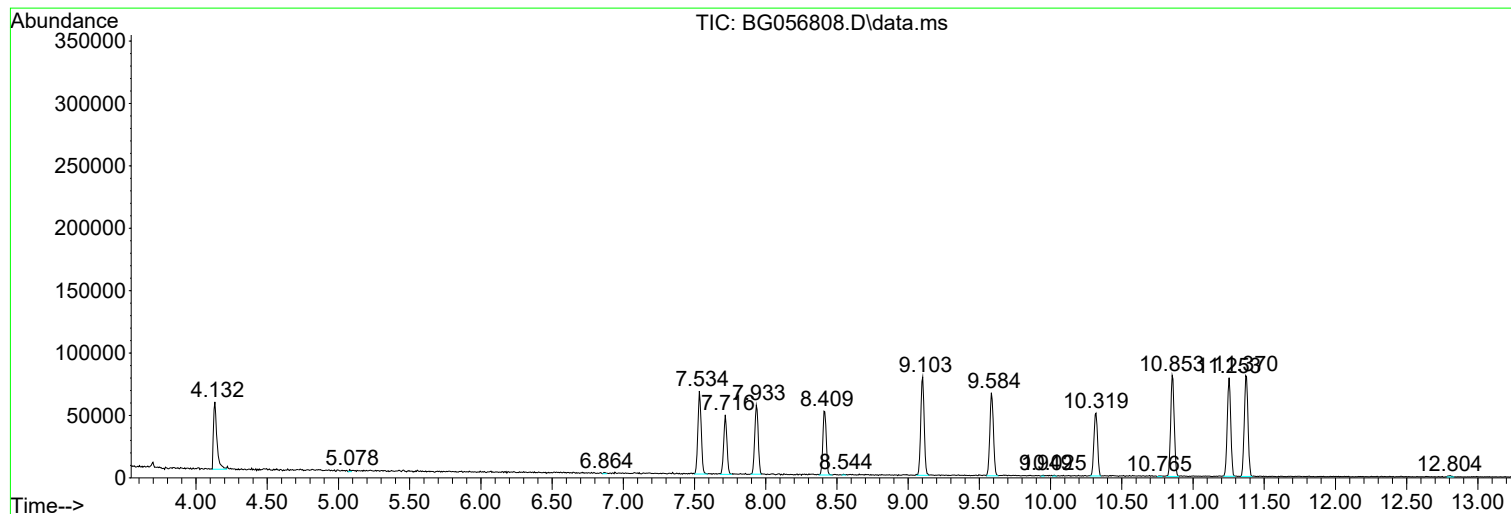

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056808.D
Acq On : 3 Mar 2023 17:49
Operator : CG/JU
Sample : PB151148BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK148

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056808.D
Acq On : 3 Mar 2023 17:49
Operator : CG/JU
Sample : PB151148BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK148

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------