

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
 Data File : BG056830.D
 Acq On : 4 Mar 2023 9:42
 Operator : CG/JU
 Sample : 01711-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBAD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.135	98	101	111	rBV	34800	54656	14.46%	1.317%
2	7.537	674	680	689	rVB	48163	83529	22.10%	2.012%
3	7.719	705	711	717	rBV	32724	53017	14.03%	1.277%
4	7.942	742	749	755	rBV	44763	74649	19.75%	1.798%
5	8.418	823	830	836	rBV	49704	81374	21.53%	1.960%
6	9.105	940	947	956	rVB2	61381	106063	28.07%	2.555%
7	9.587	1023	1029	1036	rVB2	47435	86327	22.85%	2.080%
8	10.316	1147	1153	1163	rVB2	41823	74024	19.59%	1.783%
9	10.698	1215	1218	1221	rBV	761	834	0.22%	0.020%
10	10.856	1238	1245	1254	rBV	64945	110691	29.29%	2.667%
11	11.256	1306	1313	1319	rBV	75343	128589	34.03%	3.098%
12	11.373	1326	1333	1340	rBV	61196	109157	28.89%	2.630%
13	12.795	1573	1575	1579	rVB3	814	1005	0.27%	0.024%
14	13.823	1747	1750	1752	rBV3	874	1119	0.30%	0.027%
15	13.894	1756	1762	1765	rVB	1098	1553	0.41%	0.037%
16	14.405	1843	1849	1856	rVB	134347	188219	49.81%	4.534%
17	14.716	1896	1902	1911	rVB	148044	225362	59.64%	5.429%
18	14.875	1924	1929	1930	rVB	577	703	0.19%	0.017%
19	15.022	1947	1954	1961	rVB	135781	213307	56.45%	5.139%
20	15.175	1973	1980	1989	rBV	59463	93027	24.62%	2.241%
21	15.239	1989	1991	1995	rVB2	548	677	0.18%	0.016%
22	15.721	2070	2073	2077	rVB2	844	990	0.26%	0.024%
23	16.003	2115	2121	2128	rBV	194009	287028	75.96%	6.915%
24	16.103	2130	2138	2143	rBV	52507	75370	19.95%	1.816%
25	16.350	2175	2180	2186	rBV	12371	17895	4.74%	0.431%
26	17.125	2310	2312	2314	rVB	669	550	0.15%	0.013%
27	17.149	2314	2316	2318	rBV	691	631	0.17%	0.015%
28	17.443	2363	2366	2368	rBV	546	656	0.17%	0.016%
29	17.754	2413	2419	2428	rVB	194863	289193	76.53%	6.967%
30	17.854	2428	2436	2442	rBV	202172	313298	82.91%	7.547%
31	17.913	2442	2446	2449	rVB3	2394	2229	0.59%	0.054%
32	18.118	2480	2481	2483	rBV	968	613	0.16%	0.015%
33	18.594	2557	2562	2570	rBV3	13743	20697	5.48%	0.499%
34	18.665	2572	2574	2580	rVB2	809	1201	0.32%	0.029%
35	18.735	2584	2586	2588	rBV3	622	726	0.19%	0.017%
36	18.776	2592	2593	2596	rBV2	661	665	0.18%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
 Data File : BG056830.D
 Acq On : 4 Mar 2023 9:42
 Operator : CG/JU
 Sample : 01711-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBAD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	18.870	2607	2609	2612	rBV2	872	696	0.18%	0.017%
38	18.964	2623	2625	2628	rVB	834	855	0.23%	0.021%
39	19.005	2628	2632	2637	rBV3	1616	2647	0.70%	0.064%
40	19.246	2671	2673	2677	rVB2	628	660	0.17%	0.016%
41	19.287	2677	2680	2683	rBV	812	1123	0.30%	0.027%
42	19.681	2744	2747	2752	rBV3	2857	2882	0.76%	0.069%
43	19.752	2754	2759	2766	rVB3	2401	4083	1.08%	0.098%
44	19.810	2767	2769	2771	rVB2	1176	838	0.22%	0.020%
45	19.840	2771	2774	2777	rBV3	2111	2718	0.72%	0.065%
46	19.869	2777	2779	2783	rVB3	909	920	0.24%	0.022%
47	19.910	2783	2786	2789	rBV3	750	799	0.21%	0.019%
48	19.987	2797	2799	2804	rVB2	1468	1481	0.39%	0.036%
49	20.028	2804	2806	2808	rBV	627	583	0.15%	0.014%
50	20.069	2811	2813	2814	rVV2	1609	1272	0.34%	0.031%
51	20.110	2814	2820	2827	rVB	273109	377880	100.00%	9.103%
52	20.204	2833	2836	2837	rVB	1314	1065	0.28%	0.026%
53	20.222	2837	2839	2840	rBV2	1093	806	0.21%	0.019%
54	20.357	2859	2862	2863	rBV2	1120	1199	0.32%	0.029%
55	20.398	2867	2869	2871	rBV	1012	860	0.23%	0.021%
56	20.504	2885	2887	2890	rBV3	1001	709	0.19%	0.017%
57	20.527	2890	2891	2894	rVV2	1161	814	0.22%	0.020%
58	20.592	2899	2902	2904	rVB3	2890	3307	0.88%	0.080%
59	20.974	2961	2967	2969	rBV4	2762	4216	1.12%	0.102%
60	21.097	2985	2988	2990	rVB2	4124	3895	1.03%	0.094%
61	21.138	2993	2995	2996	rBV	1563	1120	0.30%	0.027%
62	21.632	3075	3079	3083	rBV3	14195	20706	5.48%	0.499%
63	21.779	3102	3104	3109	rVB4	2010	2682	0.71%	0.065%
64	22.061	3146	3152	3159	rVB	176261	314667	83.27%	7.580%
65	22.196	3173	3175	3176	rBV	1643	1001	0.26%	0.024%
66	22.219	3176	3179	3184	rVB5	4094	5954	1.58%	0.143%
67	22.354	3200	3202	3205	rBV3	2058	1829	0.48%	0.044%
68	22.401	3209	3210	3211	rBV	1550	726	0.19%	0.017%
69	22.918	3296	3298	3301	rBV3	1811	2202	0.58%	0.053%
70	22.983	3308	3309	3311	rBV	1552	664	0.18%	0.016%
71	24.517	3566	3570	3577	rVB7	4787	8837	2.34%	0.213%
72	25.339	3700	3710	3722	rVB2	123330	356963	94.46%	8.599%
73	25.580	3741	3751	3766	rBV2	101743	313577	82.98%	7.554%
74	26.808	3958	3960	3962	rBV2	2869	3279	0.87%	0.079%
75	32.307	4894	4896	4897	rBV	1923	904	0.24%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056830.D
Acq On : 4 Mar 2023 9:42
Operator : CG/JU
Sample : 01711-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAD3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Title : SVOA CALIBRATION




Sum of corrected areas: 4151043

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056830.D
Acq On : 4 Mar 2023 9:42
Operator : CG/JU
Sample : 01711-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

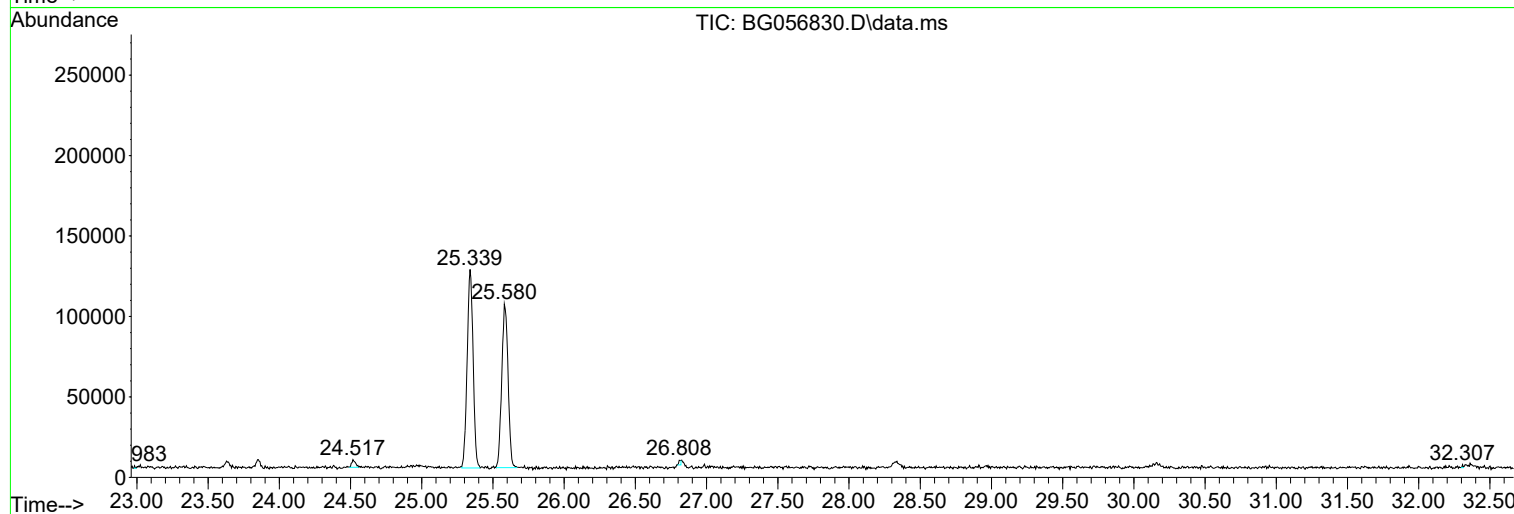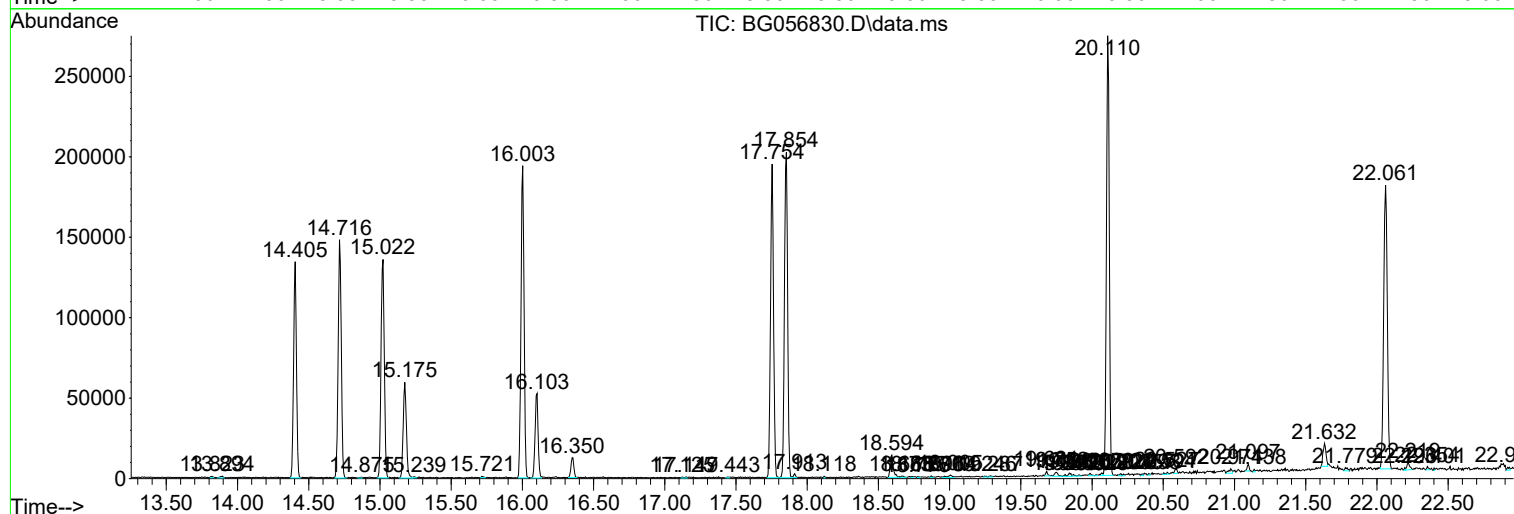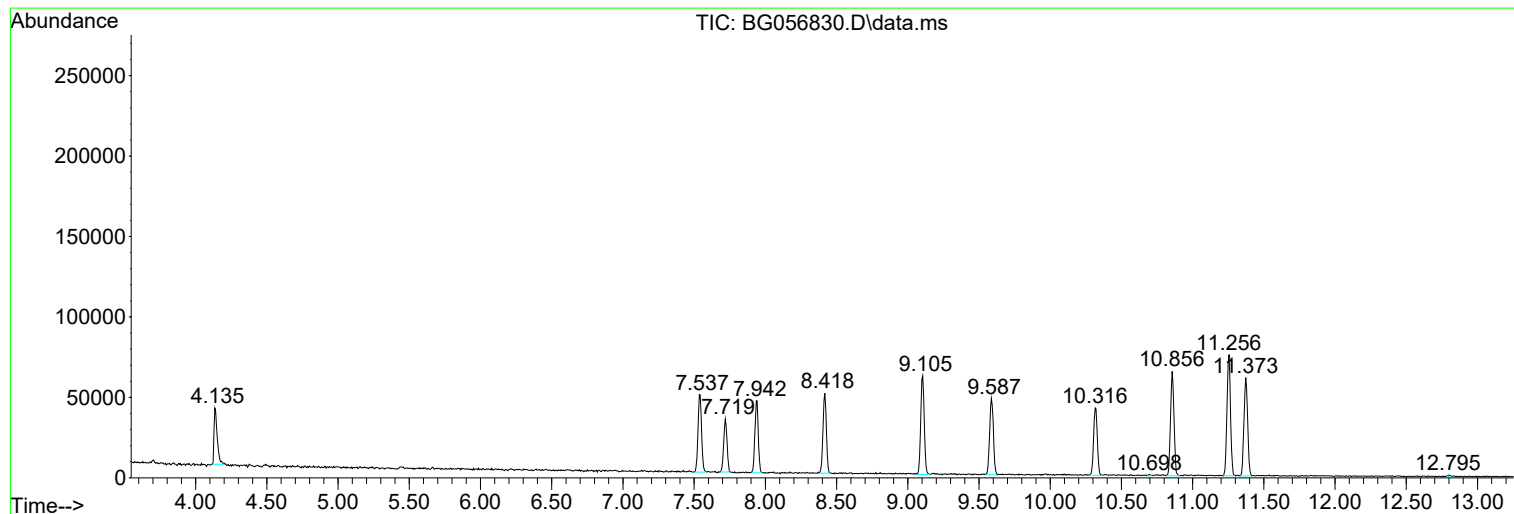

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056830.D
Acq On : 4 Mar 2023 9:42
Operator : CG/JU
Sample : 01711-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030323\
Data File : BG056830.D
Acq On : 4 Mar 2023 9:42
Operator : CG/JU
Sample : 01711-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc