
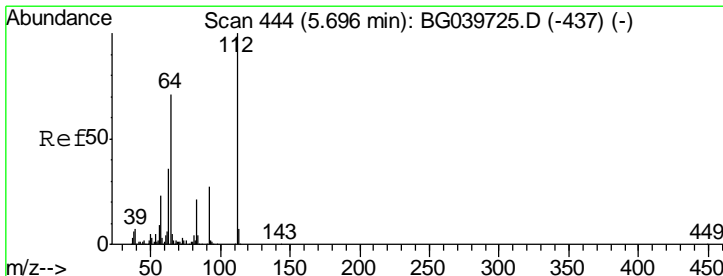
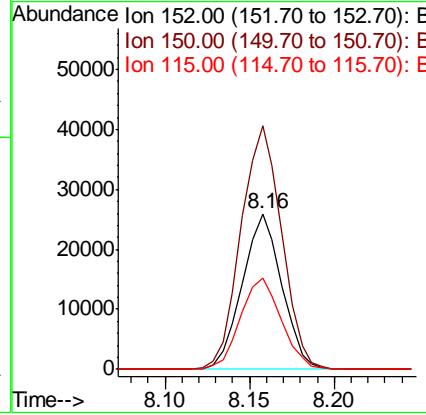
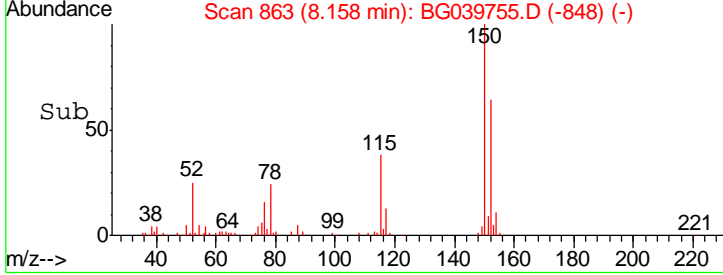


#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.16 min Scan# 863
 Delta R.T. -0.01 min
 Lab File: BG039755.D
 Acq: 5 Mar 2019 7:32

Instrument :
 BNA_G
 ClientSampled :

Tgt Ion	Resp	Lower	Upper
152	42265		
150	156.2	123.7	185.5
115	58.8	45.9	68.9

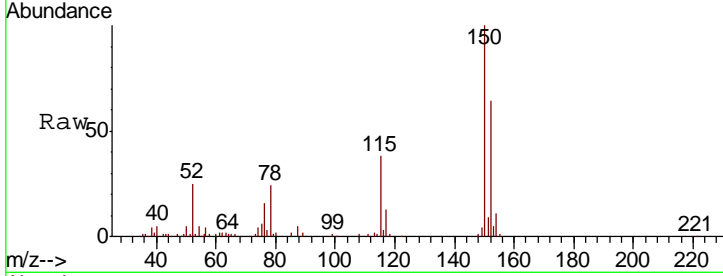

#5
 2-Fluorophenol
 Concen: 131.465 ng
 RT: 5.70 min Scan# 445
 Delta R.T. -0.01 min
 Lab File: BG039755.D
 Acq: 5 Mar 2019 7:32

Tgt Ion	Resp	Lower	Upper
112	325695		
64	66.5	57.8	86.8
63	36.5	29.8	44.6

