





#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.98 min Scan# 1343
Delta R.T. -0.01 min
Lab File: BG039755.D
Acq: 5 Mar 2019 7:32

Instrument :
BNA_G
ClientSampleId :

Tgt Ion:	136	Resp:	182132
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.1	13.7
54	12.4	9.4	14.2
68	5.0	4.2	6.4

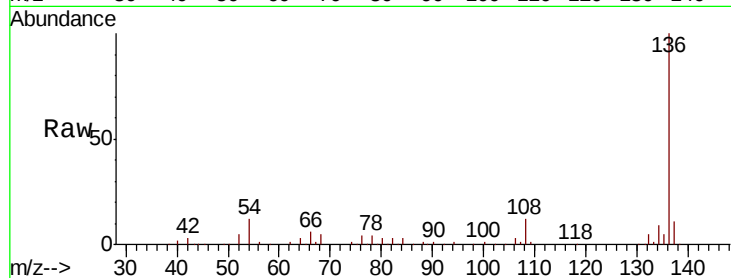


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

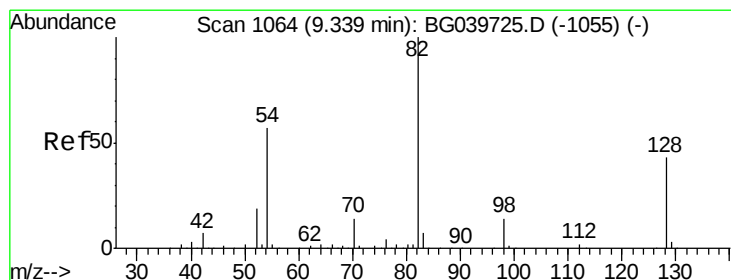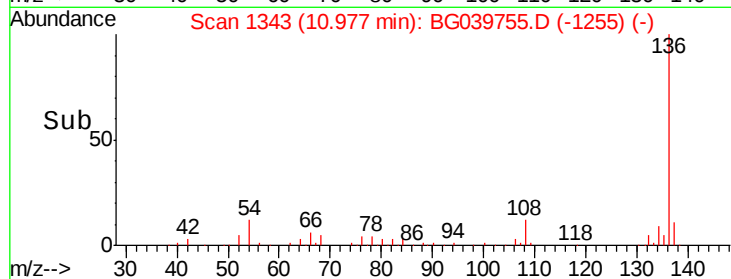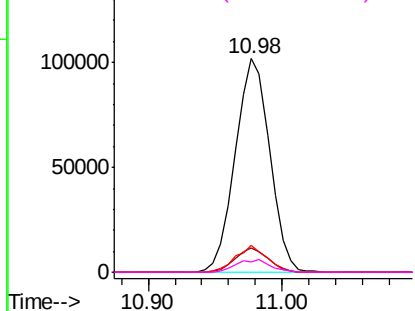

#23
Nitrobenzene-d5
Concen: 91.730 ng
RT: 9.33 min Scan# 1063
Delta R.T. -0.01 min
Lab File: BG039755.D
Acq: 5 Mar 2019 7:32

Tgt Ion:	82	Resp:	308907
Ion	Ratio	Lower	Upper
82	100		
128	43.5	31.3	46.9
54	59.4	50.9	76.3

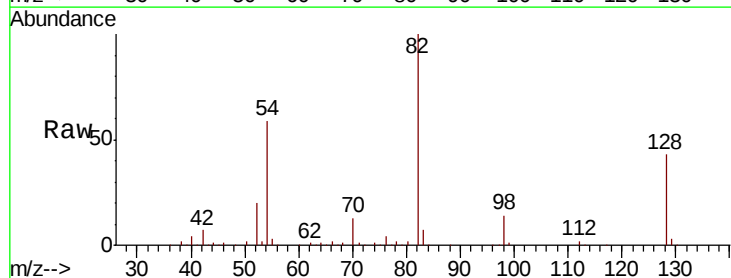

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

