
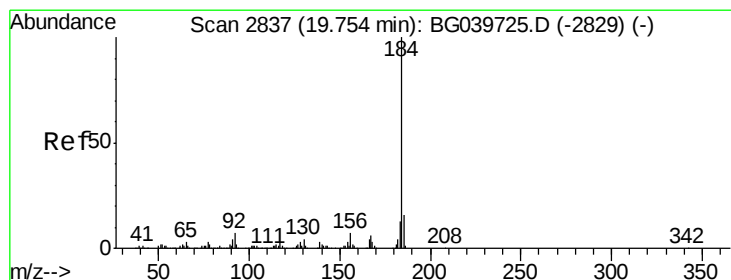
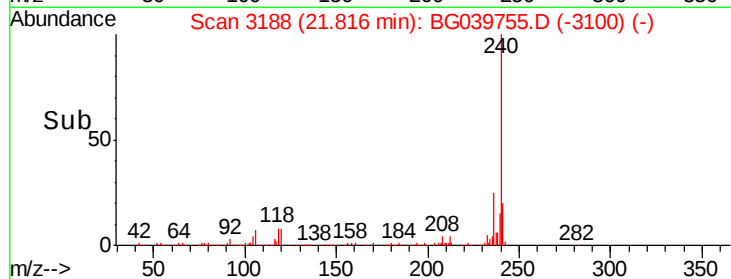
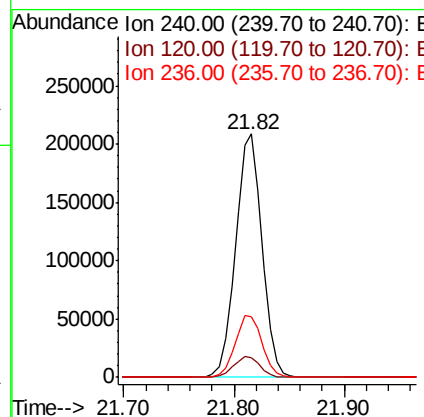


#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.82 min Scan# 3188
 Delta R.T. -0.01 min
 Lab File: BG039755.D
 Acq: 5 Mar 2019 7:32

Instrument :
 BNA_G
 ClientSampled :

Tgt Ion: 240 Resp: 348398
 Ion Ratio Lower Upper
 240 100
 120 8.3 7.0 10.6
 236 25.1 21.0 31.4

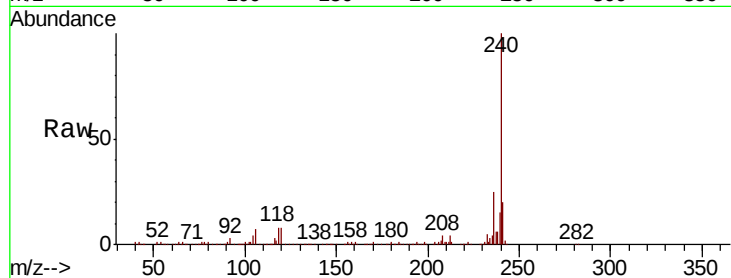

#77
 Benzidine
 Concen: 2.267 ng
 RT: 20.12 min Scan# 2899
 Delta R.T. 0.36 min
 Lab File: BG039755.D
 Acq: 5 Mar 2019 7:32

Tgt Ion: 184 Resp: 25059
 Ion Ratio Lower Upper
 184 100
 185 15.9 12.2 18.2
 183 9.3 10.6 15.8#

