
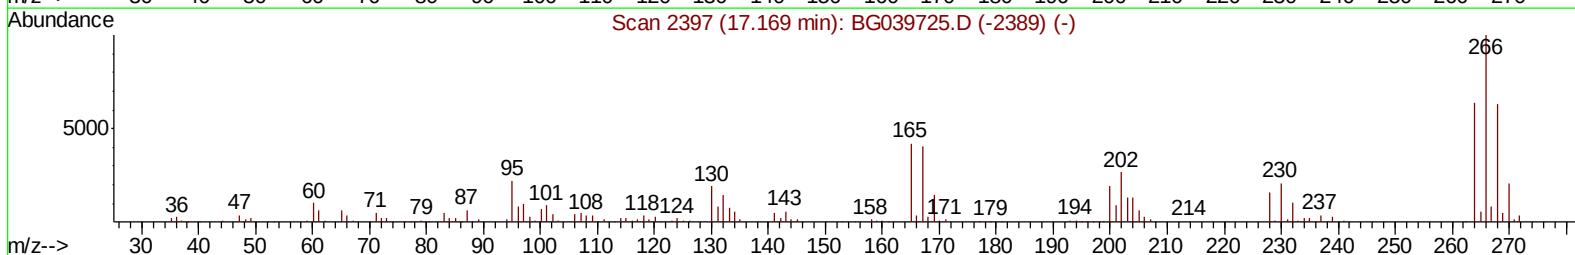
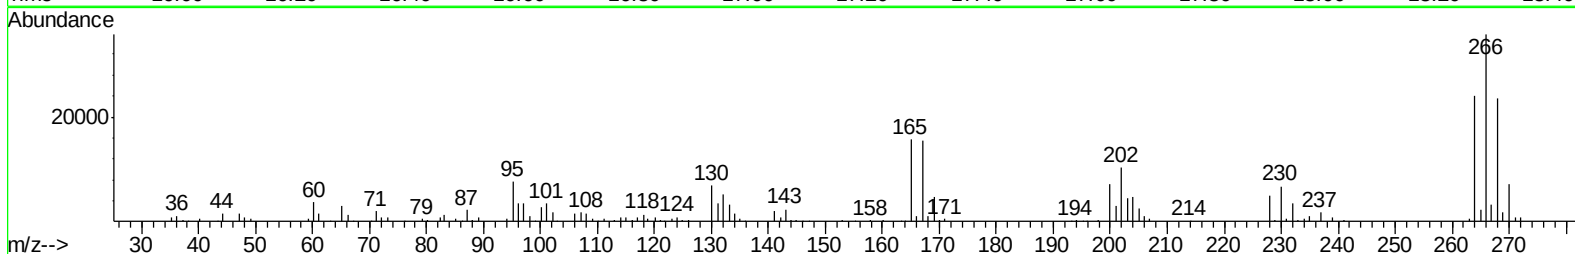


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030419\
Data File : BG039722.D
Acq On : 4 Mar 2019 9:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:49:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

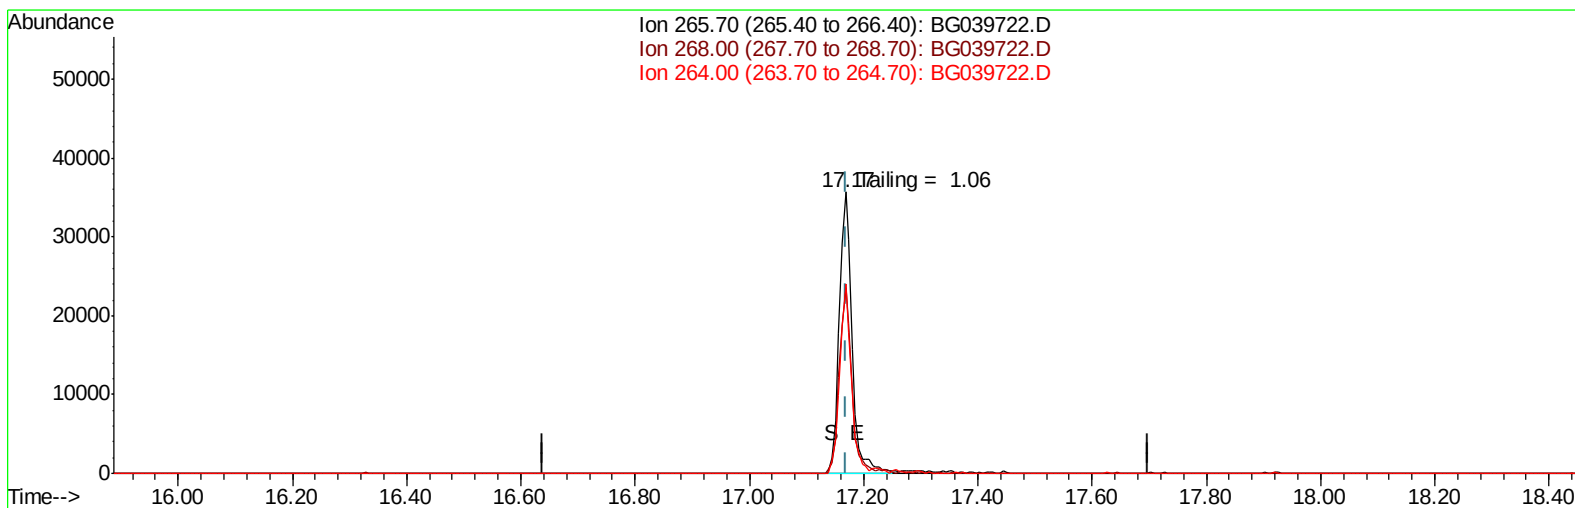

TIC: BG039722.D

(70) Pentachlorophenol (C)




17.168min (-0.002) 90309.86ng

response 55588

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.99
264.00	65.10	67.50
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030419\
Data File : BG039722.D
Acq On : 4 Mar 2019 9:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:49:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

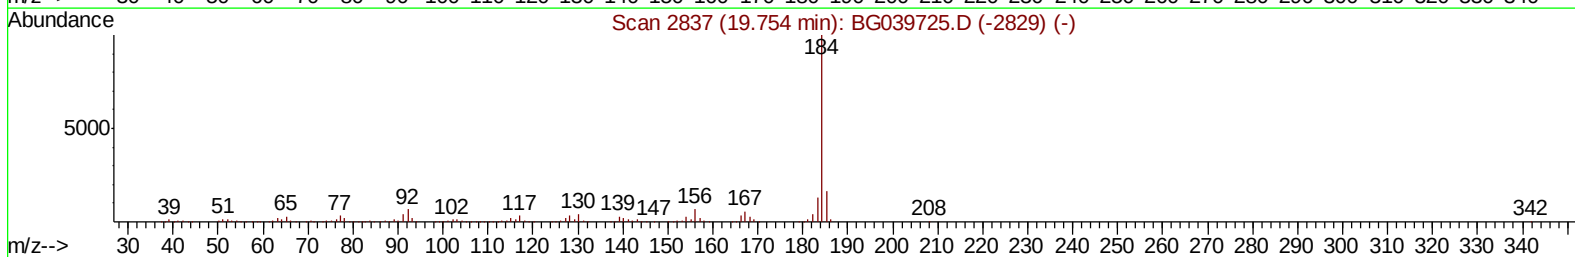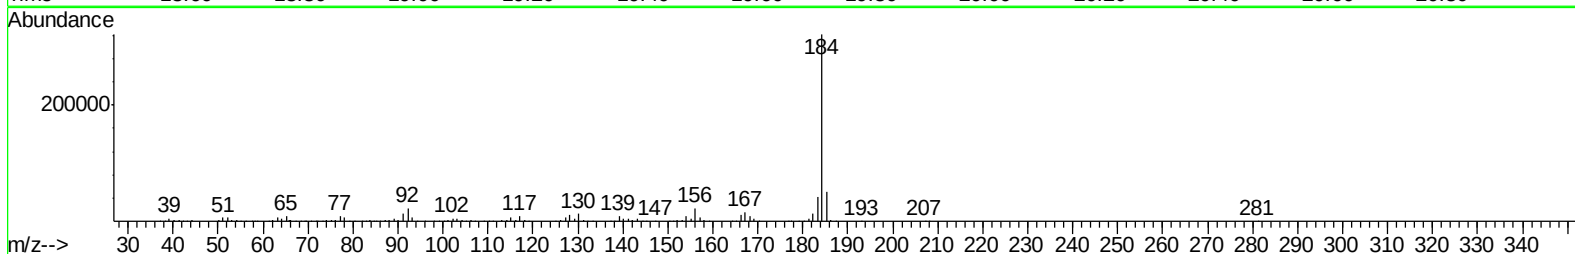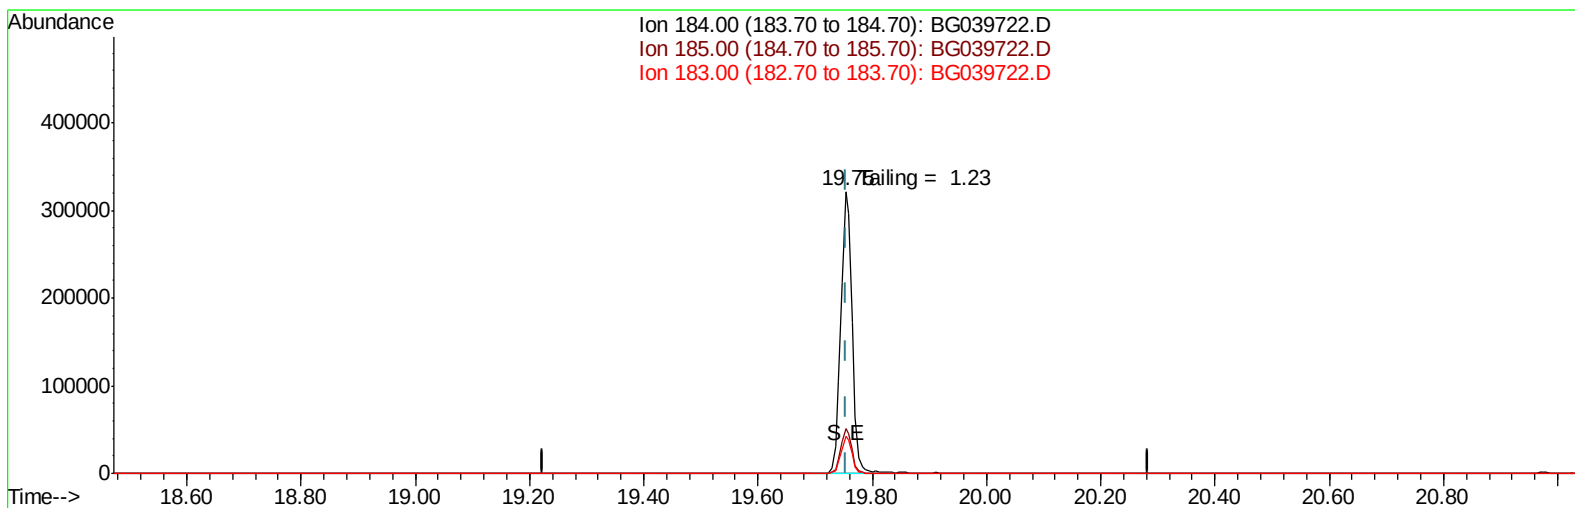

TIC: BG039722.D

(77) Benzidine

19.753min (-0.002) 191768.15ng

response 444232

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.88
183.00	13.20	13.06
0.00	0.00	0.00