
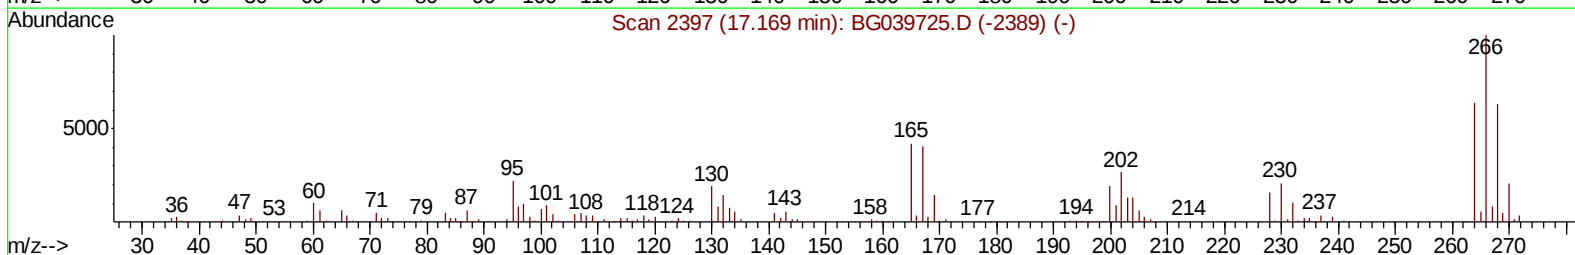
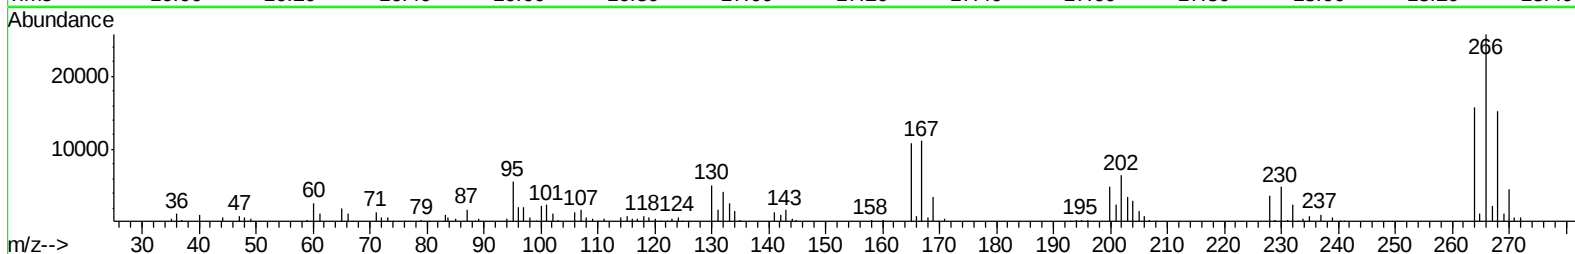


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG030419\  
Data File : BG039731.D  
Acq On : 4 Mar 2019 14:55  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:50:29 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG030419.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 04 14:38:15 2019  
Response via : Initial Calibration

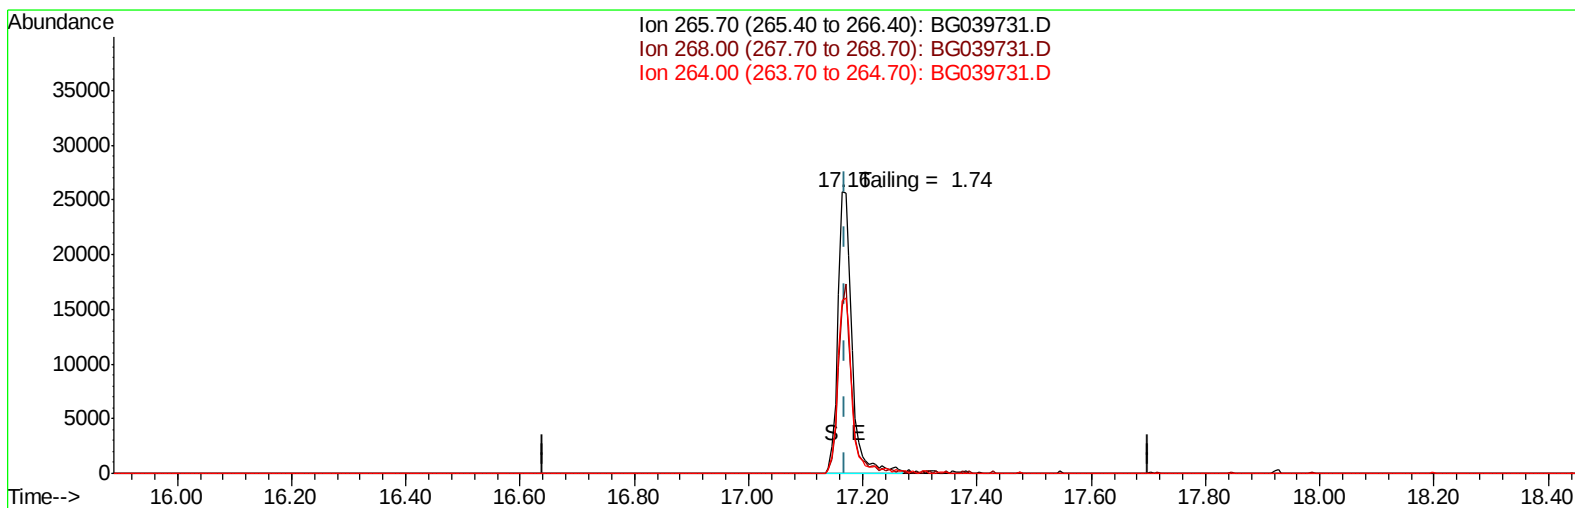

TIC: BG039731.D

(70) Pentachlorophenol (C)




17.163min (-0.006) 42947.13ng

response 43429

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 58.89 |
| 264.00 | 65.10 | 61.21 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG030419\  
 Data File : BG039731.D  
 Acq On : 4 Mar 2019 14:55  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:50:29 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG030419.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Mar 04 14:38:15 2019  
 Response via : Initial Calibration

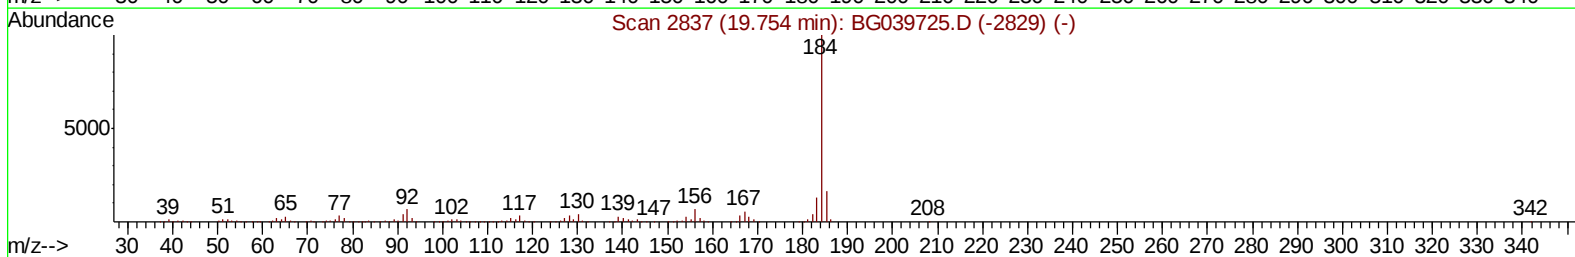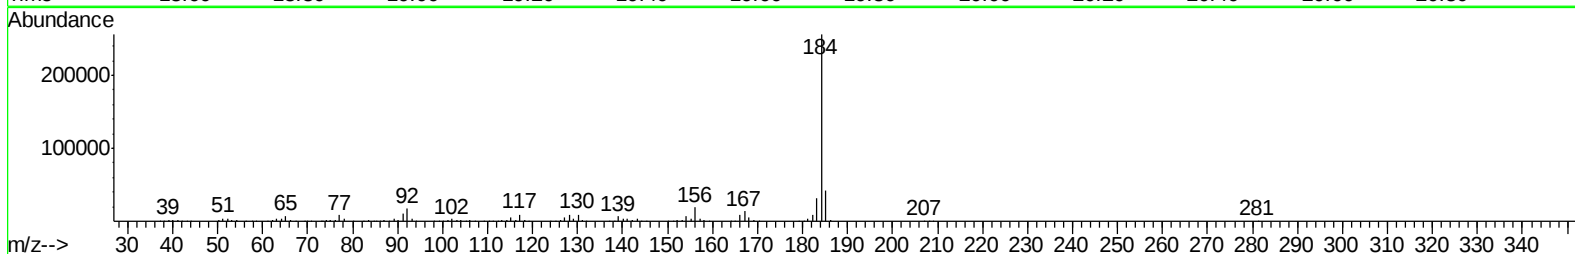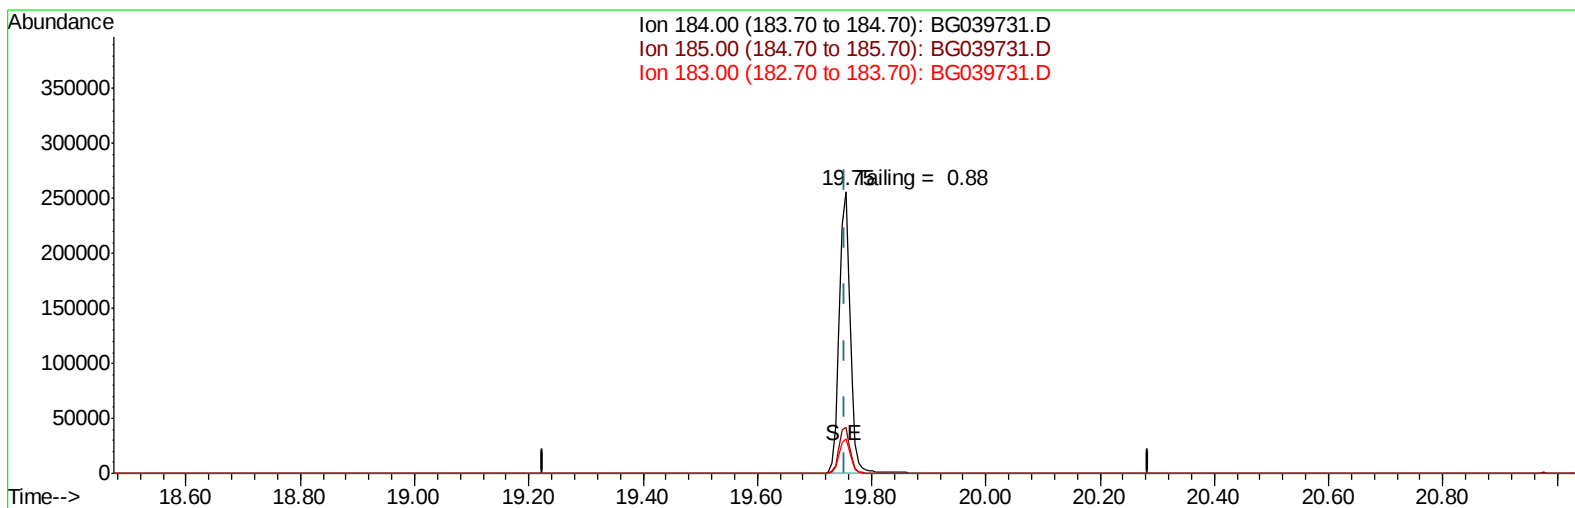

TIC: BG039731.D

(77) Benzidine

19.754min (-0.000) 20843.39ng

response 344601

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.20 | 16.40 |
| 183.00 | 13.20 | 12.48 |
| 0.00   | 0.00  | 0.00  |