
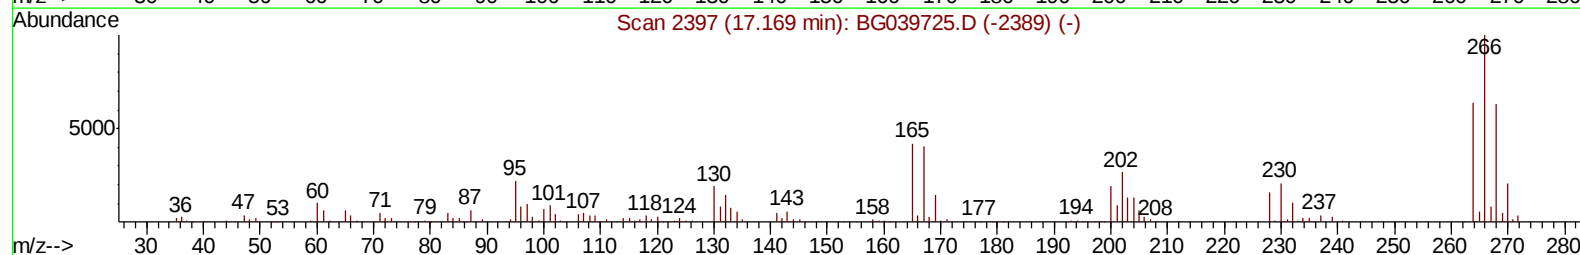
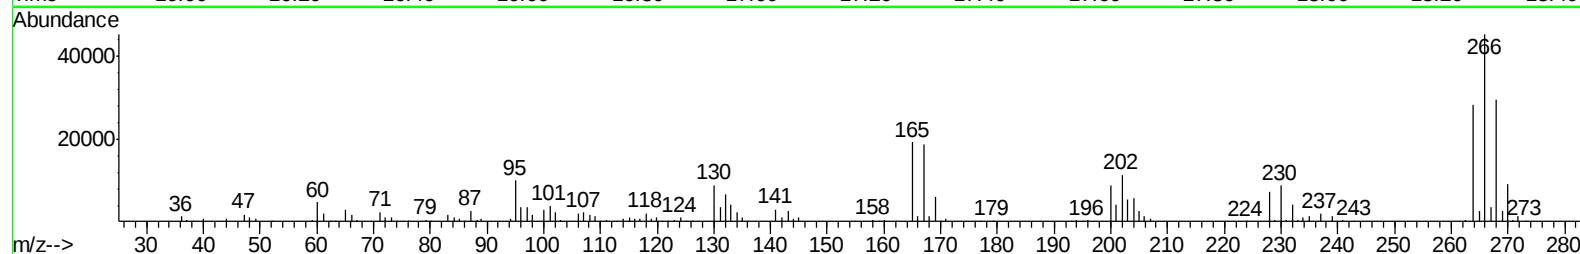


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030419\
Data File : BG039750.D
Acq On : 5 Mar 2019 4:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:52:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

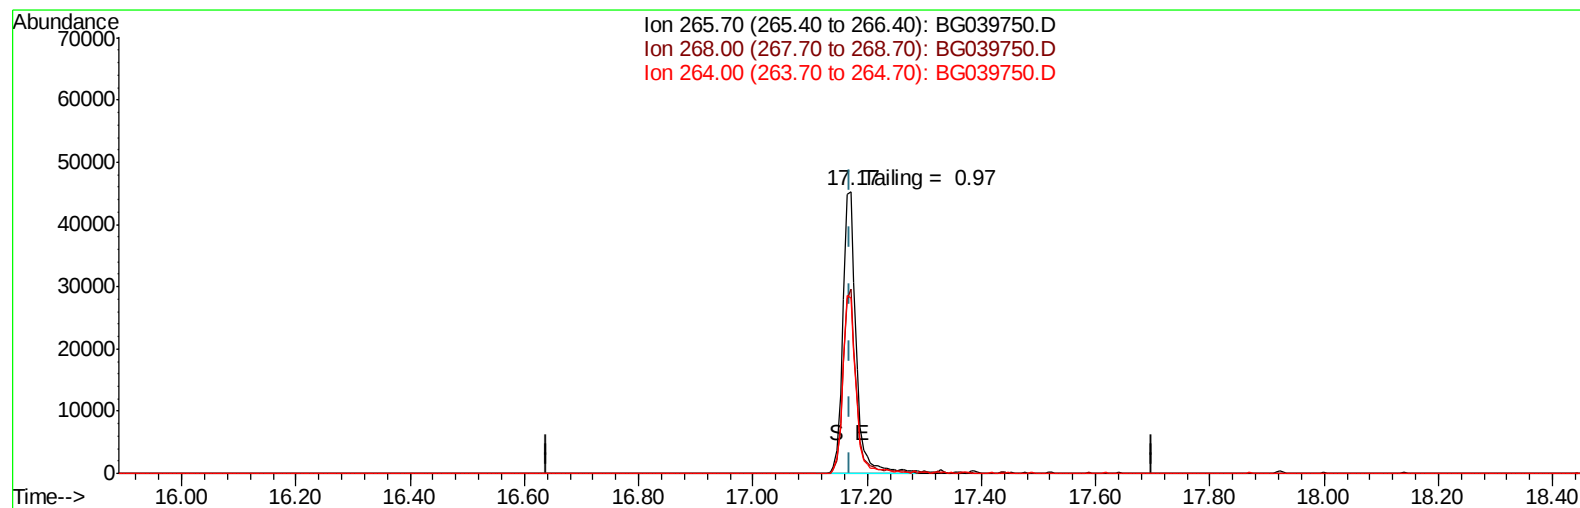

TIC: BG039750.D

(70) Pentachlorophenol (C)




17.171min (+0.001) 26990.62ng

response 72387

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.44
264.00	65.10	62.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030419\
 Data File : BG039750.D
 Acq On : 5 Mar 2019 4:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:52:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

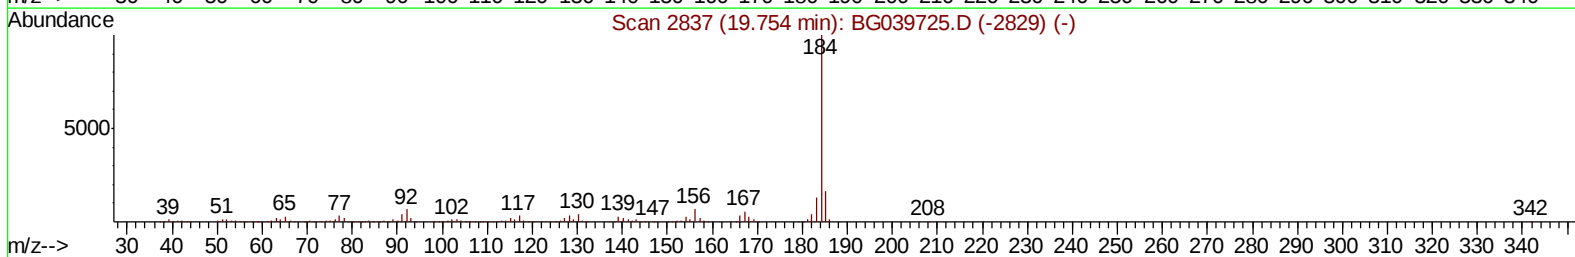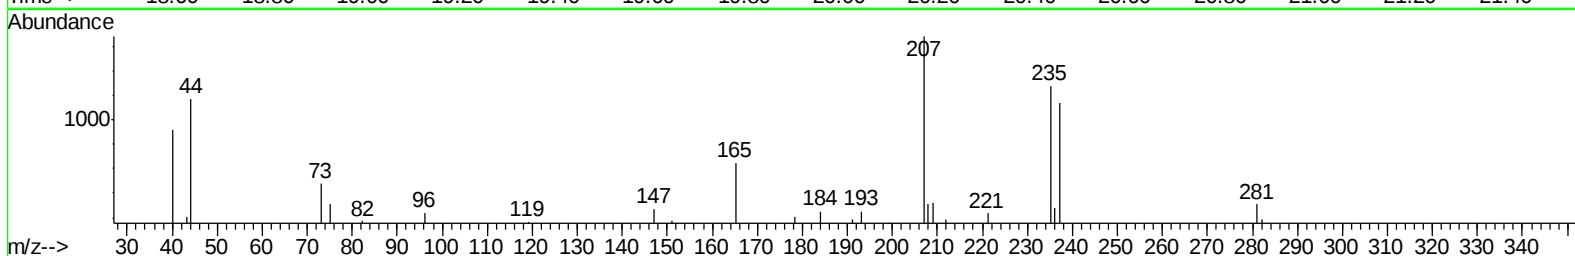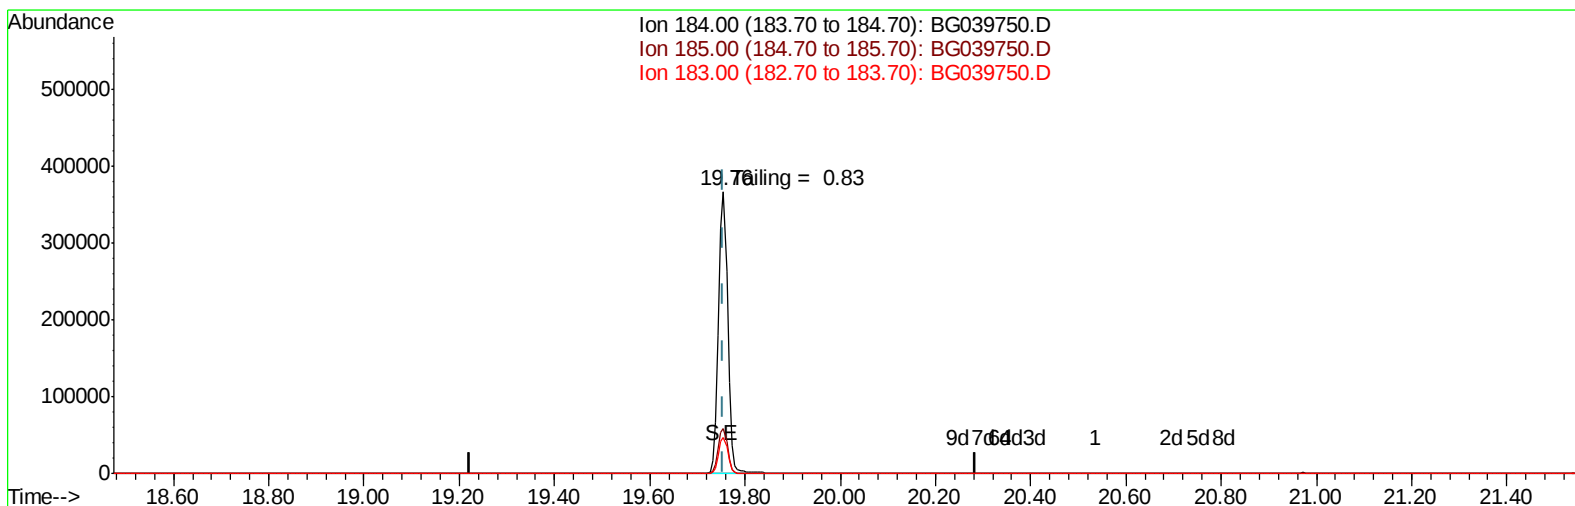

TIC: BG039750.D

(77) Benzidine

20.537min (+0.782) 51.35ng

response 88

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00