


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030419\
 Data File : BG039722.D
 Acq On : 4 Mar 2019 9:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

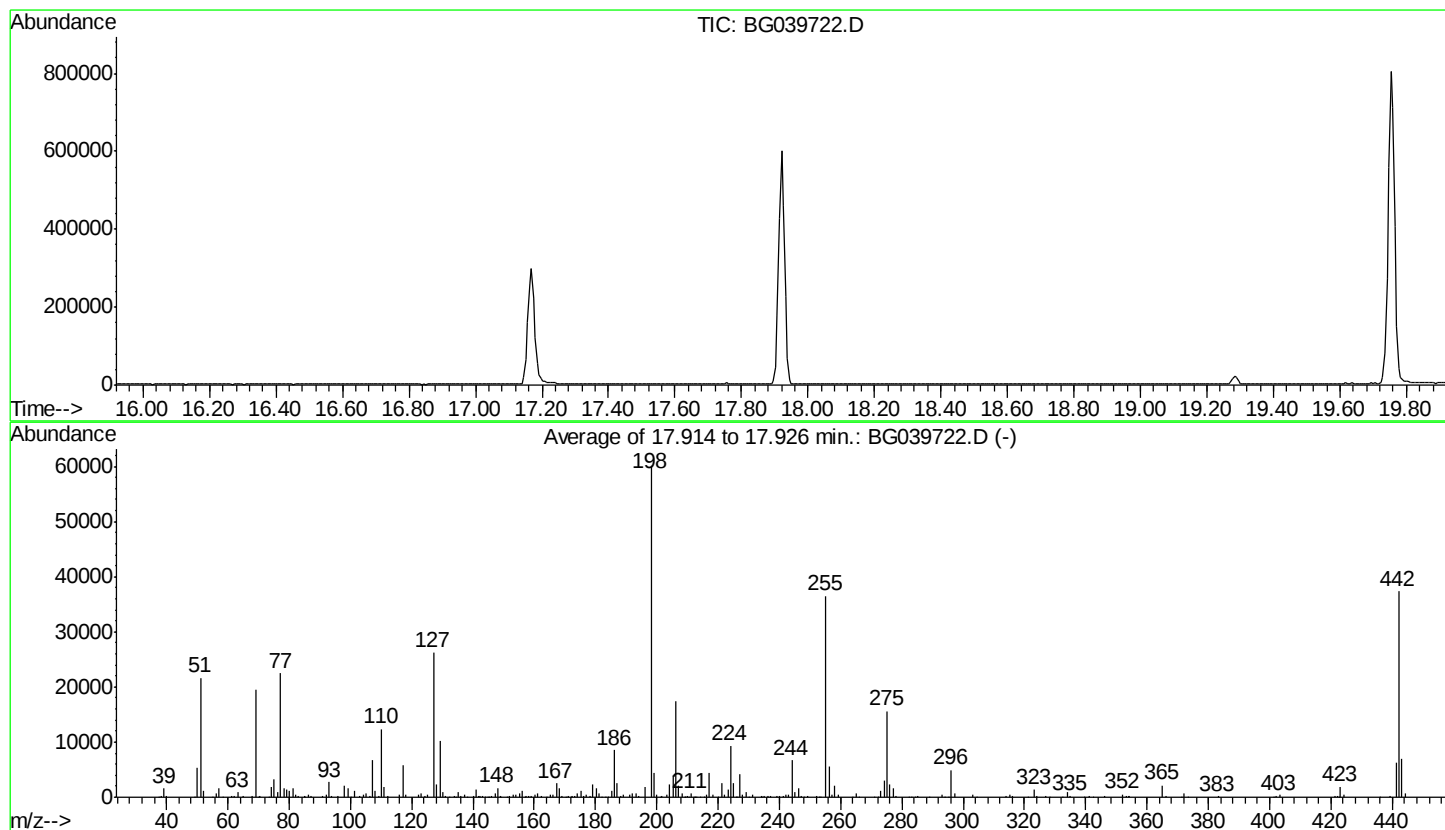

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	21693	PASS
68	69	0.00	2	1.3	253	PASS
69	198	0.00	100	32.3	19439	PASS
70	69	0.00	2	0.8	147	PASS
127	198	10	80	43.5	26149	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60141	PASS
199	198	5	9	7.4	4425	PASS
275	198	10	60	26.0	15658	PASS
365	198	1	100	3.5	2121	PASS
441	198	0.01	100	10.4	6257	PASS
442	198	50	100	62.1	37376	PASS
443	442	15	24	18.5	6928	PASS