


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030419\
 Data File : BG039731.D
 Acq On : 4 Mar 2019 14:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

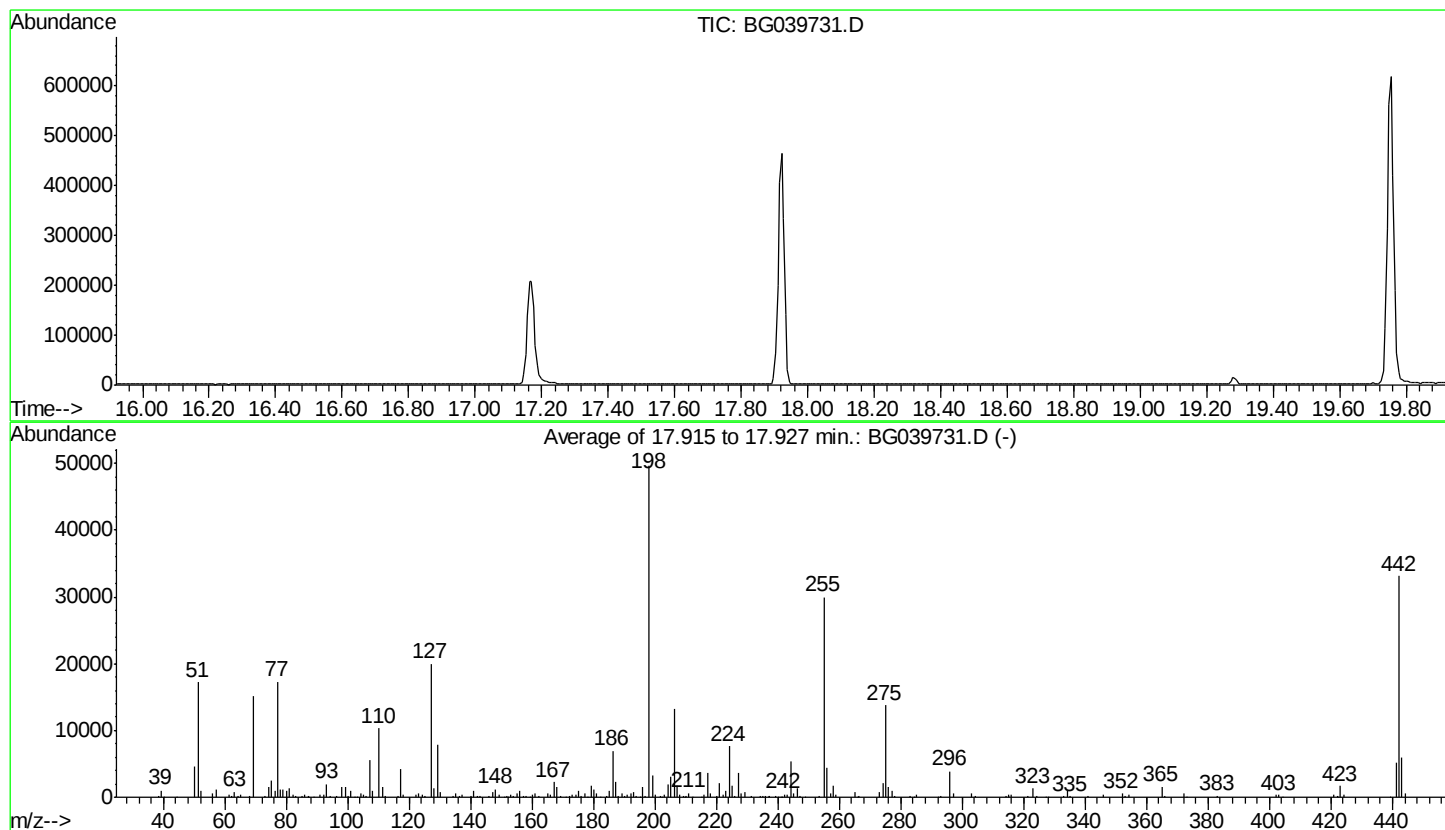

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	17208	PASS
68	69	0.00	2	1.2	176	PASS
69	198	0.00	100	30.3	15063	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.2	19974	PASS
197	198	0.00	2	0.3	144	PASS
198	198	100	100	100.0	49658	PASS
199	198	5	9	6.6	3291	PASS
275	198	10	60	27.7	13739	PASS
365	198	1	100	3.3	1618	PASS
441	198	0.01	100	10.4	5143	PASS
442	198	50	100	66.8	33152	PASS
443	442	15	24	17.7	5874	PASS