


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030419\
 Data File : BG039750.D
 Acq On : 5 Mar 2019 4:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

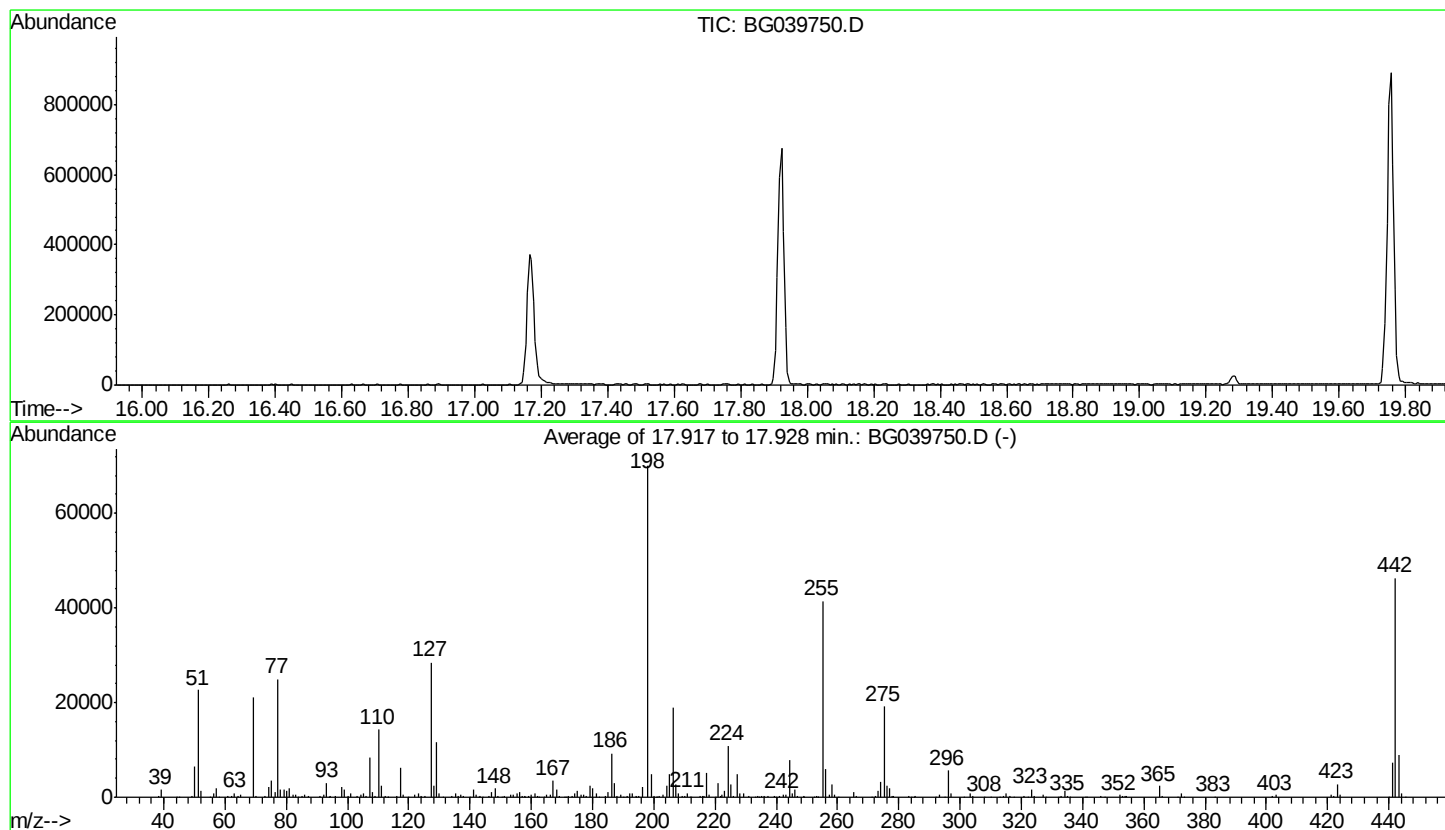

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	22625	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.0	20998	PASS
70	69	0.00	2	0.8	172	PASS
127	198	10	80	40.6	28450	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70093	PASS
199	198	5	9	7.0	4925	PASS
275	198	10	60	27.4	19192	PASS
365	198	1	100	3.4	2391	PASS
441	198	0.01	100	10.4	7317	PASS
442	198	50	100	66.2	46370	PASS
443	442	15	24	19.1	8875	PASS