
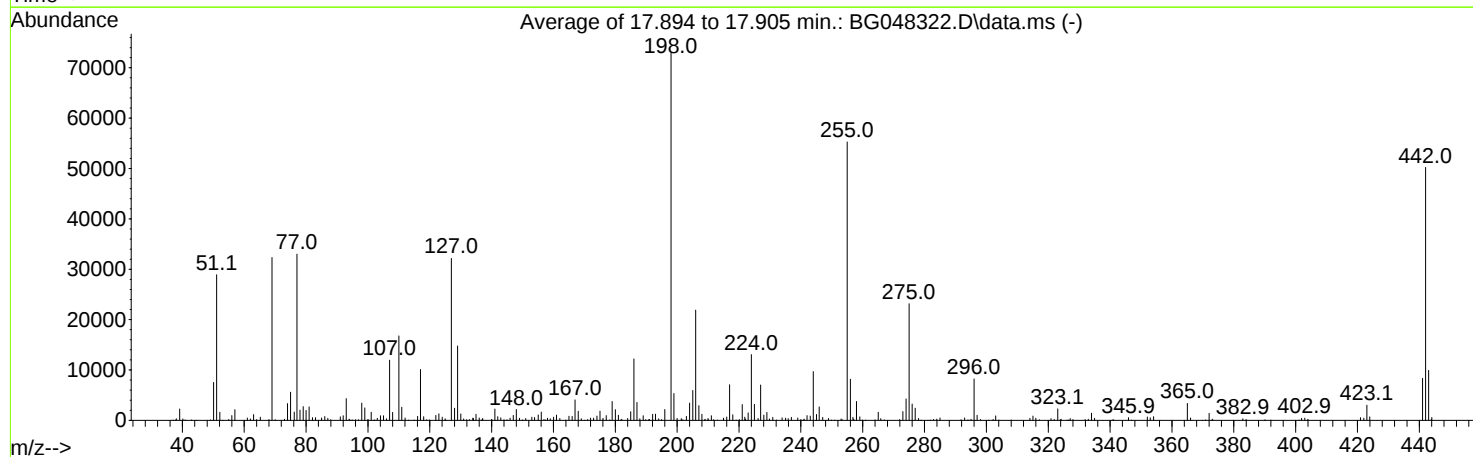


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030421\
 Data File : BG048322.D
 Acq On : 4 Mar 2021 8:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 03 16:40:27 2021

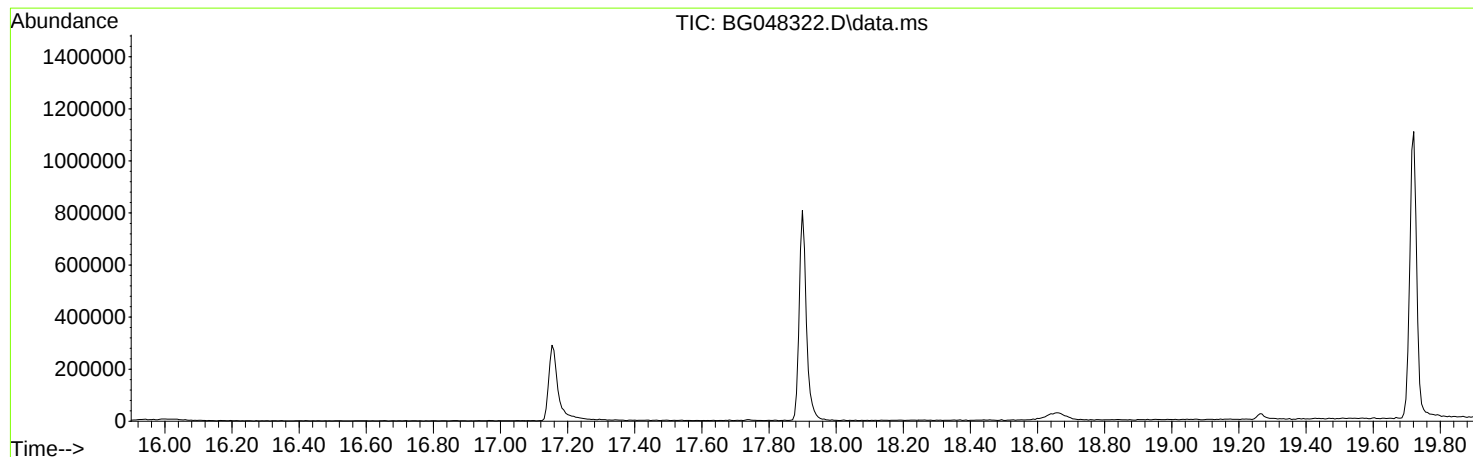

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	28915	PASS
68	69	0.00	2	0.5	149	PASS
69	198	0.00	100	44.3	32325	PASS
70	69	0.00	2	0.4	137	PASS
127	198	10	80	44.0	32155	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73032	PASS
199	198	5	9	7.3	5346	PASS
275	198	10	60	31.7	23168	PASS
365	198	1	100	4.6	3381	PASS
441	198	0.01	100	11.4	8343	PASS
442	198	50	100	68.8	50211	PASS
443	442	15	24	19.8	9924	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/4/2021	BNA_G	<u>BG048322.D</u>
Compound Name	Response	Retention Time
DDT	374689	20.93
DDD	1173	20.5
DDE	525	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1698	376387	0.45

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030421\
Data File : BG048322.D
Acq On : 4 Mar 2021 8:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 04 09:47:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 03 16:40:27 2021
Response via : Initial Calibration

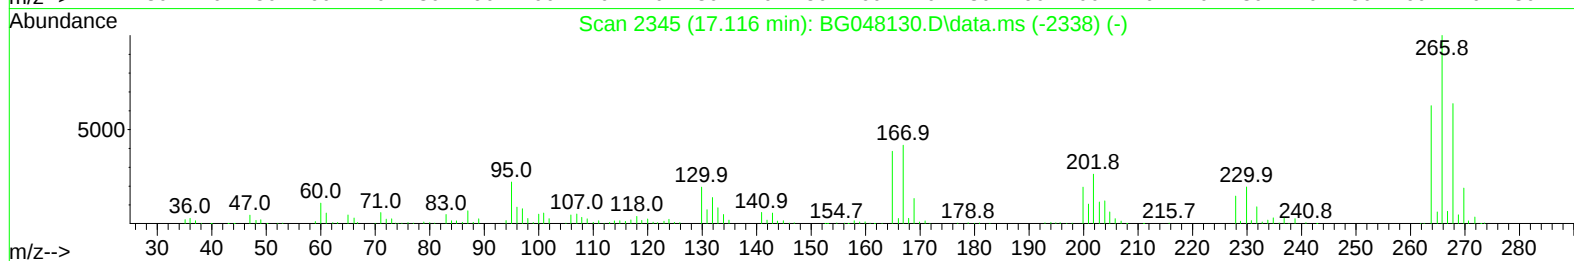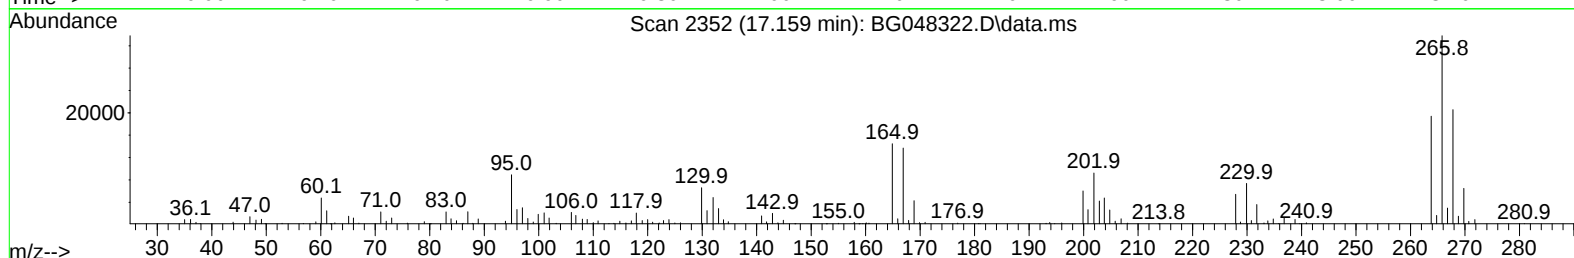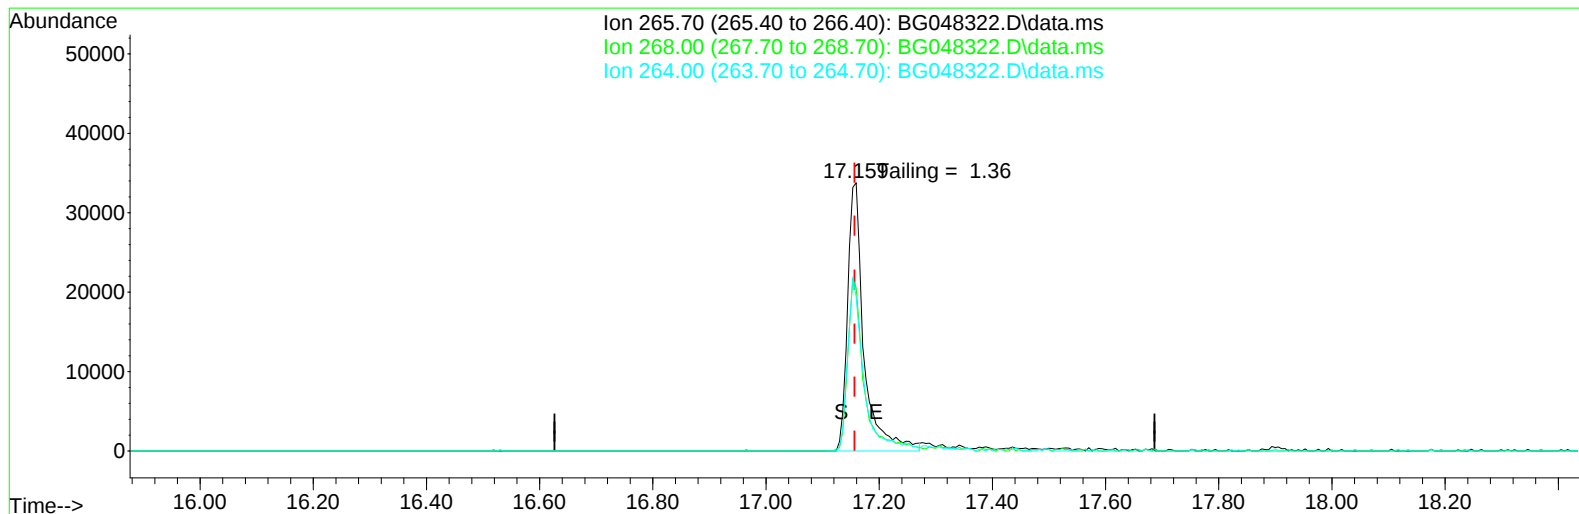

TIC: BG048322.D\data.ms

(70) Pentachlorophenol (C)

17.159min (+ 0.003) 16337.95 ng




response 67219

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.89
264.00	61.60	57.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030421\
Data File : BG048322.D
Acq On : 4 Mar 2021 8:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 04 09:47:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 03 16:40:27 2021
Response via : Initial Calibration

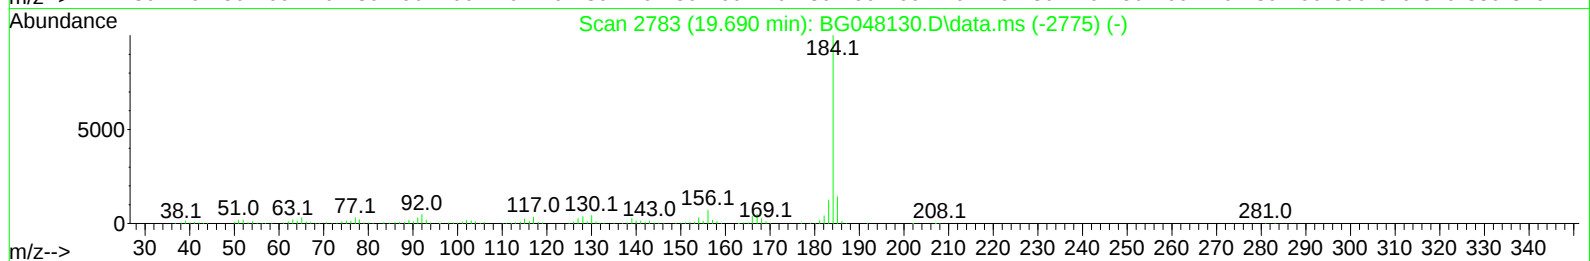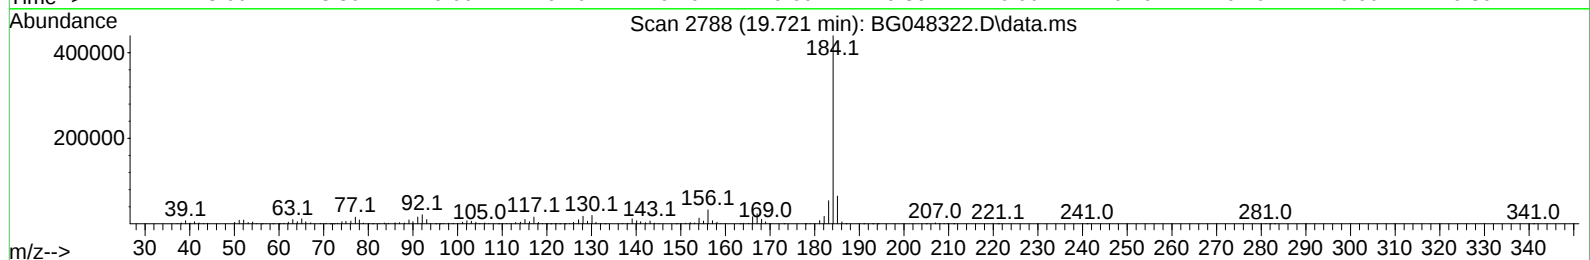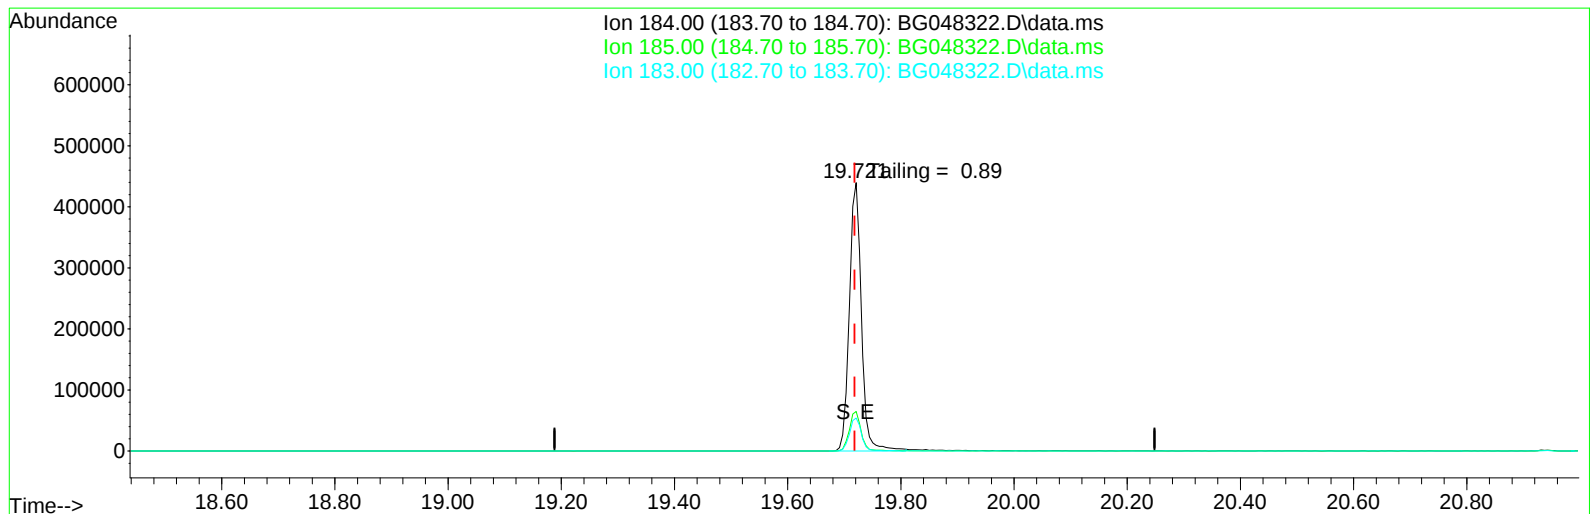

TIC: BG048322.D\data.ms

(77) Benzidine

19.721min (+ 0.003) 267348.27 ng

response 655157

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.77
183.00	13.20	12.32
0.00	0.00	0.00