




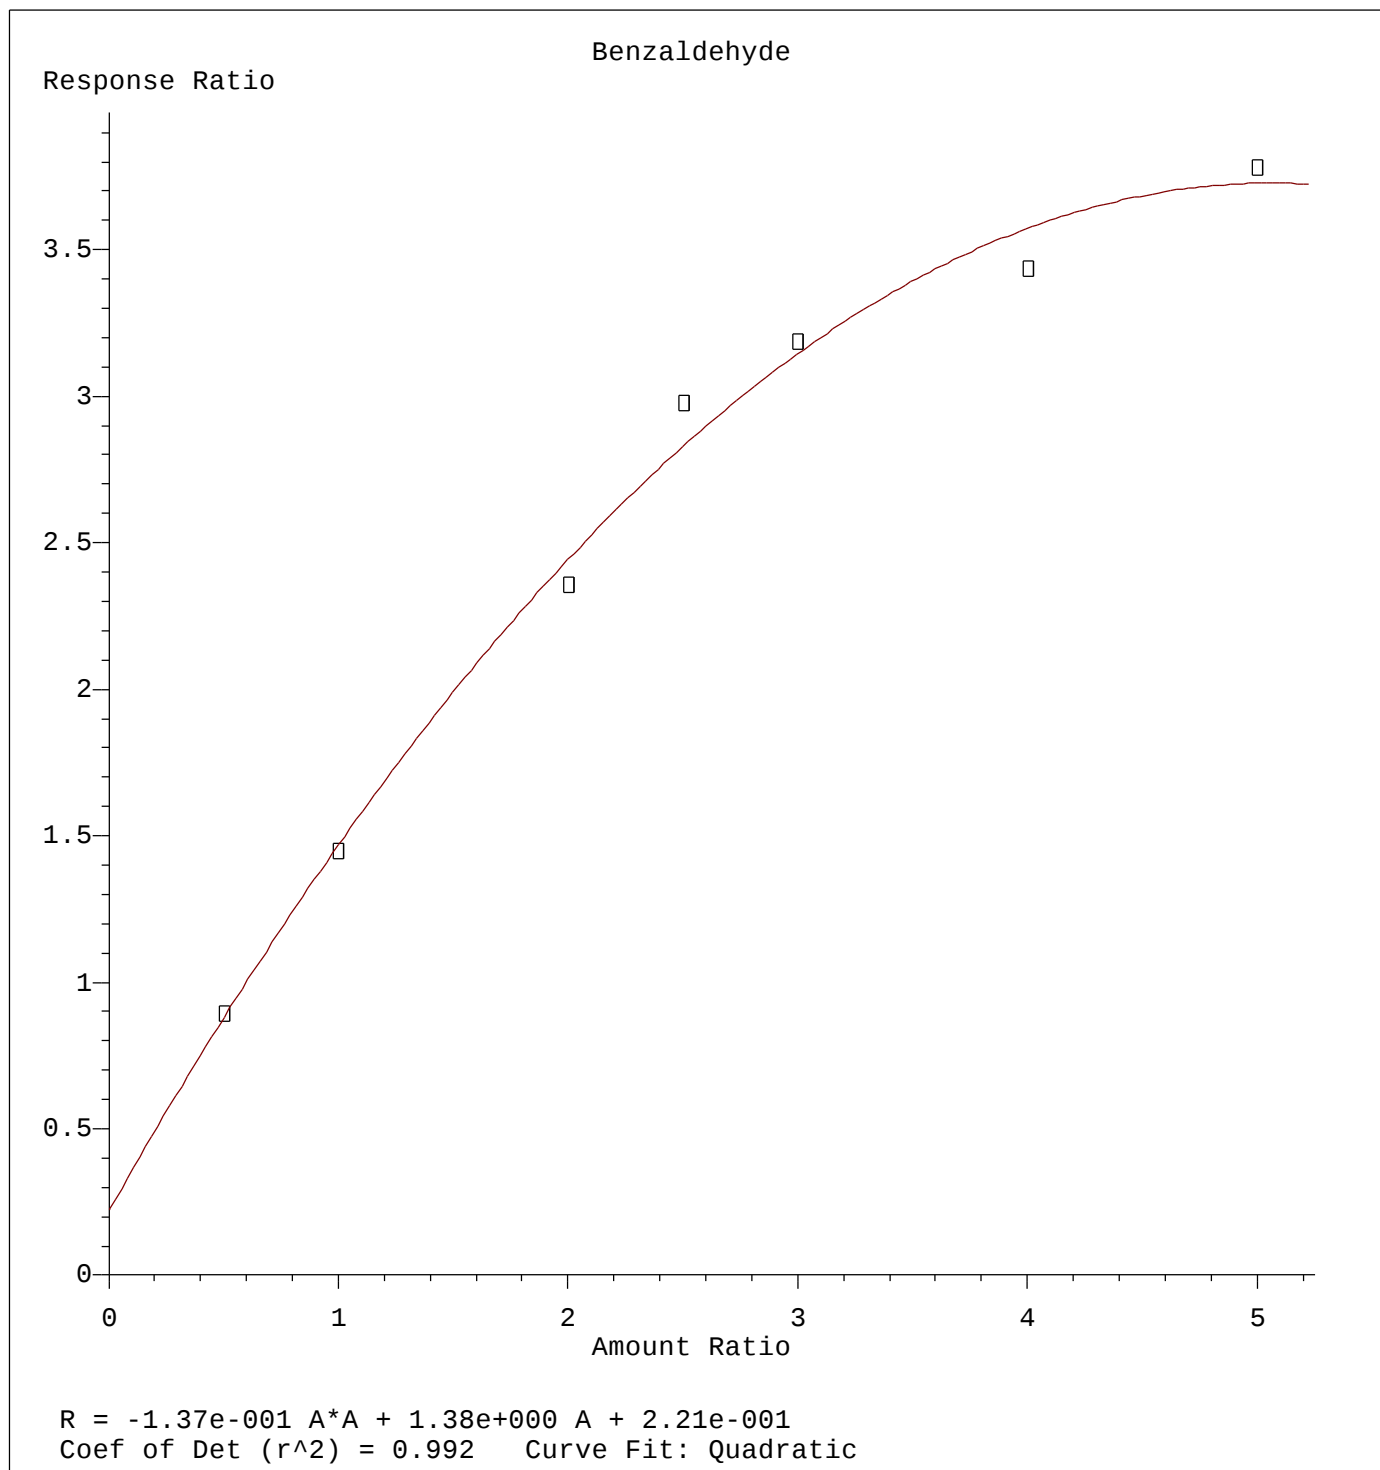

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030520.M
Calibration Table Last Updated: Thu Mar 05 17:42:35 2020

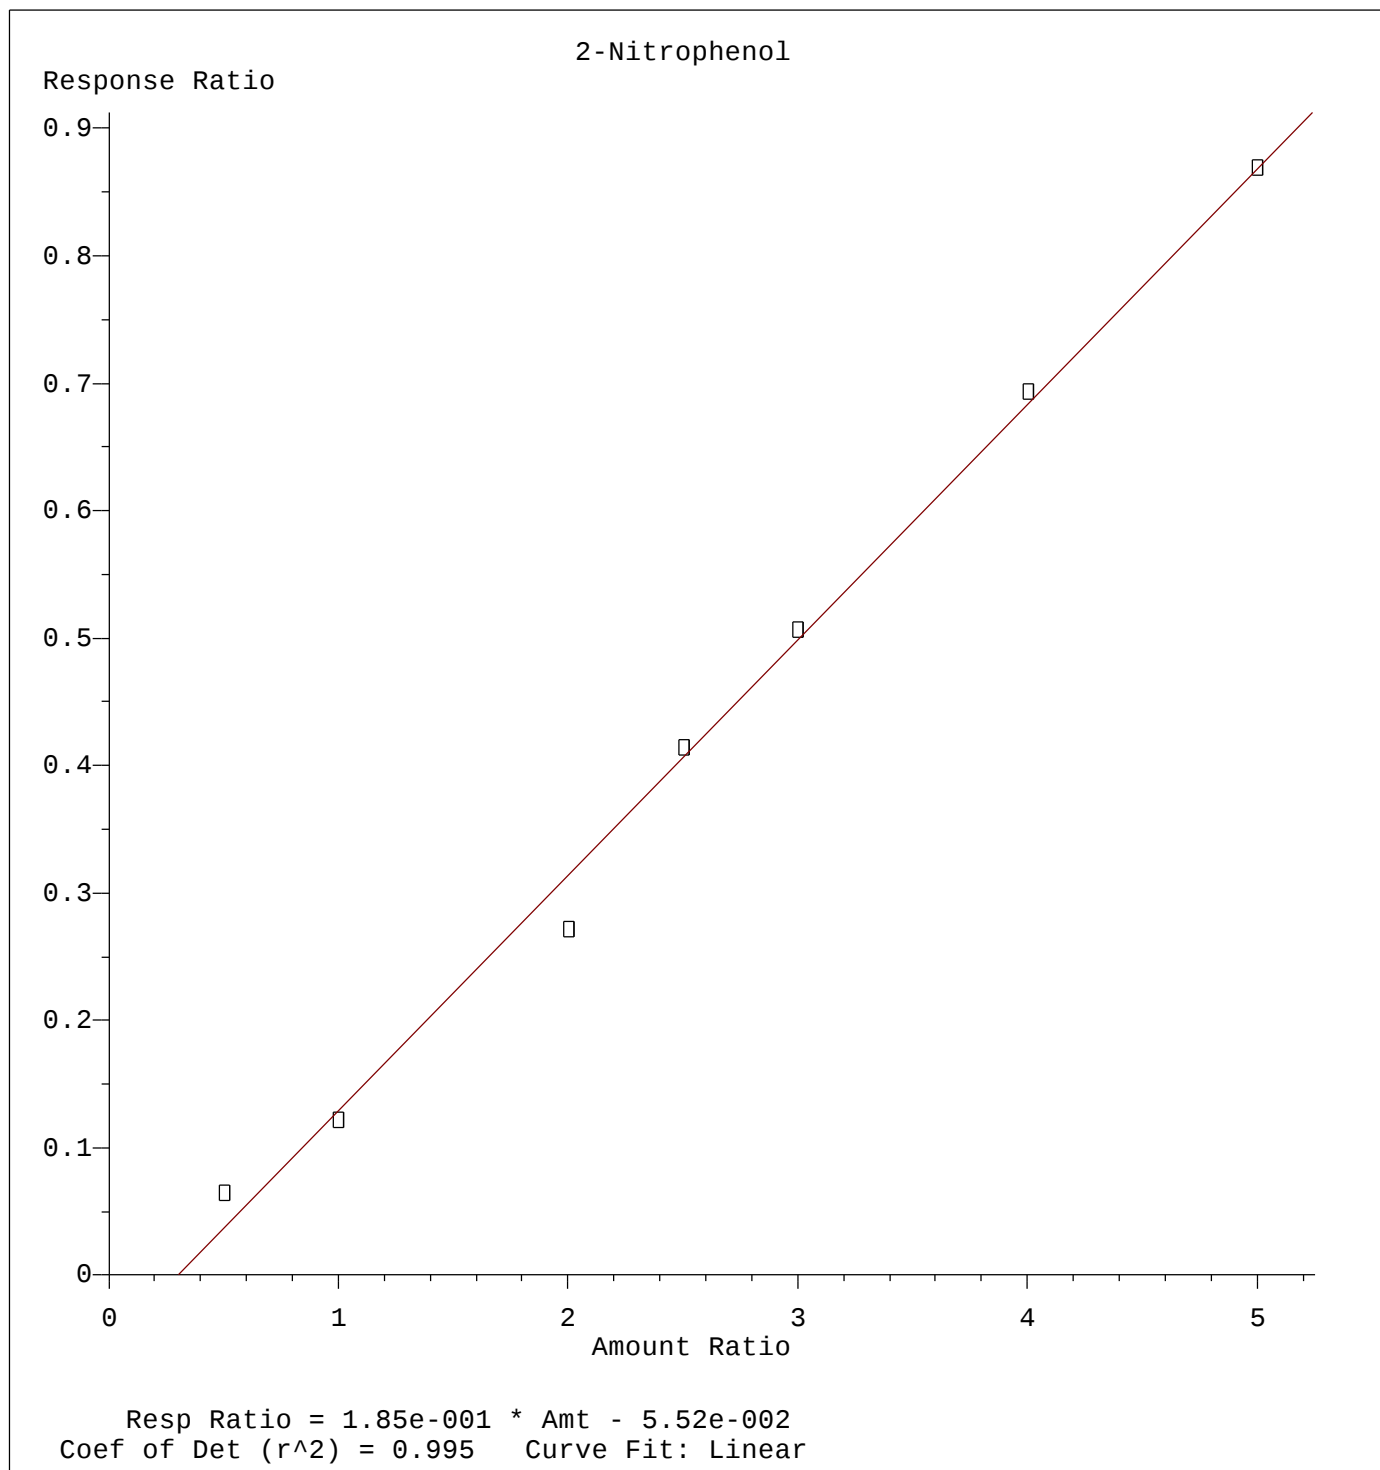


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030520.M
Calibration Table Last Updated: Thu Mar 05 17:42:35 2020

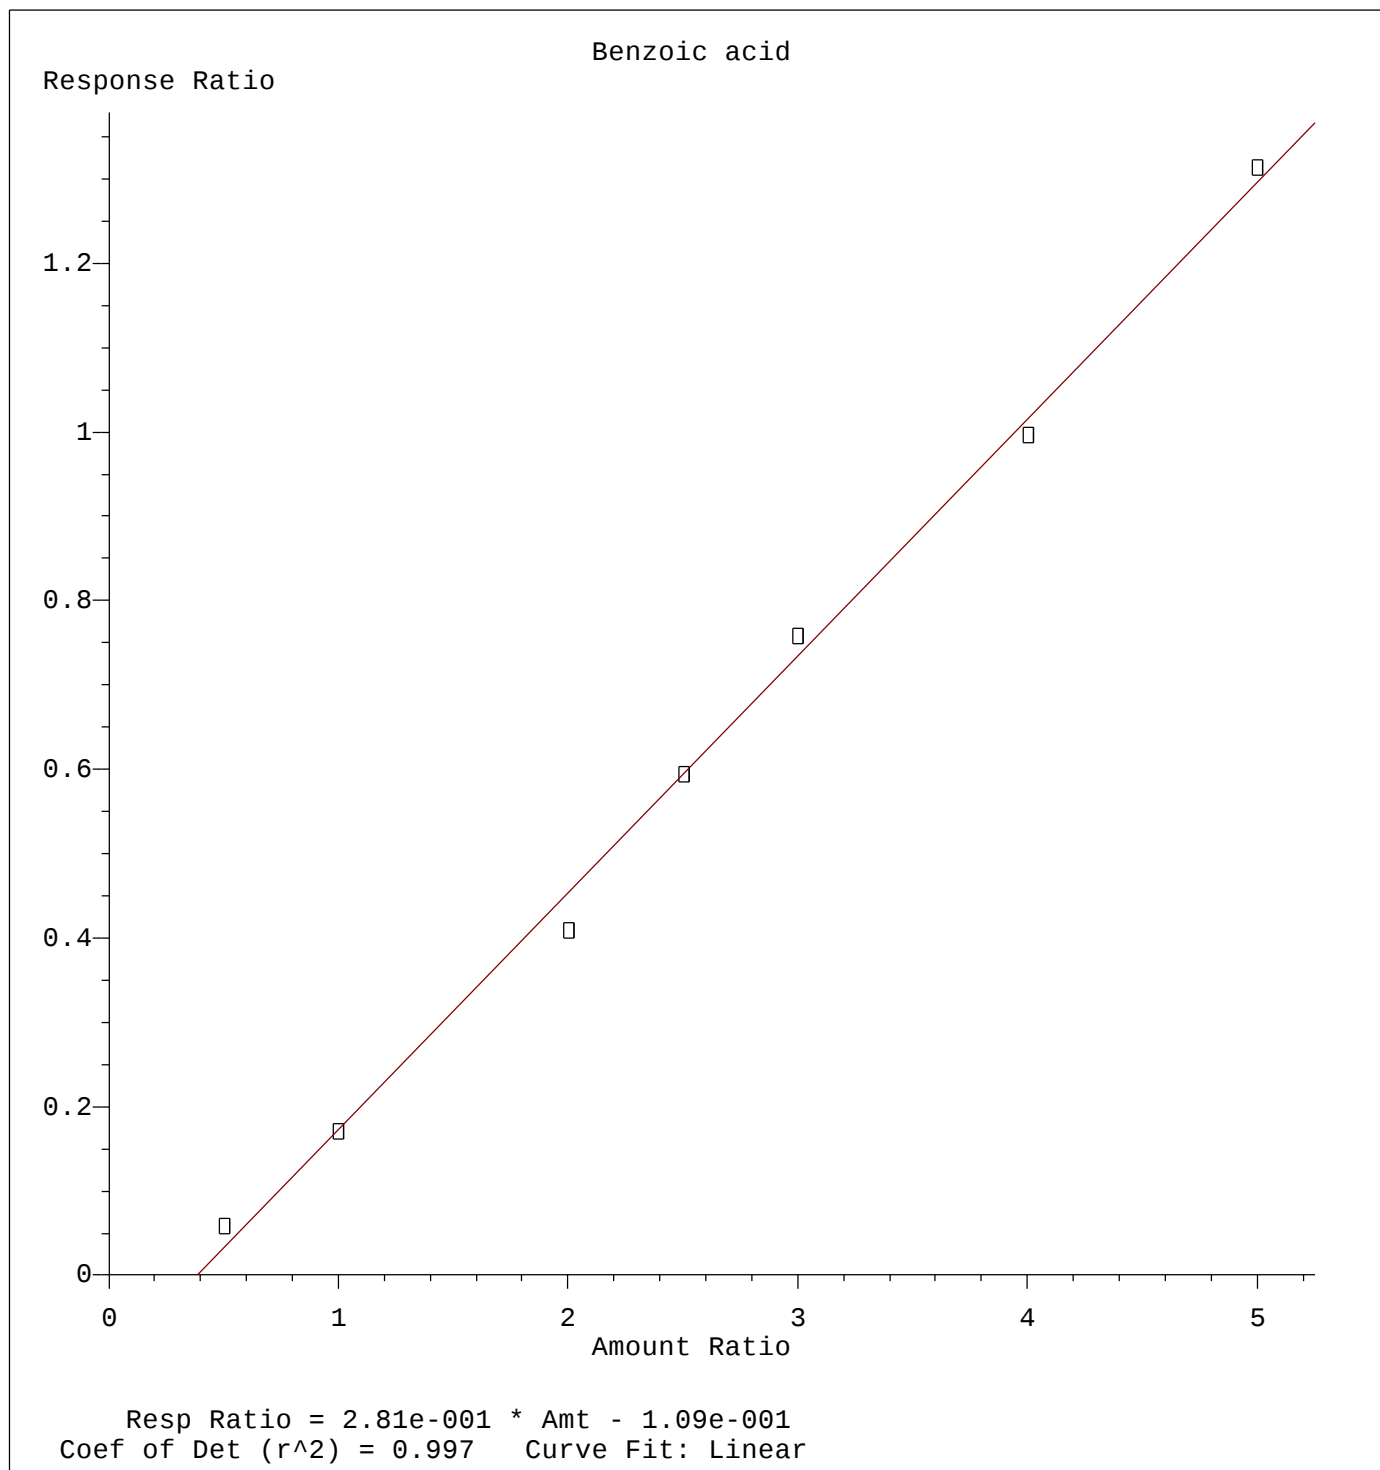

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030520.M
Calibration Table Last Updated: Thu Mar 05 17:42:35 2020

2-Nitroaniline

Response Ratio

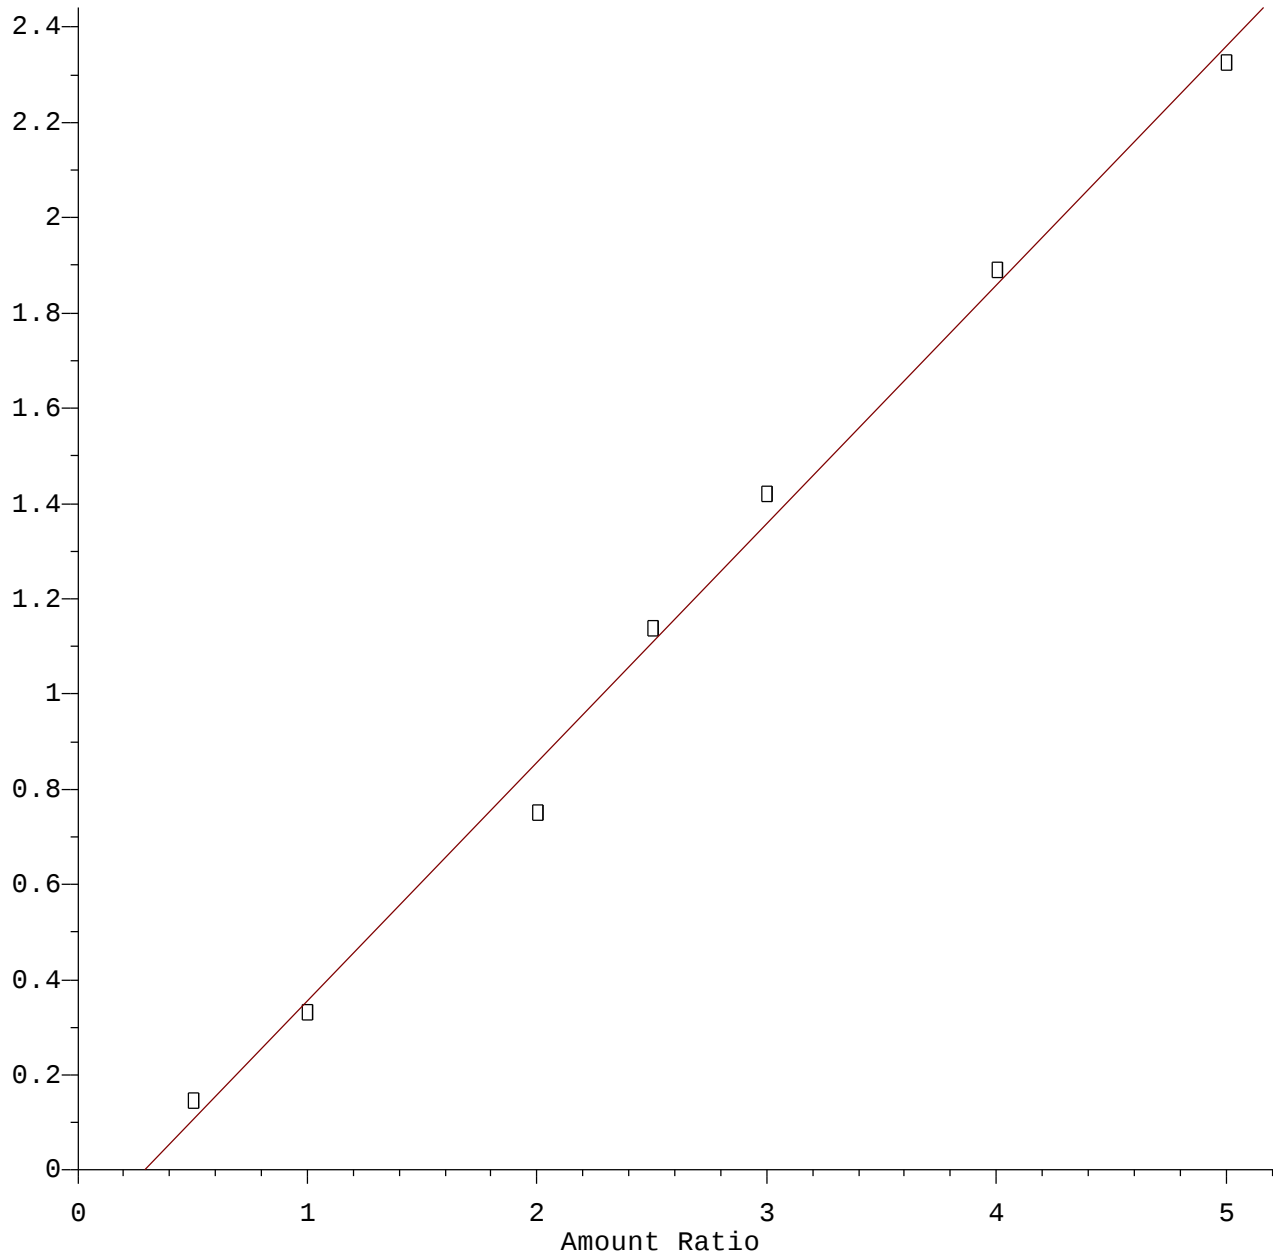


Resp Ratio = $5.01 \times 10^{-1} \times \text{Amt} - 1.45 \times 10^{-1}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030520.M
Calibration Table Last Updated: Thu Mar 05 17:42:35 2020

2,4-Dinitrophenol

Response Ratio

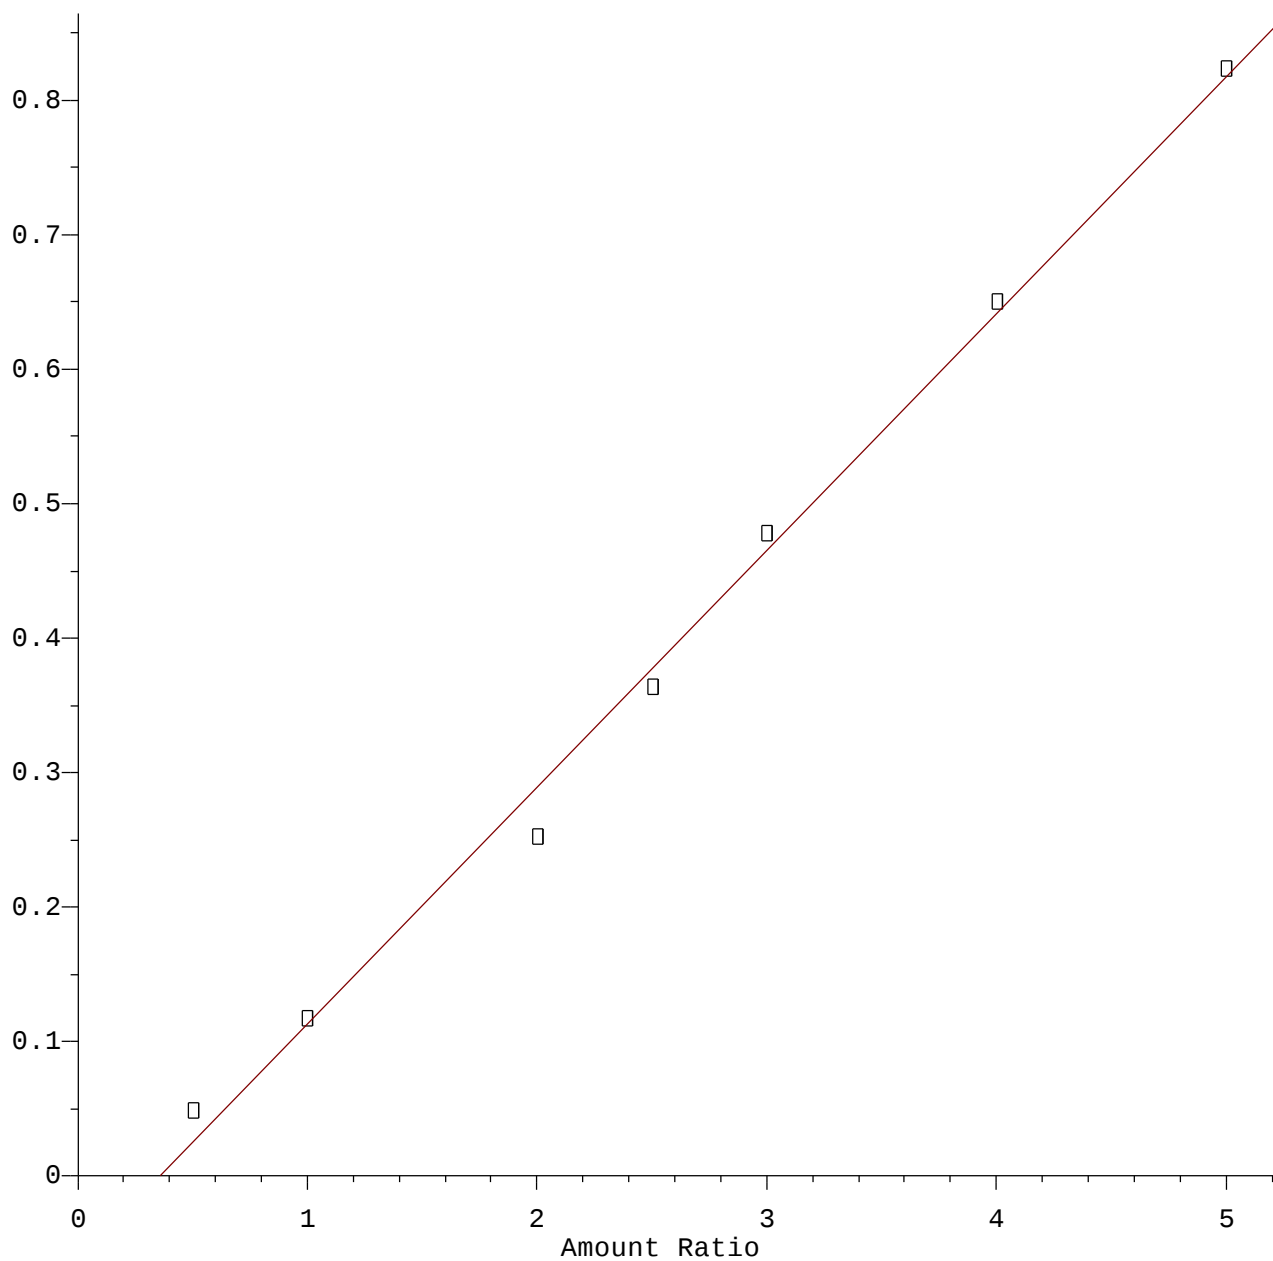


Resp Ratio = $1.76 \times 10^{-1} \times \text{Amt} - 6.23 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030520.M
Calibration Table Last Updated: Thu Mar 05 17:42:35 2020

2,4-Dinitrotoluene


Response Ratio

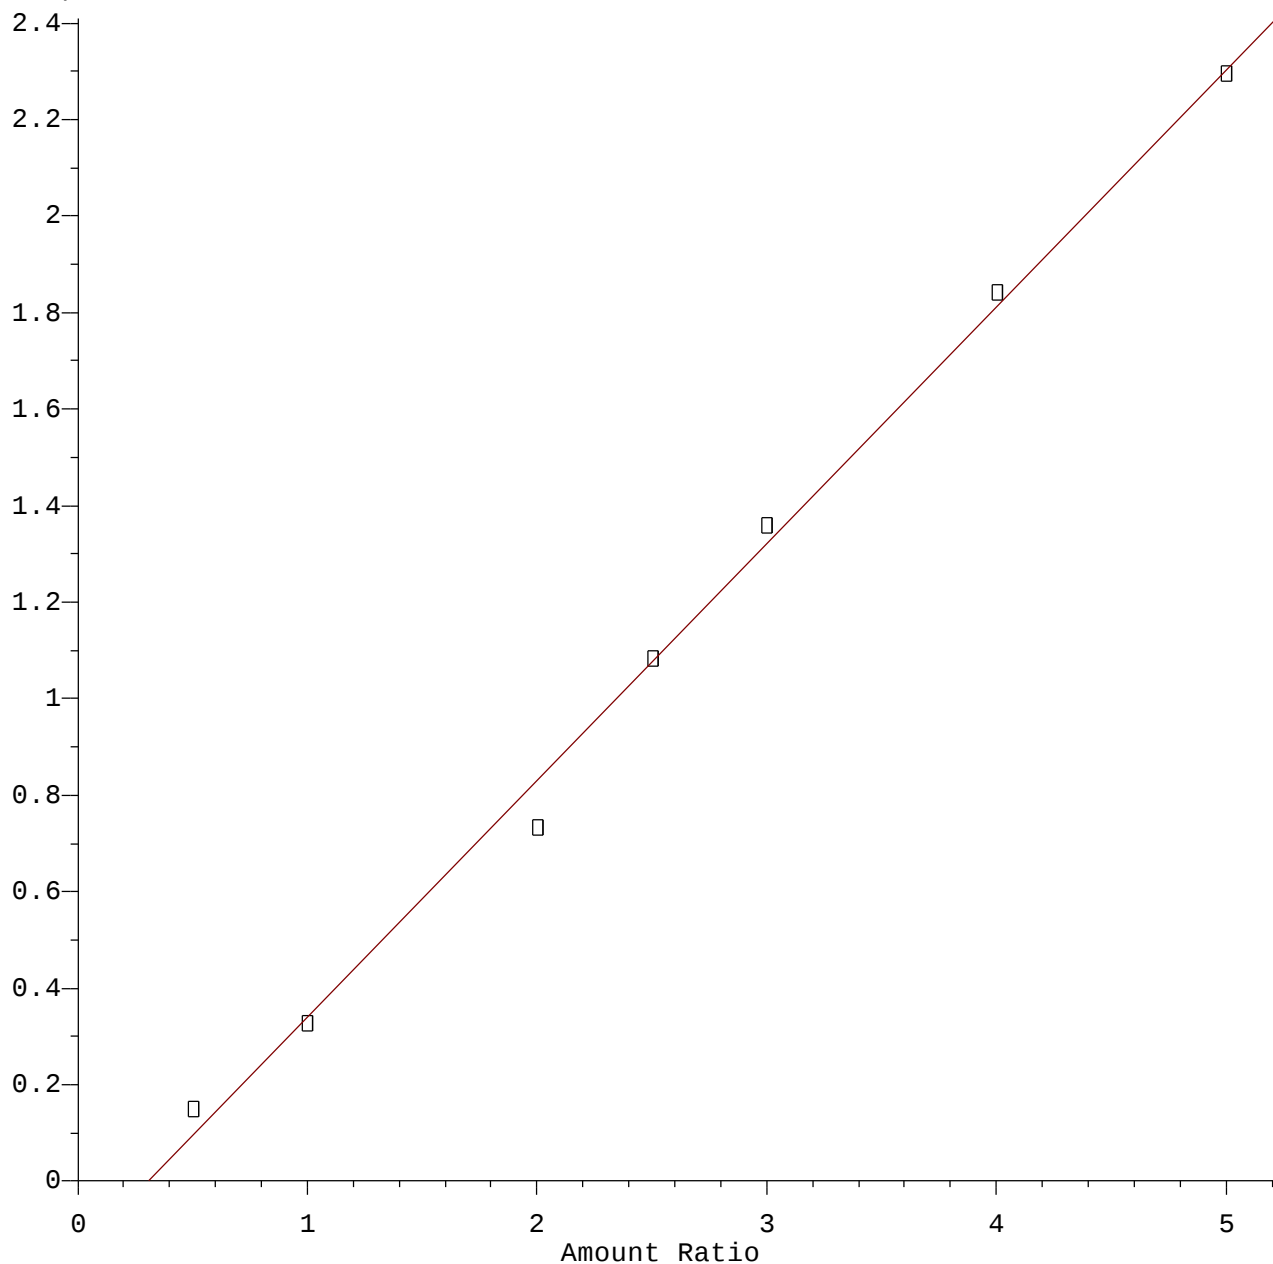

Resp Ratio = $4.90 \times 10^{-1} \times \text{Amt} - 1.50 \times 10^{-1}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030520.M
Calibration Table Last Updated: Thu Mar 05 17:42:35 2020

4,6-Dinitro-2-methylphenol

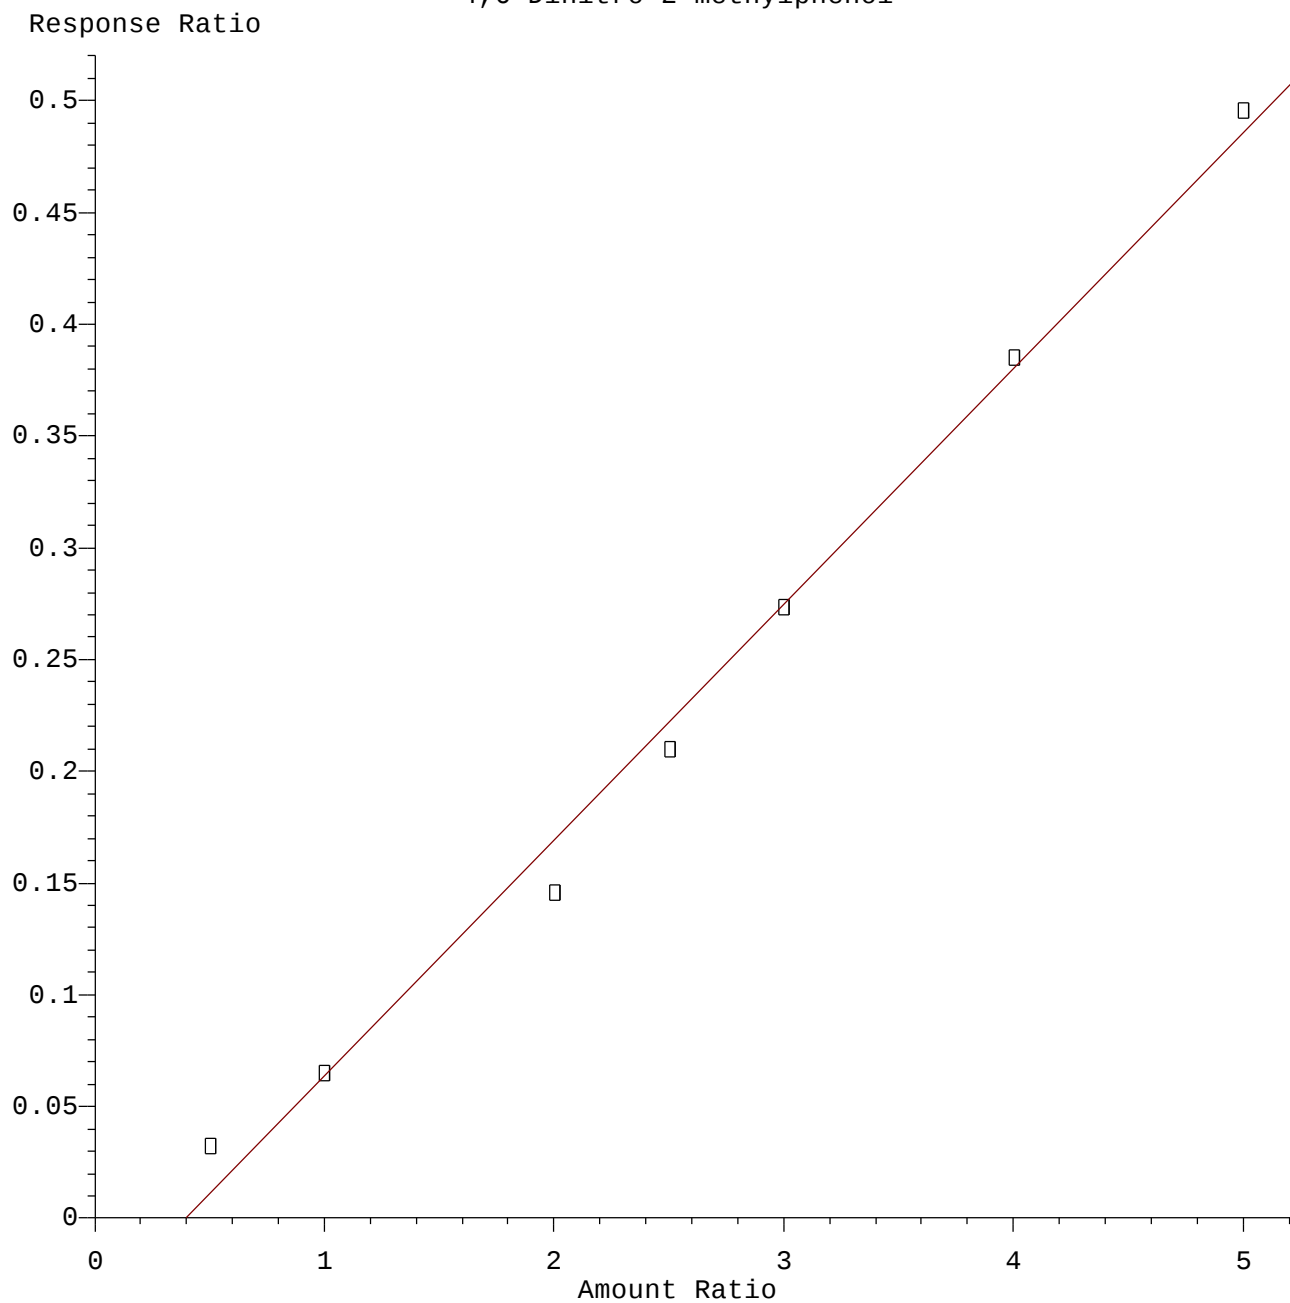

Resp Ratio = $1.05 \times 10^{-1} \times \text{Amt} - 4.17 \times 10^{-2}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030520.M
Calibration Table Last Updated: Thu Mar 05 17:42:35 2020