
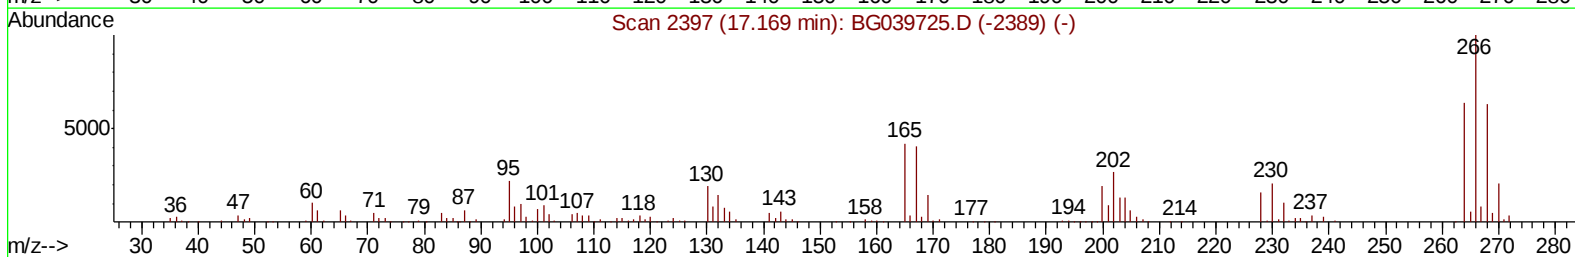
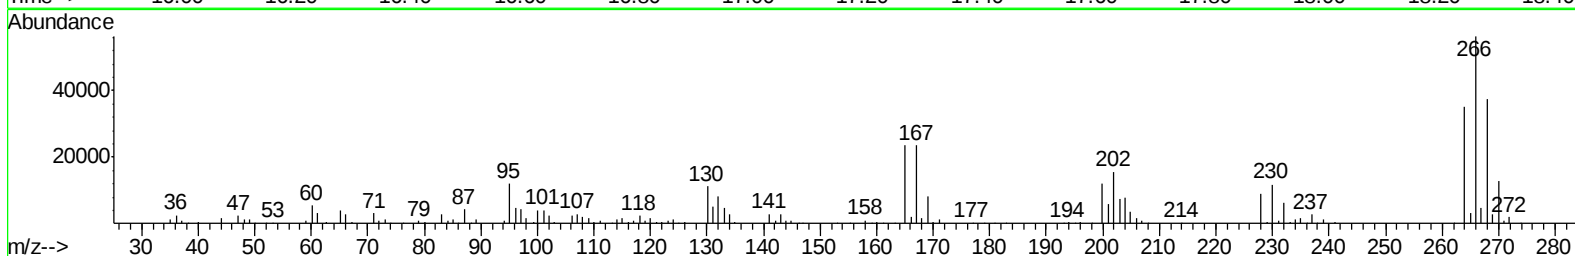


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030619\
Data File : BG039781.D
Acq On : 6 Mar 2019 10:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 03:21:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

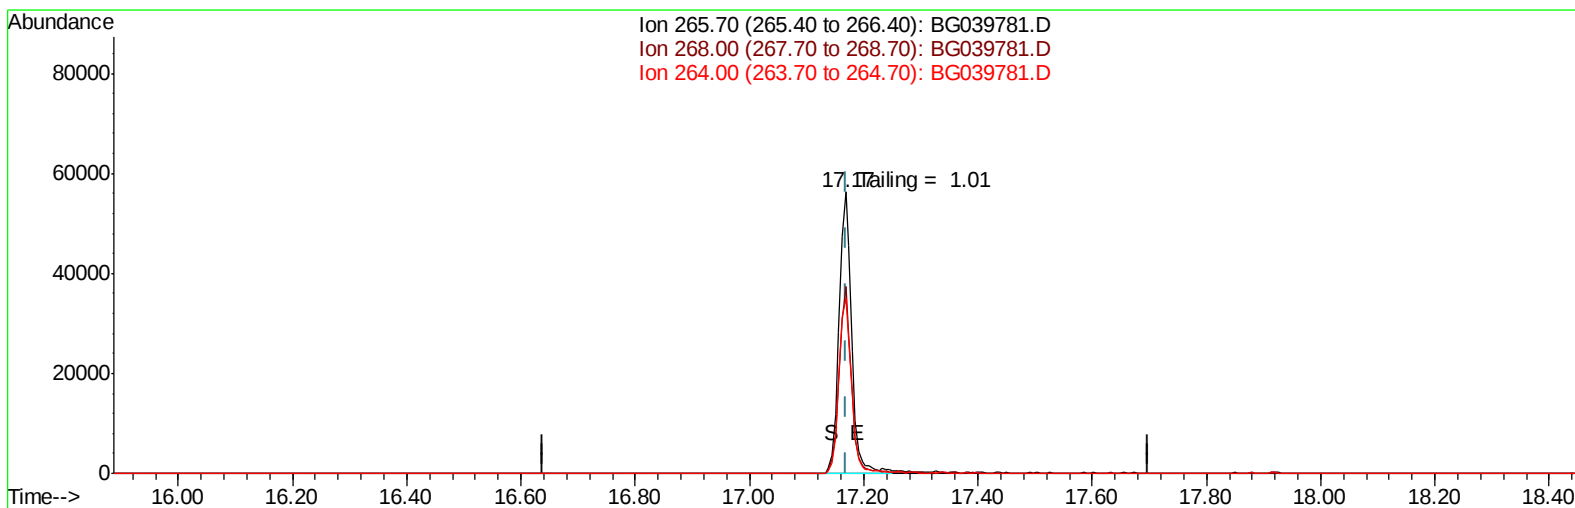

TIC: BG039781.D

(70) Pentachlorophenol (C)




17.168min (-0.002) 196531.27ng

response 84967

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.32
264.00	65.10	62.46
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030619\
Data File : BG039781.D
Acq On : 6 Mar 2019 10:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 03:21:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

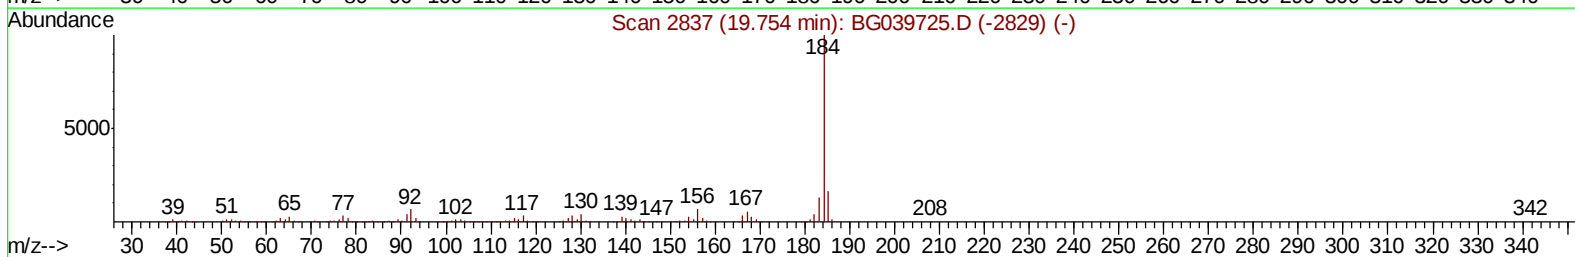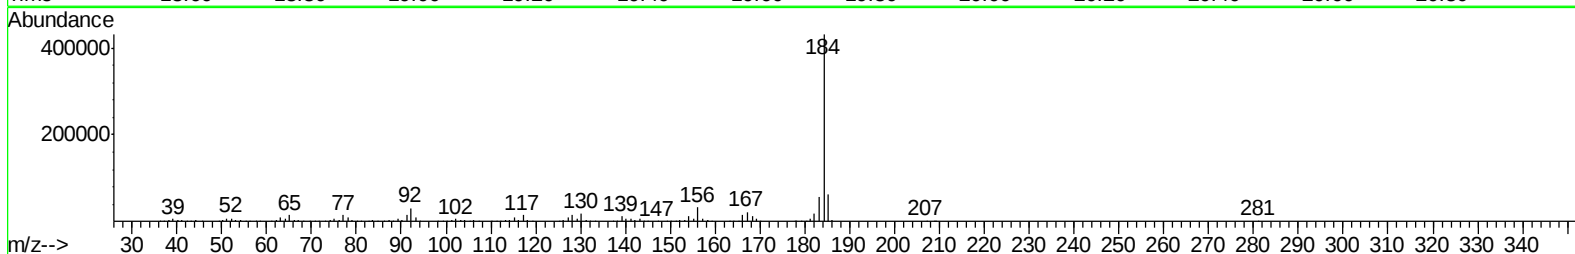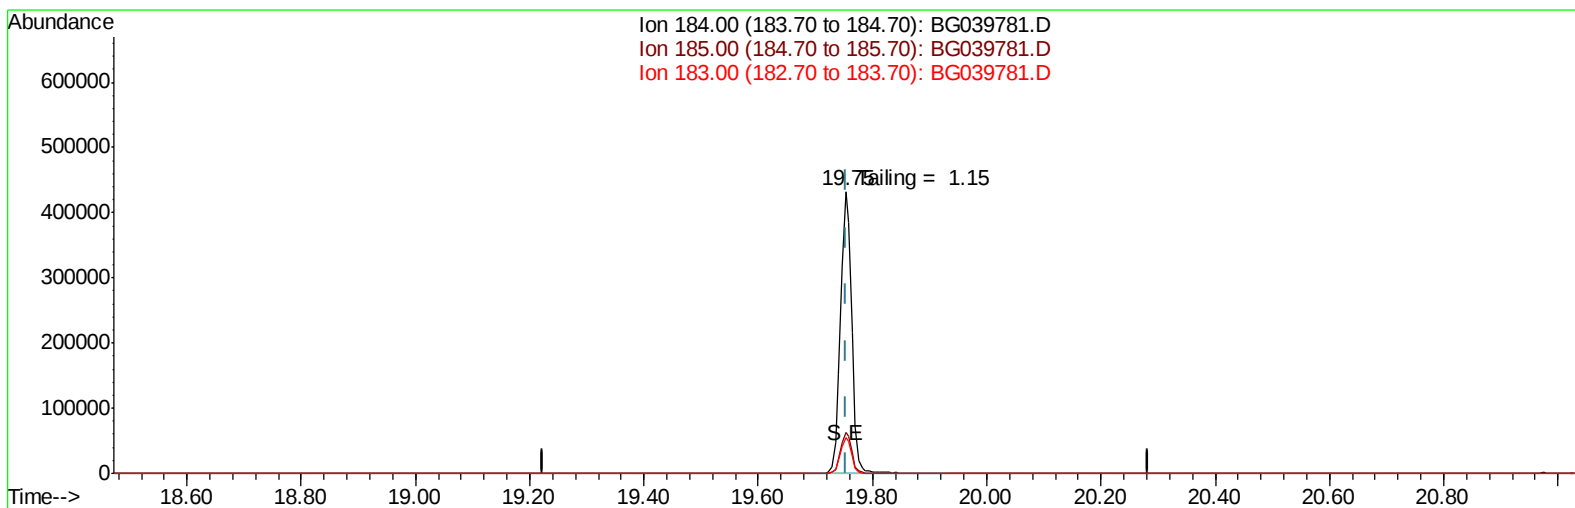

TIC: BG039781.D

(77) Benzidine

19.752min (-0.002) 27538.22ng

response 593357

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.71
183.00	13.20	12.84
0.00	0.00	0.00