
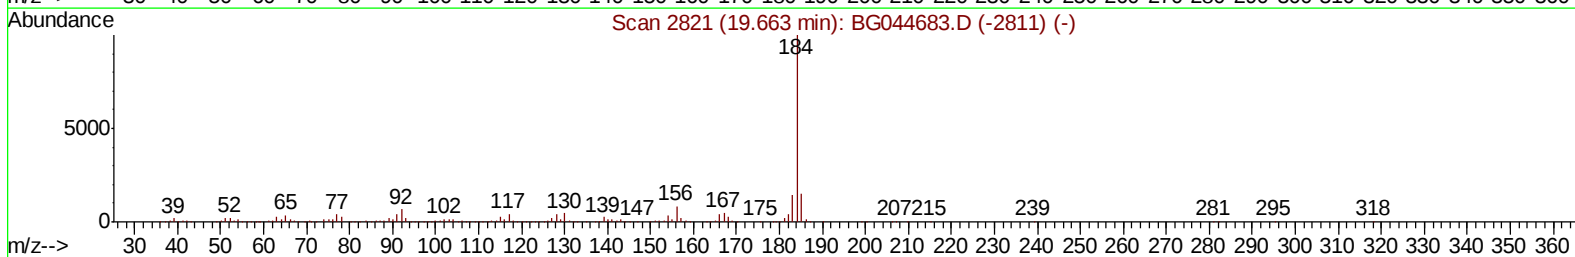
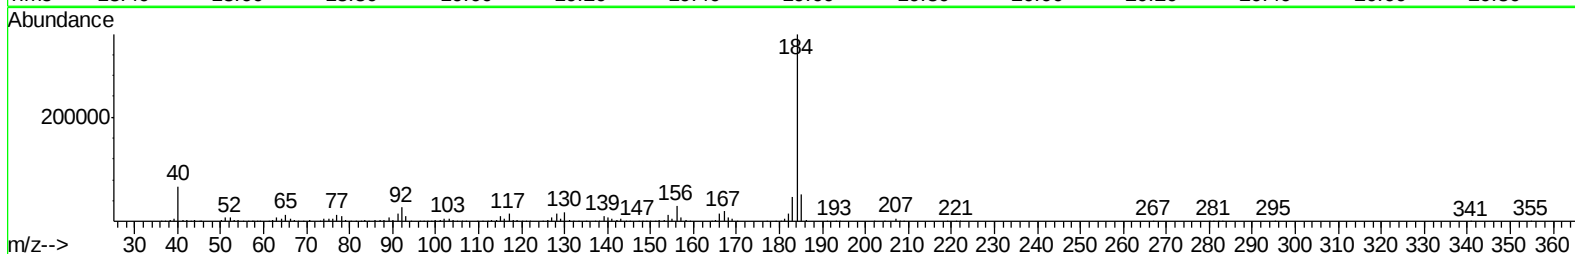


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030620\
 Data File : BG044689.D
 Acq On : 6 Mar 2020 9:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 04:02:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 17:42:35 2020
 Response via : Initial Calibration

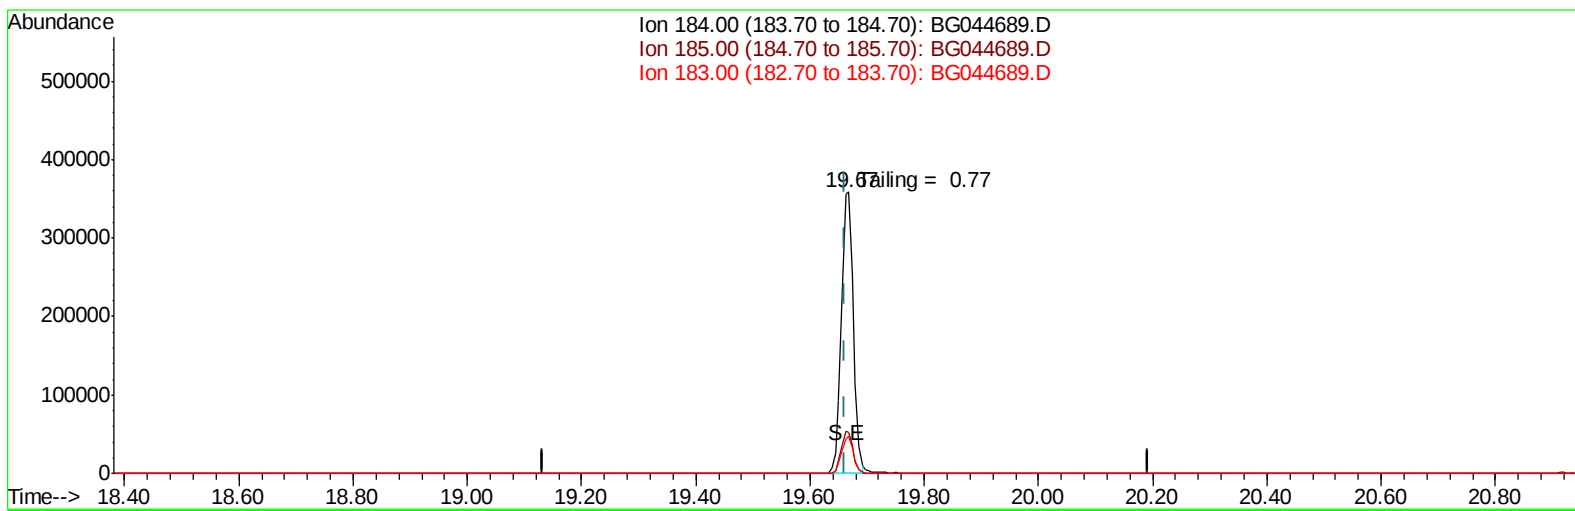

TIC: BG044689.D

(77) Benzidine




19.668min (+0.005) 211009.10ng

response 530666

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.43
183.00	14.30	12.99
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030620\
Data File : BG044689.D
Acq On : 6 Mar 2020 9:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 04:02:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 05 17:42:35 2020
Response via : Initial Calibration

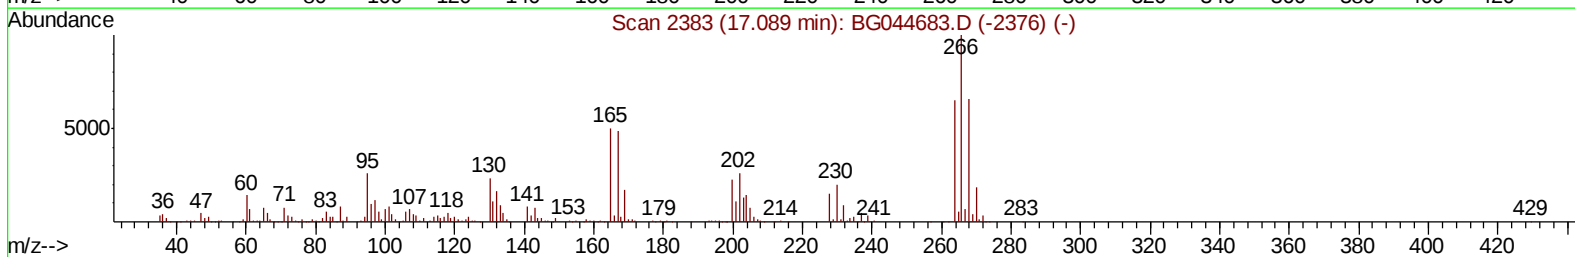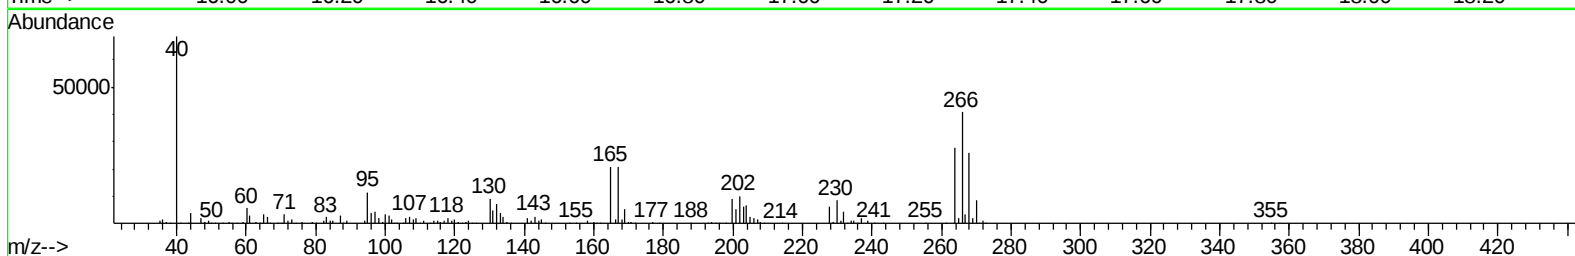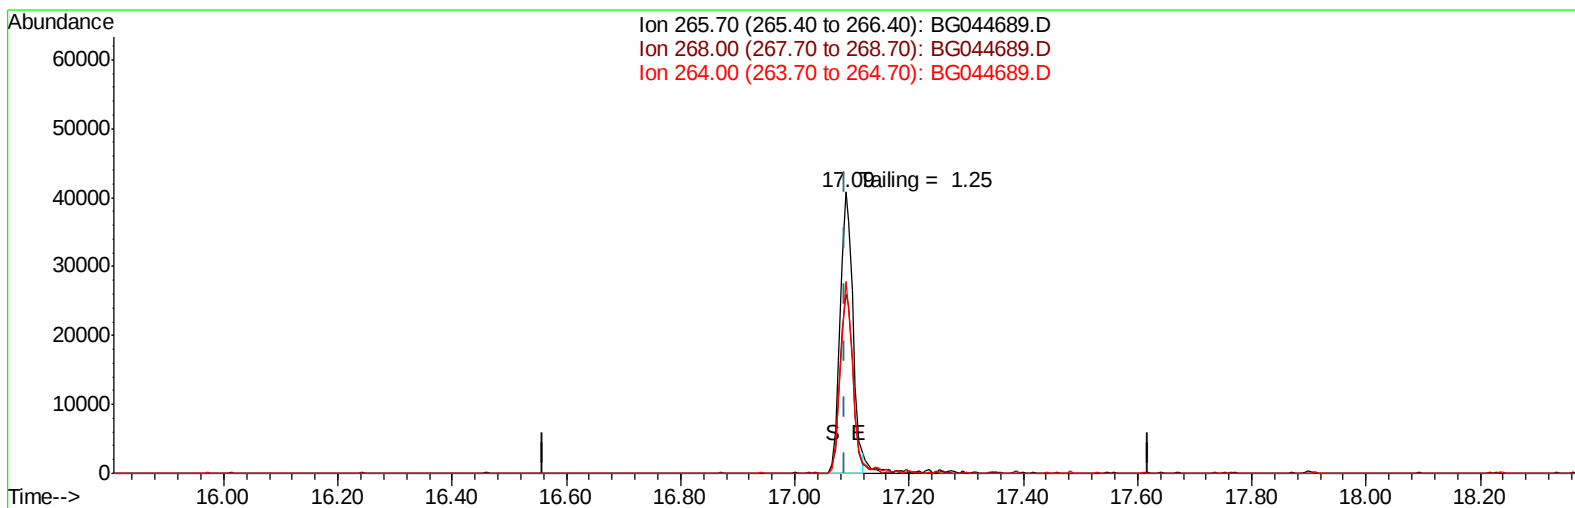

TIC: BG044689.D

(70) Pentachlorophenol (C)

17.088min (-0.001) 82057.24ng

response 65312

Ion	Exp%	Act%
265.70	100	100
268.00	65.90	63.68
264.00	65.40	68.29
0.00	0.00	0.00