


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030620\
 Data File : BG044689.D
 Acq On : 6 Mar 2020 9:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 05 17:42:35 2020

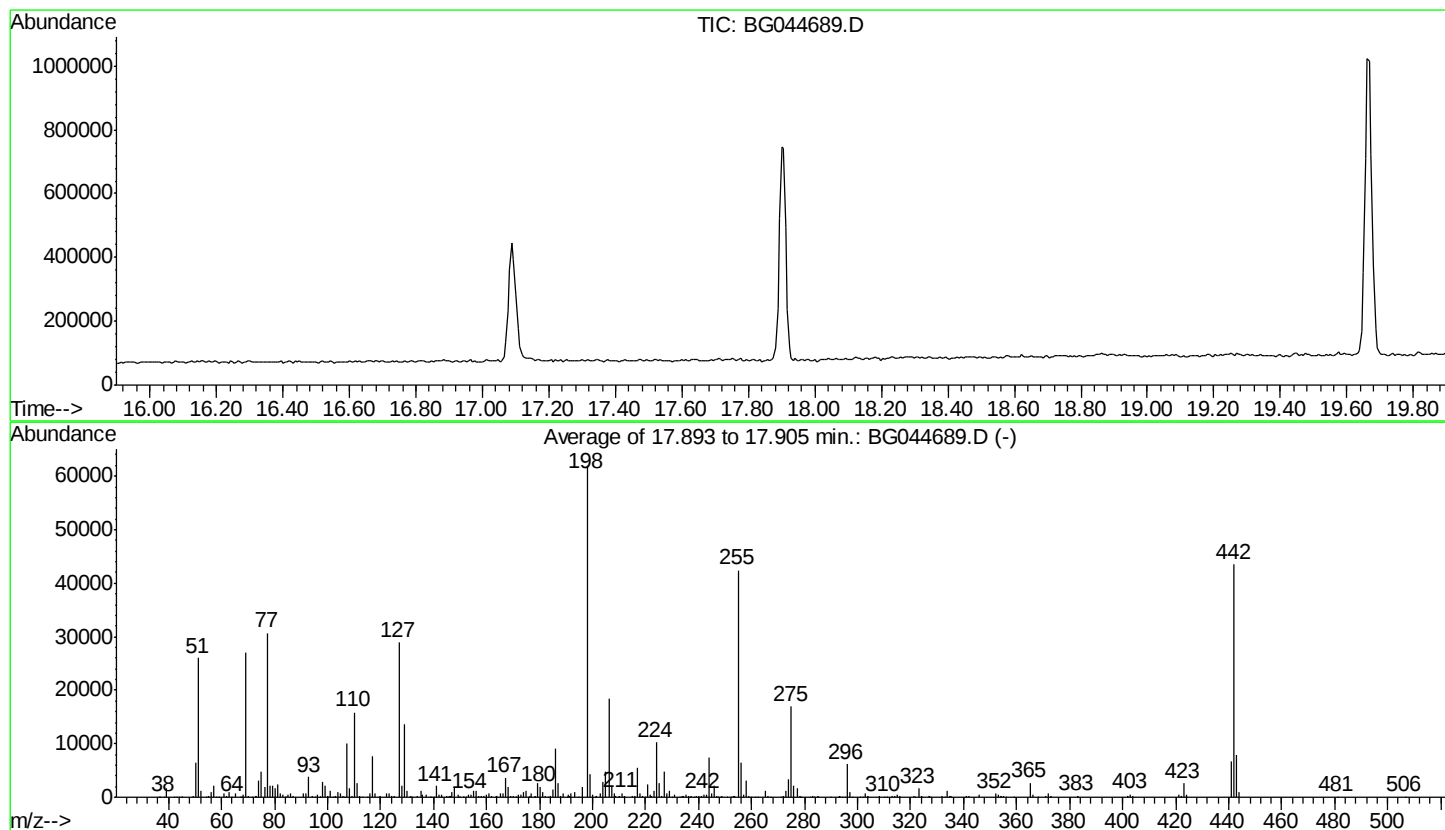

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	26006	PASS
68	69	0.00	2	1.8	472	PASS
69	198	0.00	100	43.5	26957	PASS
70	69	0.00	2	0.7	183	PASS
127	198	10	80	46.6	28896	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61968	PASS
199	198	5	9	6.8	4236	PASS
275	198	10	60	27.3	16926	PASS
365	198	1	100	4.4	2715	PASS
441	198	0.01	100	10.9	6733	PASS
442	198	50	100	70.2	43482	PASS
443	442	15	24	18.1	7851	PASS