


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030819\
 Data File : BG039816.D
 Acq On : 8 Mar 2019 11:45
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

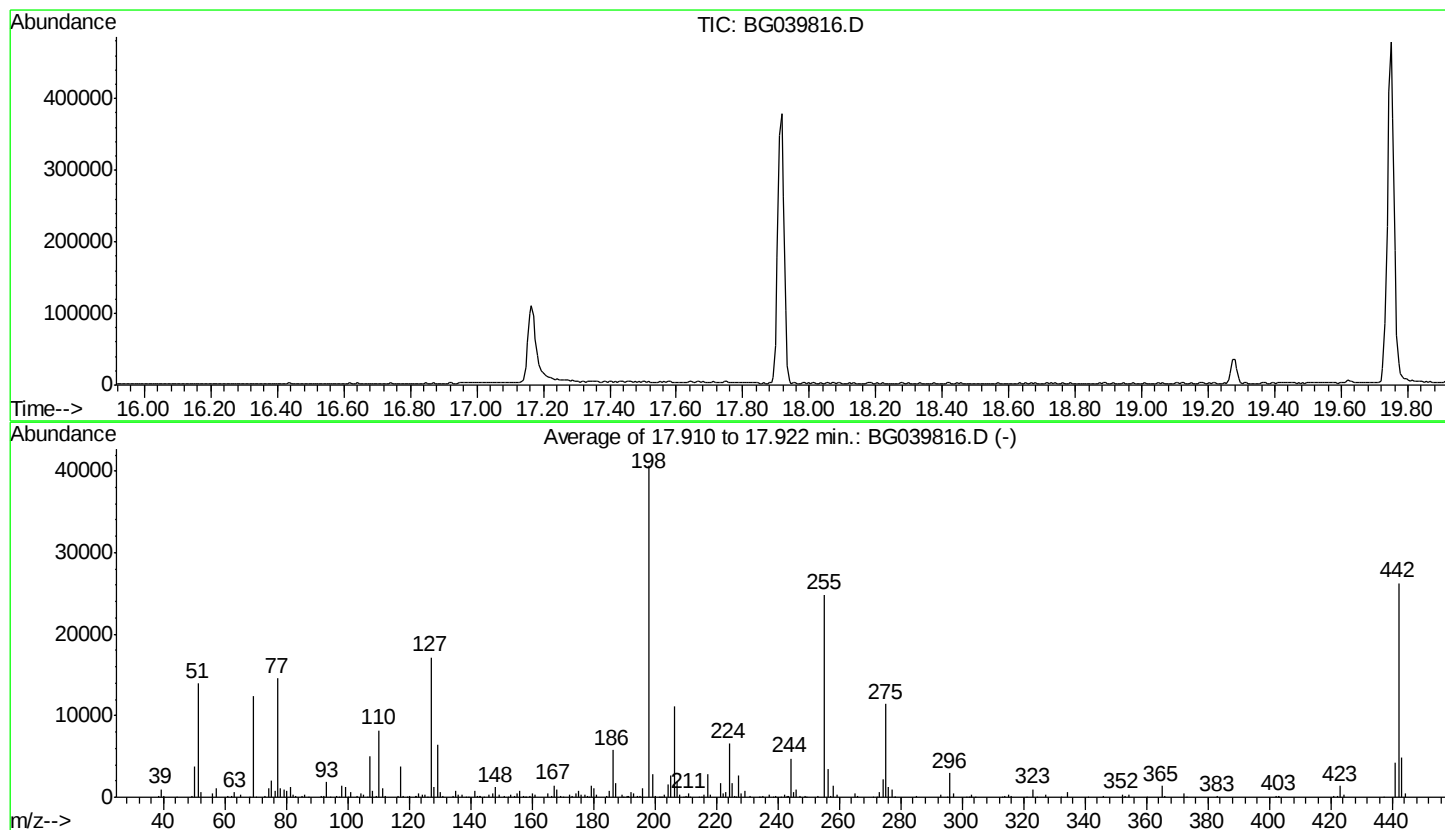

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	13959	PASS
68	69	0.00	2	0.5	64	PASS
69	198	0.00	100	30.3	12338	PASS
70	69	0.00	2	0.4	52	PASS
127	198	10	80	42.1	17141	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40674	PASS
199	198	5	9	7.0	2838	PASS
275	198	10	60	28.2	11454	PASS
365	198	1	100	3.4	1366	PASS
441	198	0.01	100	10.3	4202	PASS
442	198	50	100	64.6	26288	PASS
443	442	15	24	18.7	4908	PASS