

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
 Data File : BG052611.D
 Acq On : 8 Mar 2022 19:18
 Operator : CG/JU
 Sample : N1730-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 31-32-SAMPLE-LOCATION-16

Quant Time: Mar 09 04:19:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 08 01:09:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.212	152	26492	20.000	ng	0.00
21) Naphthalene-d8	11.050	136	104678	20.000	ng	#-0.01
39) Acenaphthene-d10	14.862	164	72731	20.000	ng	0.00
64) Phenanthrene-d10	17.611	188	181864	20.000	ng	0.00
76) Chrysene-d12	21.923	240	204021	20.000	ng	-0.01
86) Perylene-d12	25.383	264	204988	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.745	112	140796	90.546	ng	0.00
7) Phenol-d6	7.361	99	194893	89.198	ng	-0.01
23) Nitrobenzene-d5	9.381	82	137656	59.951	ng	-0.02
42) 2,4,6-Tribromophenol	16.348	330	96560	92.378	ng	0.00
45) 2-Fluorobiphenyl	13.482	172	300578	56.987	ng	0.00
79) Terphenyl-d14	20.202	244	564316	49.532	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propyla...	9.387	70	18178	12.219	ng	# 75
50) Dimethylphthalate	14.298	163	29610	5.286	ng	# 98
51) 2,6-Dinitrotoluene	14.856	165	9989	8.216	ng	# 16
57) 2,4-Dinitrotoluene	14.856	165	9989	5.809	ng	# 15
67) 4-Bromophenyl-phenylether	16.354	248	5196	2.364	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052611.D
Acq On : 8 Mar 2022 19:18
Operator : CG/JU
Sample : N1730-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
31-32-SAMPLE-LOCATION-16

Quant Time: Mar 09 04:19:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 08 01:09:10 2022
Response via : Initial Calibration




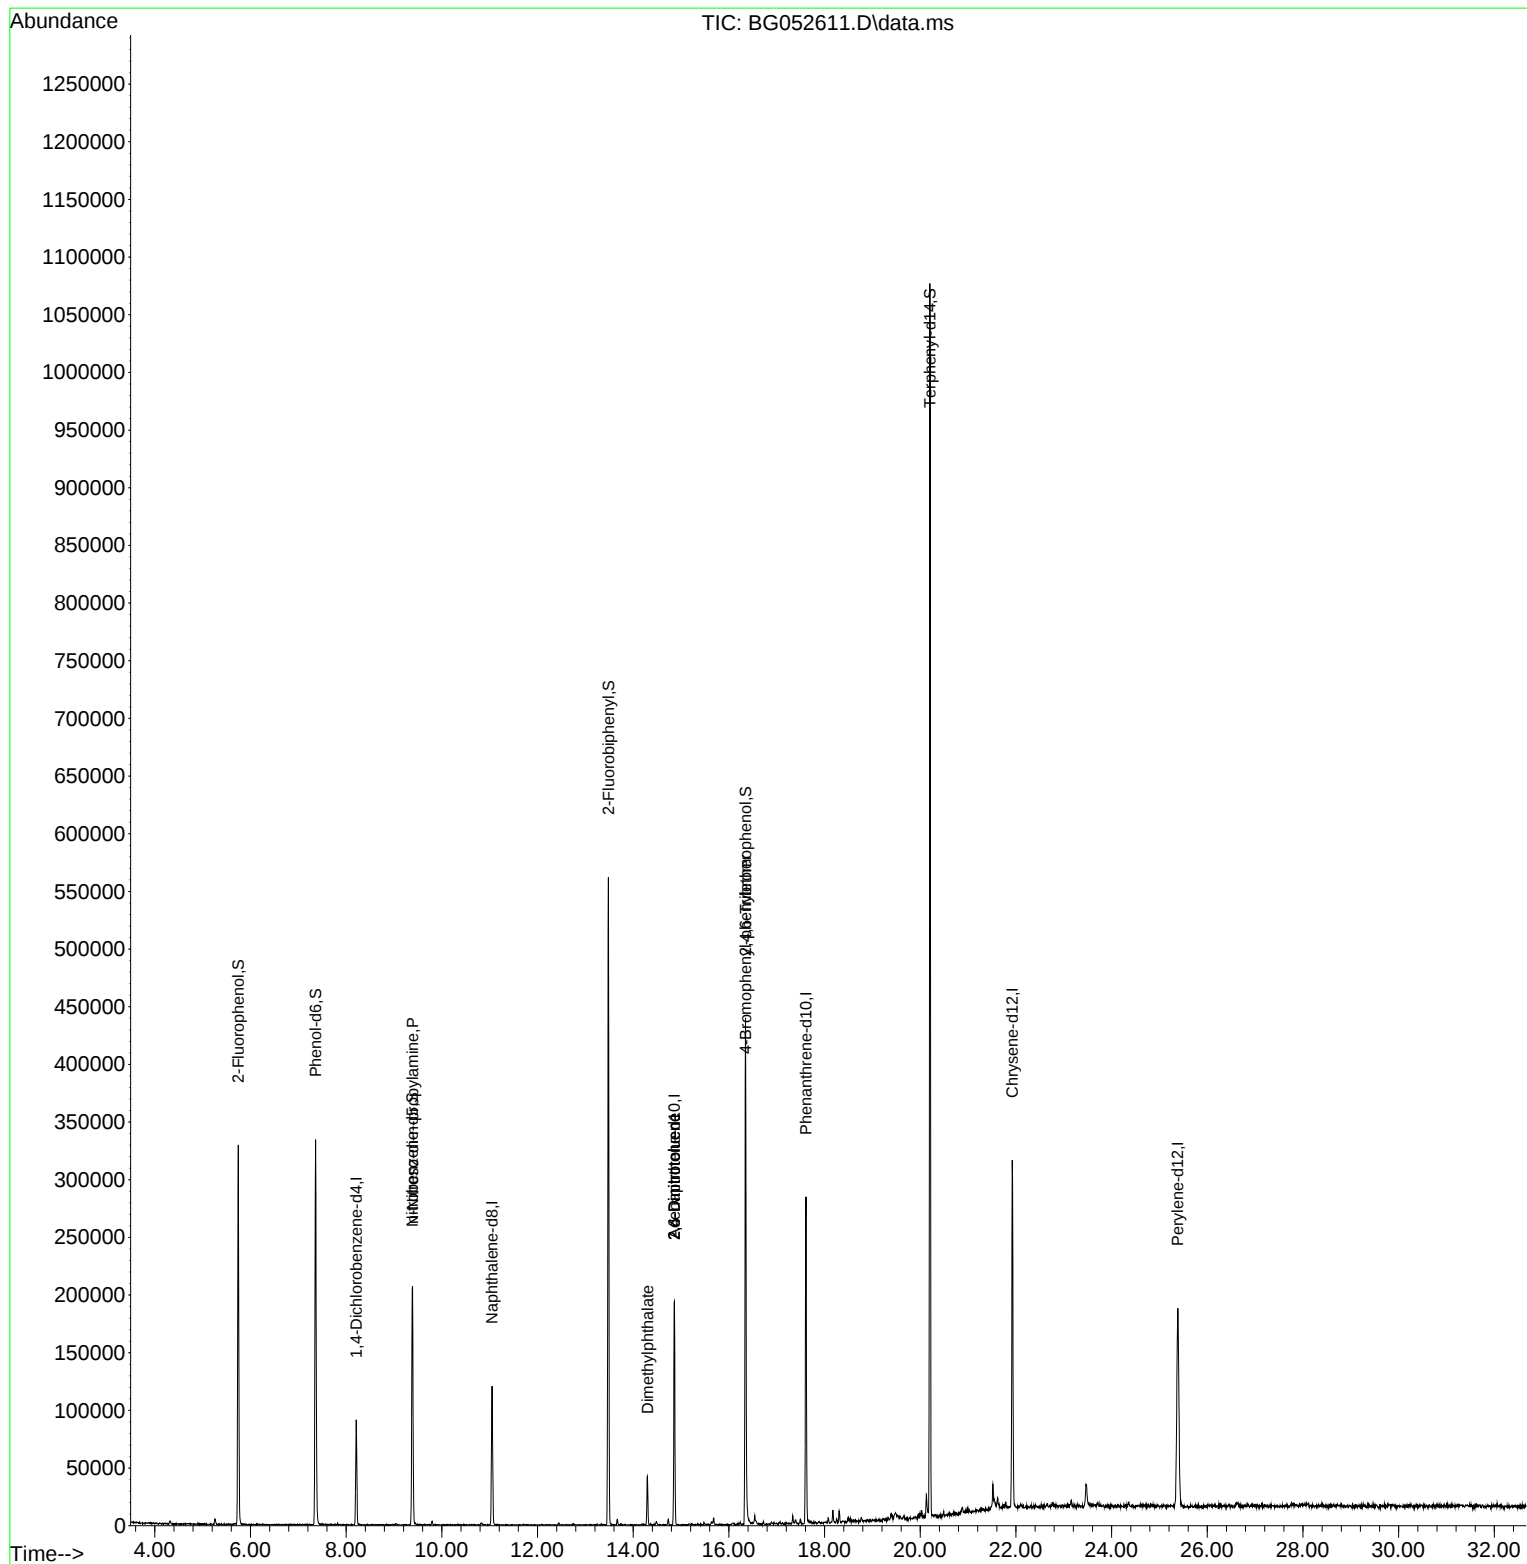




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.212 min Scan# 806
Delta R.T. -0.010 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18




Instrument :
BNA_G
ClientSampleId :
31-32-SAMPLE-LOCATION-16


Tgt Ion:152 Resp: 26492
Ion Ratio Lower Upper
152 100
150 154.3 117.8 176.8
115 56.5 50.2 75.2

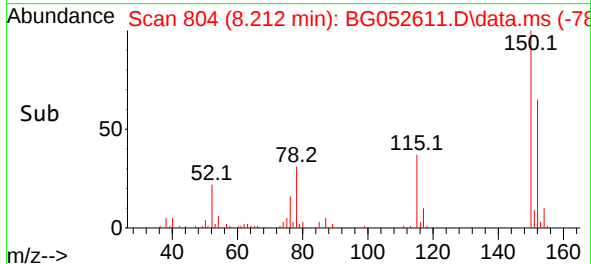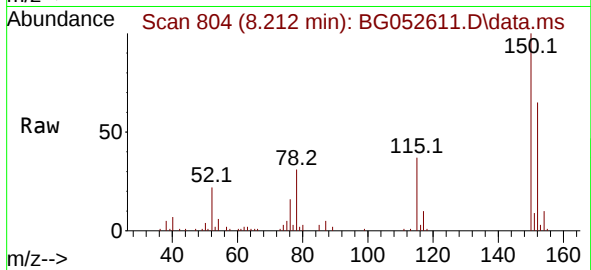

#5
2-Fluorophenol
Concen: 90.546 ng
RT: 5.745 min Scan# 384
Delta R.T. -0.004 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18

Tgt Ion:112 Resp: 140796
Ion Ratio Lower Upper
112 100
64 62.5 60.4 90.6
63 35.0 33.3 49.9


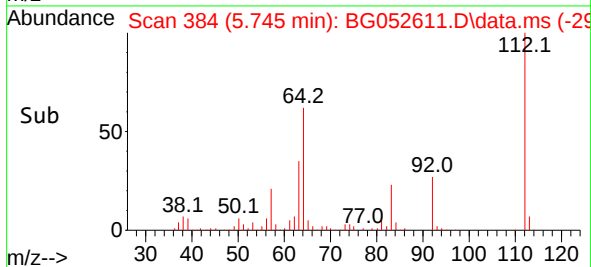

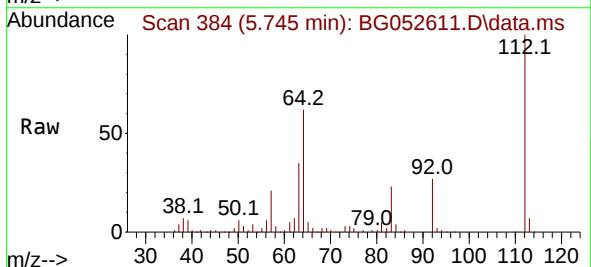


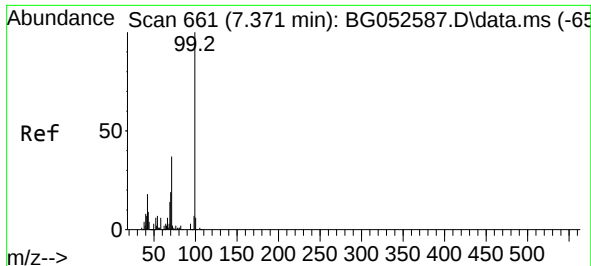

#7
Phenol-d6
Concen: 89.198 ng
RT: 7.361 min Scan# 61
Delta R.T. -0.010 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18




Instrument :
BNA_G
ClientSampleId :
31-32-SAMPLE-LOCATION-16


Tgt Ion: 99 Resp: 194893
Ion Ratio Lower Upper
99 100
42 19.2 19.1 28.7
71 38.3 33.4 50.2

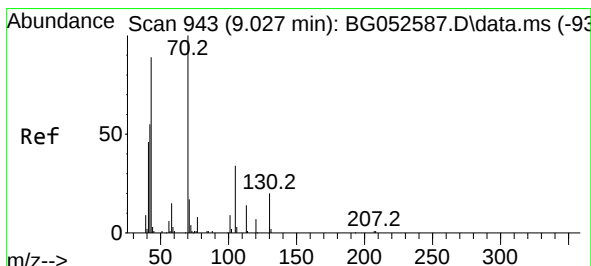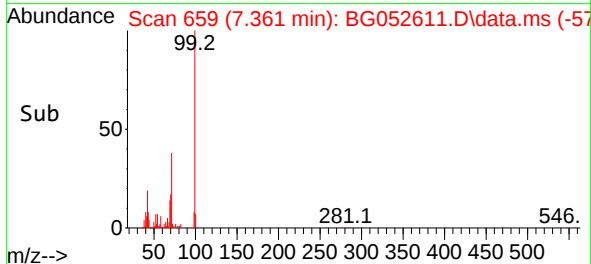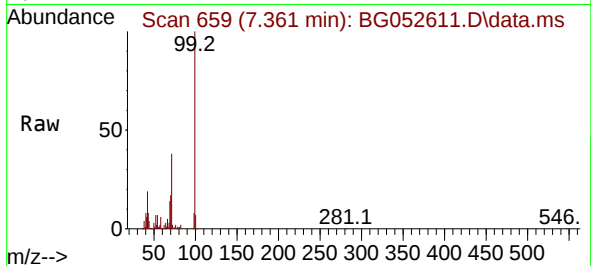

#19
n-Nitroso-di-n-propylamine
Concen: 12.219 ng
RT: 9.387 min Scan# 1004
Delta R.T. 0.360 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18

Tgt Ion: 70 Resp: 18178
Ion Ratio Lower Upper
70 100
42 47.3 51.8 77.6#
101 0.0 6.6 10.0#
130 1.8 14.7 22.1#


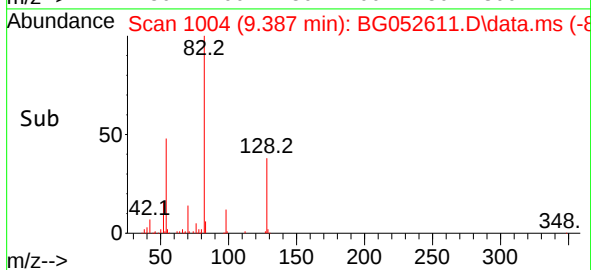

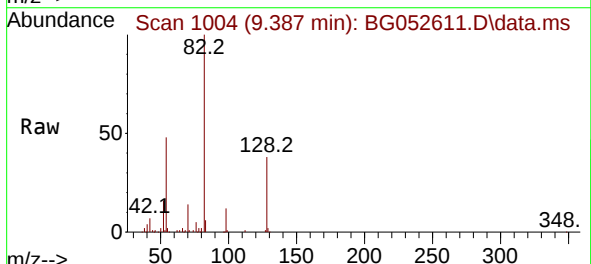


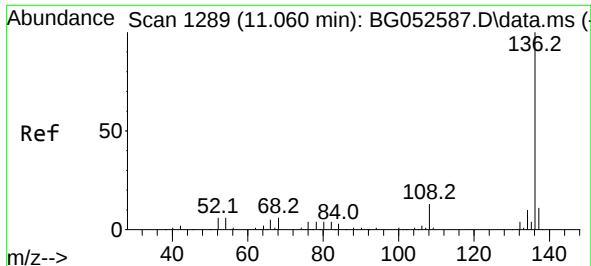

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.050 min Scan# 1103
Delta R.T. -0.010 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18




Instrument :
BNA_G
ClientSampleId :
31-32-SAMPLE-LOCATION-16


Tgt Ion:136 Resp: 104678
Ion Ratio Lower Upper
136 100
137 11.0 9.1 13.7
54 8.3 8.3 12.5#
68 5.7 4.5 6.7

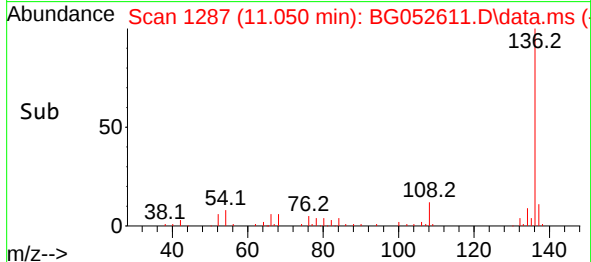

#23
Nitrobenzene-d5
Concen: 59.951 ng
RT: 9.381 min Scan# 1003
Delta R.T. -0.016 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18

Tgt Ion: 82 Resp: 137656
Ion Ratio Lower Upper
82 100
128 36.3 27.0 40.4
54 46.3 41.0 61.6


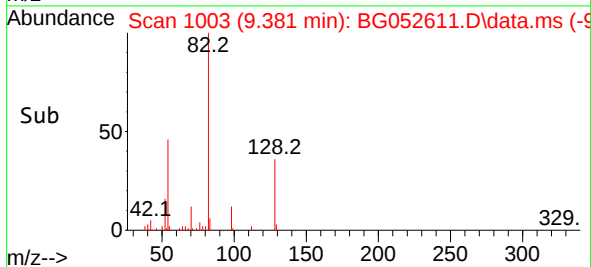

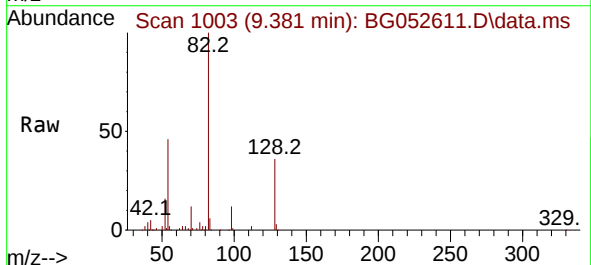




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.862 min Scan# 1937
Delta R.T. -0.004 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18




Instrument :
BNA_G
ClientSampleId :
31-32-SAMPLE-LOCATION-16


Tgt Ion:164 Resp: 72731
Ion Ratio Lower Upper
164 100
162 100.7 82.2 123.2
160 41.2 36.2 54.2

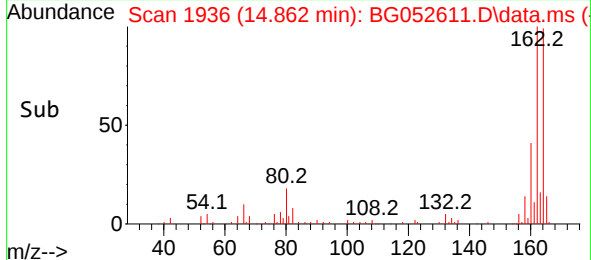

#42
2,4,6-Tribromophenol
Concen: 92.378 ng
RT: 16.348 min Scan# 2189
Delta R.T. -0.004 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18

Tgt Ion:330 Resp: 96560
Ion Ratio Lower Upper
330 100
332 94.4 78.6 117.8
141 31.8 28.8 43.2


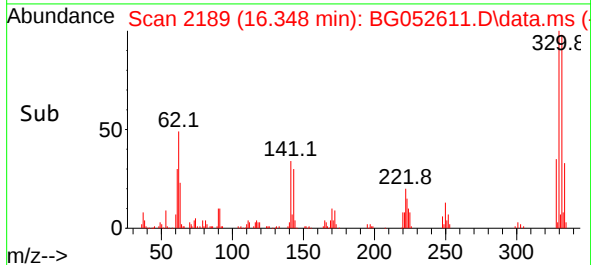

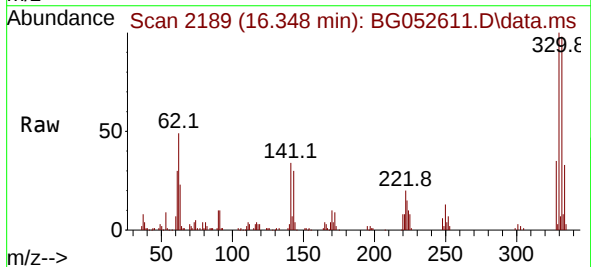


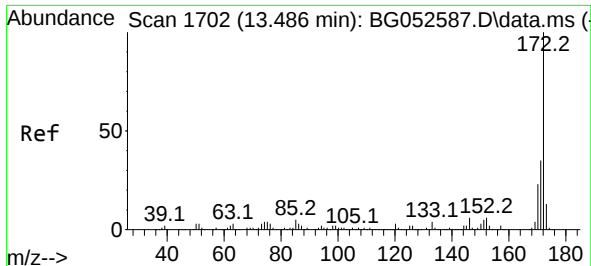

#45
2-Fluorobiphenyl
Concen: 56.987 ng
RT: 13.482 min Scan# 11
Delta R.T. -0.004 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18




Instrument :
BNA_G
ClientSampleId :
31-32-SAMPLE-LOCATION-16


Tgt Ion:172 Resp: 300578
Ion Ratio Lower Upper
172 100
171 35.6 28.3 42.5
170 22.4 18.3 27.5

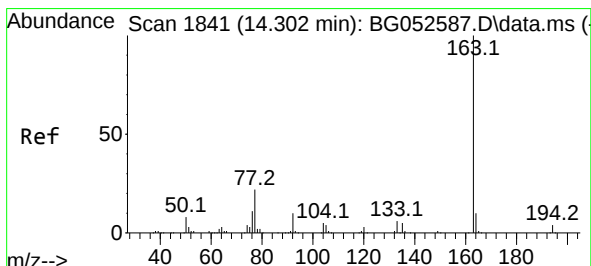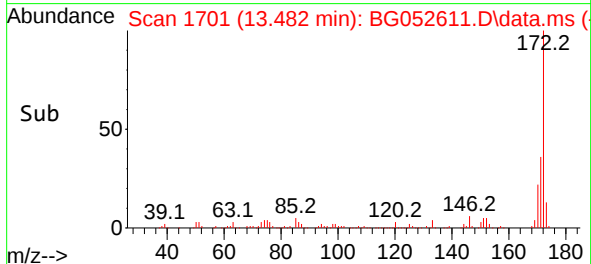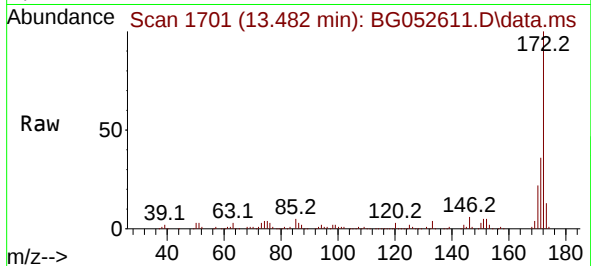

#50
Dimethylphthalate
Concen: 5.286 ng
RT: 14.298 min Scan# 1840
Delta R.T. -0.004 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18

Tgt Ion:163 Resp: 29610
Ion Ratio Lower Upper
163 100
194 3.1 3.4 5.2#
164 9.8 8.4 12.6



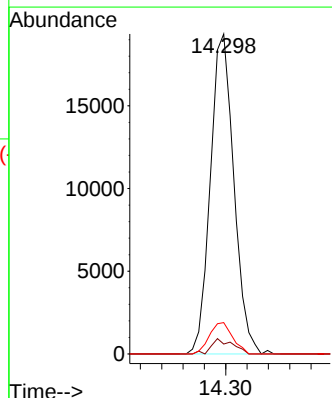
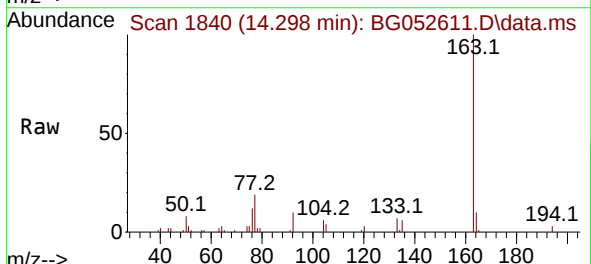


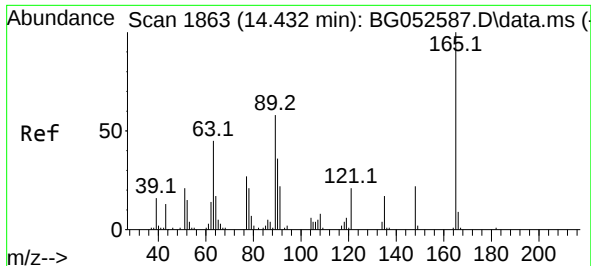

#51
2,6-Dinitrotoluene
Concen: 8.216 ng
RT: 14.856 min Scan# 1935
Delta R.T. 0.425 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18




Instrument :
BNA_G
ClientSampleId :
31-32-SAMPLE-LOCATION-16


Tgt Ion:165 Resp: 9989
Ion Ratio Lower Upper
165 100
63 0.0 59.0 88.4#
89 0.0 49.4 74.0#

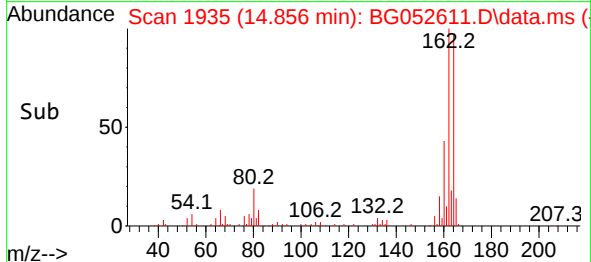

#57
2,4-Dinitrotoluene
Concen: 5.809 ng
RT: 14.856 min Scan# 1935
Delta R.T. -0.363 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18

Tgt Ion:165 Resp: 9989
Ion Ratio Lower Upper
165 100
63 0.0 44.6 66.8#
89 0.0 67.4 101.0#
182 0.0 1.6 2.4#


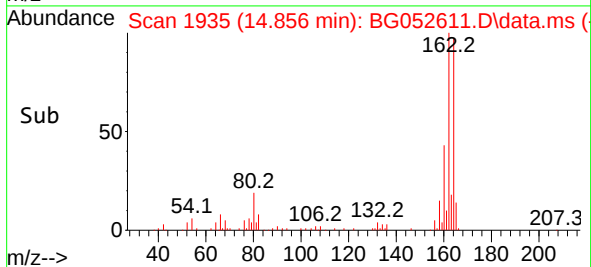

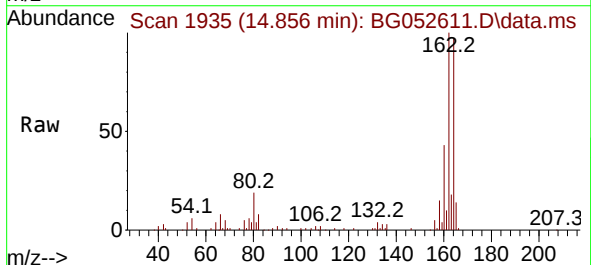


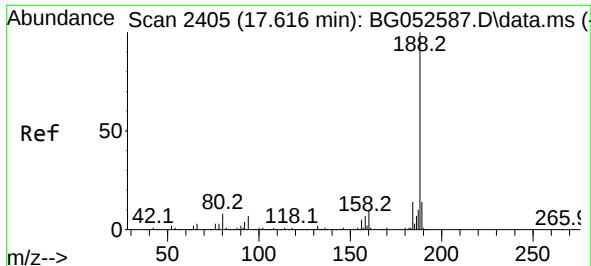

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.611 min Scan# 2405
Delta R.T. -0.005 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18




Instrument :
BNA_G
ClientSampleId :
31-32-SAMPLE-LOCATION-16


Tgt Ion:188 Resp: 181864
Ion Ratio Lower Upper
188 100
94 6.6 5.9 8.9
80 8.6 6.6 10.0

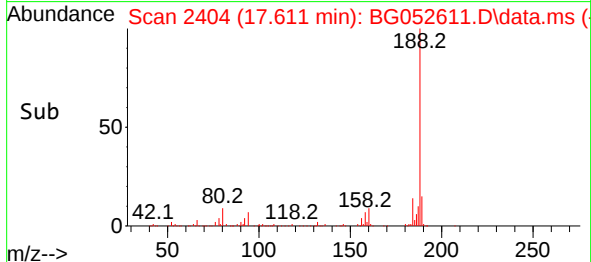

#67
4-Bromophenyl-phenylether
Concen: 2.364 ng
RT: 16.354 min Scan# 2190
Delta R.T. -0.439 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18

Tgt Ion:248 Resp: 5196
Ion Ratio Lower Upper
248 100
250 166.3 79.6 119.4#
141 433.6 54.6 81.8#


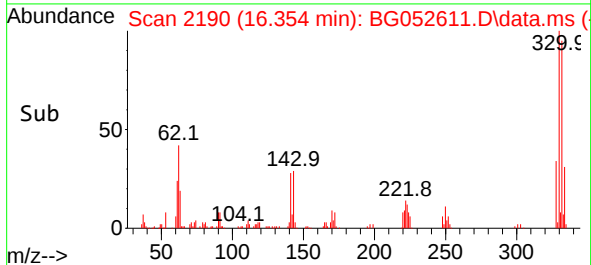

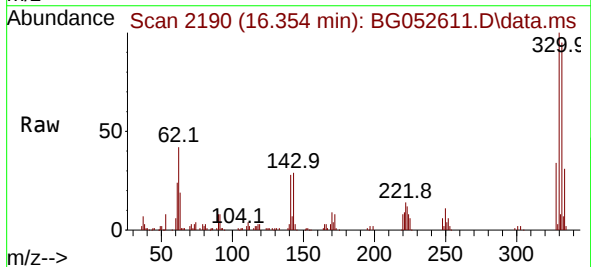




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.923 min Scan# 31
Delta R.T. -0.010 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18




Instrument :
BNA_G
ClientSampleId :
31-32-SAMPLE-LOCATION-16


Tgt Ion:240 Resp: 204021
Ion Ratio Lower Upper
240 100
120 5.6 4.4 6.6
236 24.9 20.8 31.2

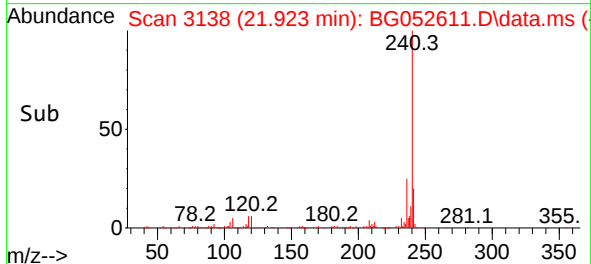

#79
Terphenyl-d14
Concen: 49.532 ng
RT: 20.202 min Scan# 2845
Delta R.T. -0.004 min
Lab File: BG052611.D
Acq: 8 Mar 2022 19:18

Tgt Ion:244 Resp: 564316
Ion Ratio Lower Upper
244 100
212 6.7 6.0 9.0
122 6.9 6.2 9.4

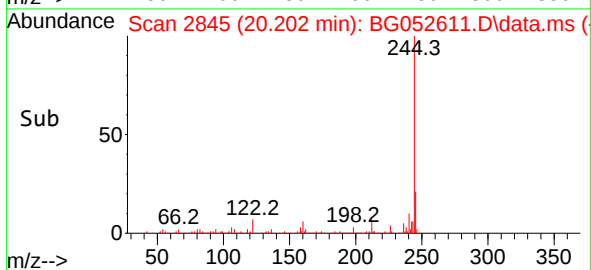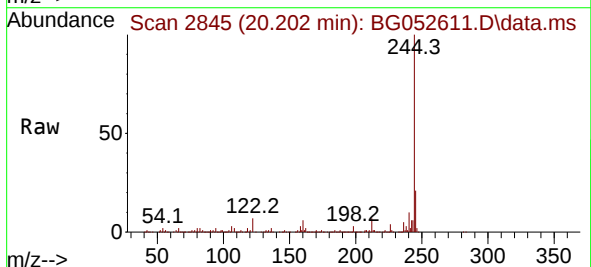



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.383 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: BG052611.D
 Acq: 8 Mar 2022 19:18

Instrument :
 BNA_G
 ClientSampleId :
 31-32-SAMPLE-LOCATION-16

Tgt Ion:264 Resp: 204988
 Ion Ratio Lower Upper
 264 100
 260 21.9 18.5 27.7
 265 22.4 17.8 26.6

