
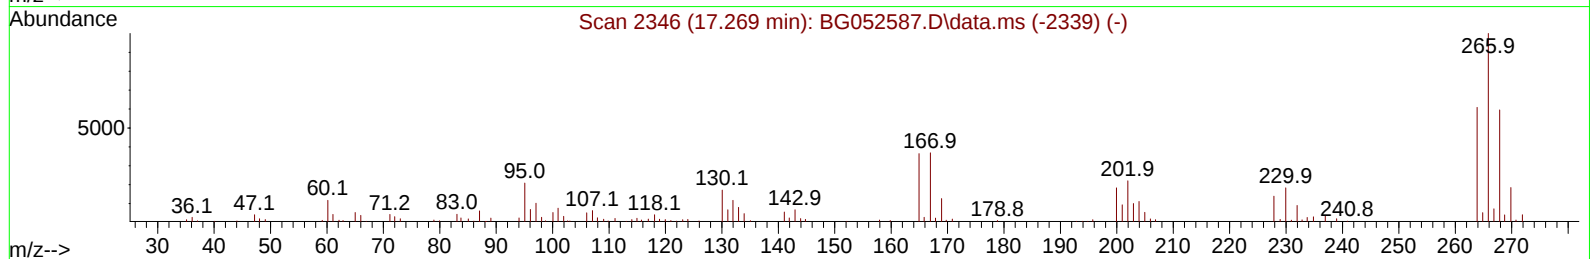
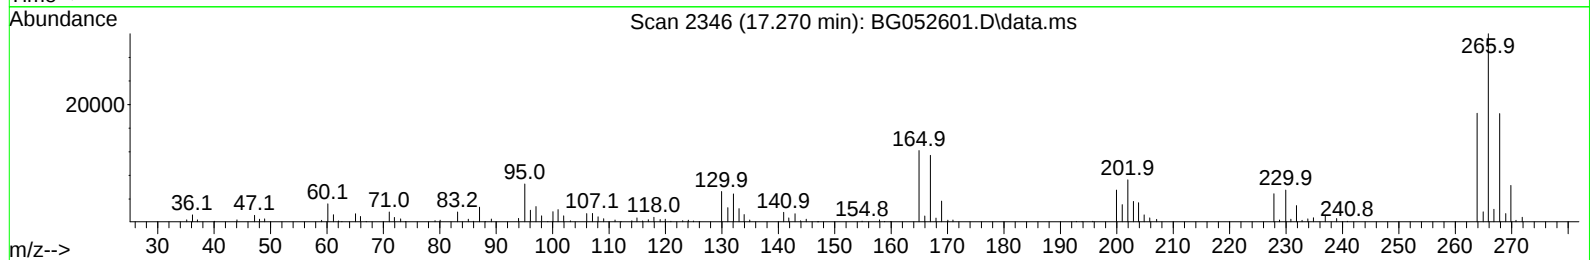


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052601.D
Acq On : 8 Mar 2022 12:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 05:02:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 08 01:09:10 2022
Response via : Initial Calibration

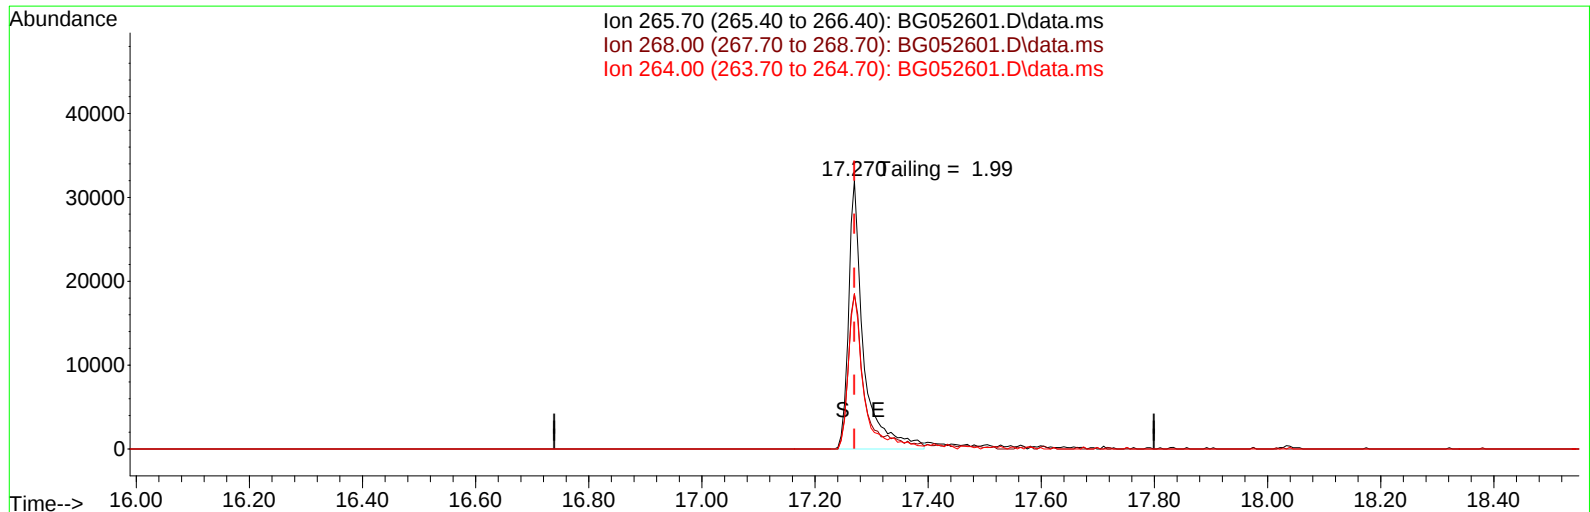

TIC: BG052601.D\data.ms

(70) Pentachlorophenol (C)




17.270min (+ 0.001) 120019.68 ng

response 59115

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	57.70
264.00	65.20	57.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052601.D
Acq On : 8 Mar 2022 12:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 05:02:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 08 01:09:10 2022
Response via : Initial Calibration

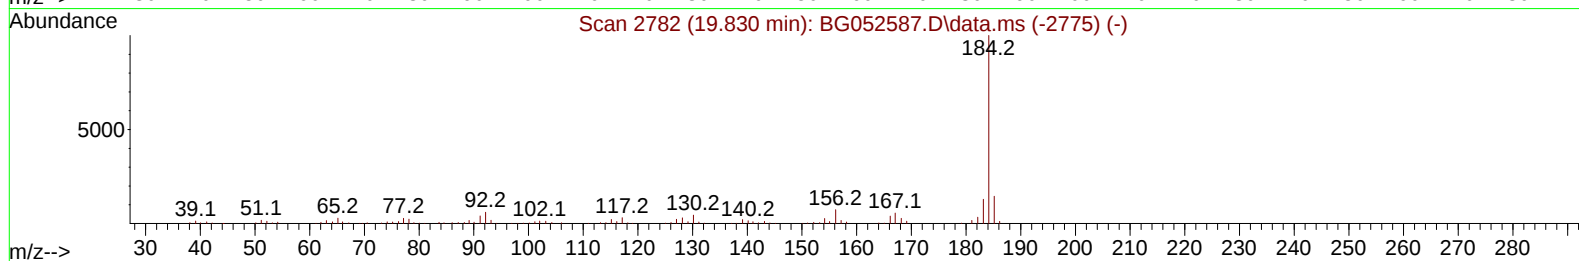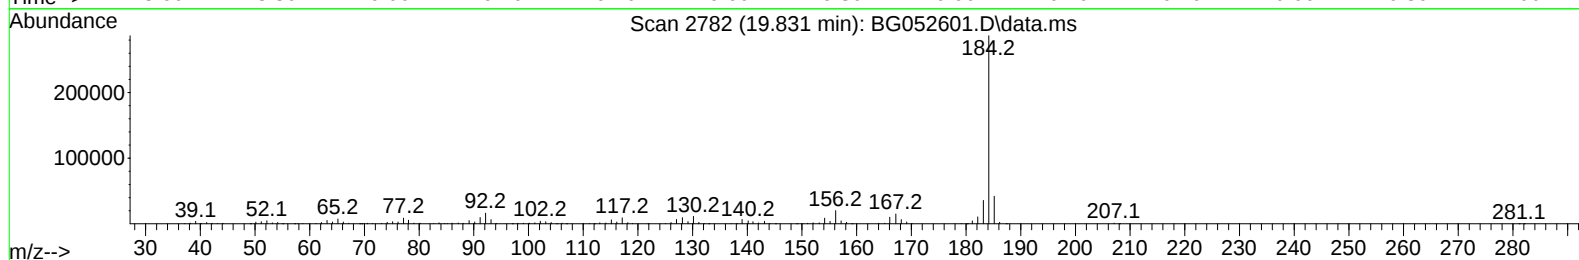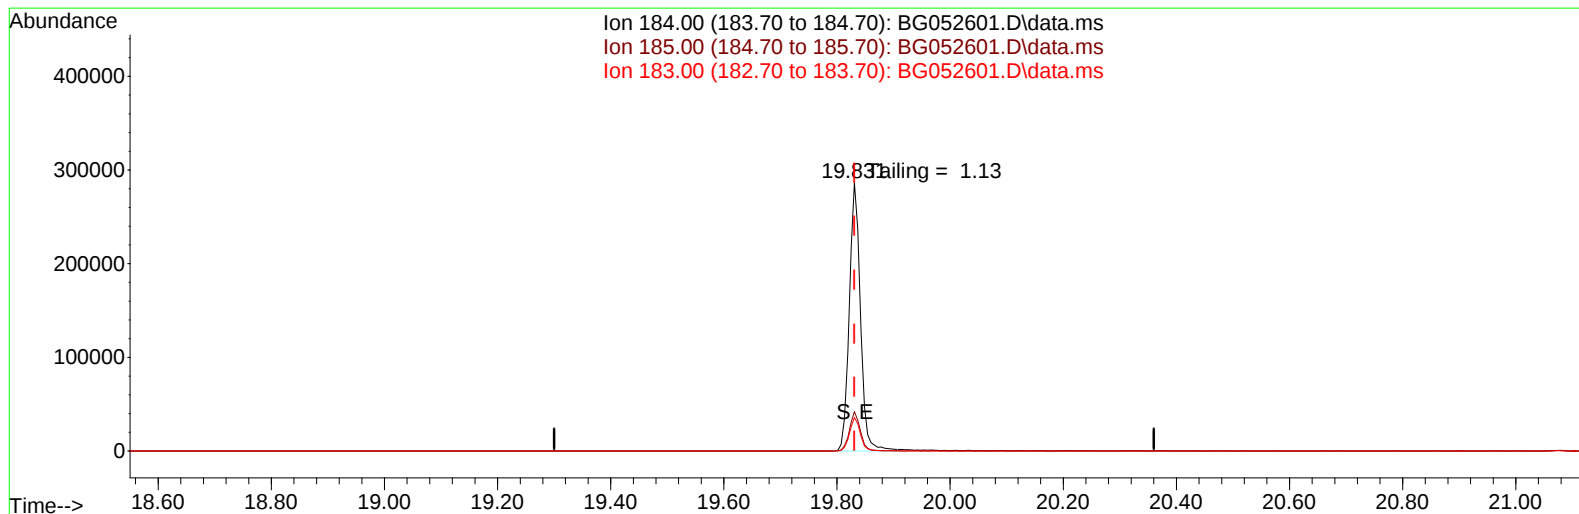

TIC: BG052601.D\data.ms

(77) Benzidine

19.831min (+ 0.001) 22563.44 ng

response 395618

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.66
183.00	12.20	12.47
0.00	0.00	0.00