

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
 Data File : BG052603.D
 Acq On : 8 Mar 2022 13:20
 Operator : CG/JU
 Sample : PB143083BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB143083BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.744	376	384	397	rBV	563338	916688	30.55%	8.354%
2	7.365	652	660	669	rBV	555036	963783	32.12%	8.783%
3	8.217	798	805	813	rVB	105324	176835	5.89%	1.611%
4	9.386	995	1004	1013	rBV	353462	639922	21.33%	5.832%
5	11.054	1281	1288	1298	rBV	133332	249189	8.30%	2.271%
6	13.480	1693	1701	1713	rBV	1005230	1546950	51.56%	14.097%
7	14.861	1929	1936	1947	rBV	225238	364466	12.15%	3.321%
8	16.353	2183	2190	2204	rBV	661155	1096209	36.53%	9.990%
9	17.610	2398	2404	2417	rBV	313194	483198	16.10%	4.403%
10	20.207	2840	2846	2852	rBV	2223823	3000568	100.00%	27.344%
11	21.928	3132	3139	3150	rVB	346442	609597	20.32%	5.555%
12	23.496	3401	3406	3413	rVB4	18030	33952	1.13%	0.309%
13	24.372	3549	3555	3563	rVB4	24088	55530	1.85%	0.506%
14	25.394	3717	3729	3743	rBV2	217031	674984	22.50%	6.151%
15	26.639	3931	3941	3949	rVB5	28379	81523	2.72%	0.743%
16	28.114	4184	4192	4193	rBV5	21820	45719	1.52%	0.417%
17	29.893	4484	4495	4496	rBV9	13770	34382	1.15%	0.313%




Sum of corrected areas: 10973495

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052603.D
Acq On : 8 Mar 2022 13:20
Operator : CG/JU
Sample : PB143083BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143083BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

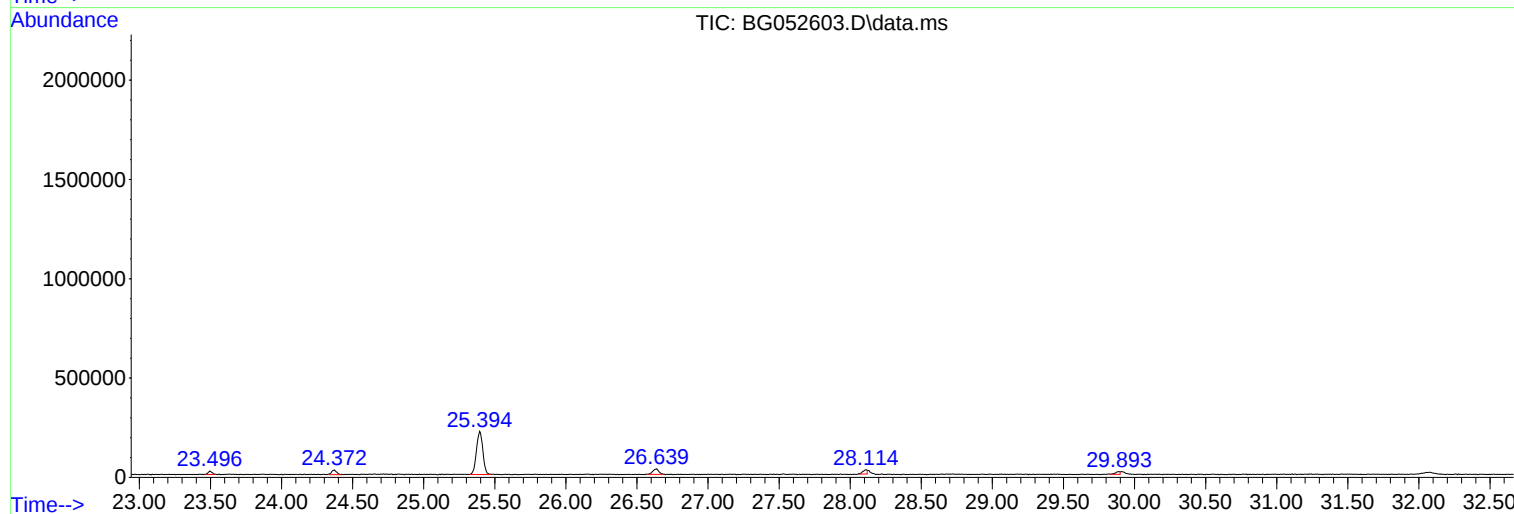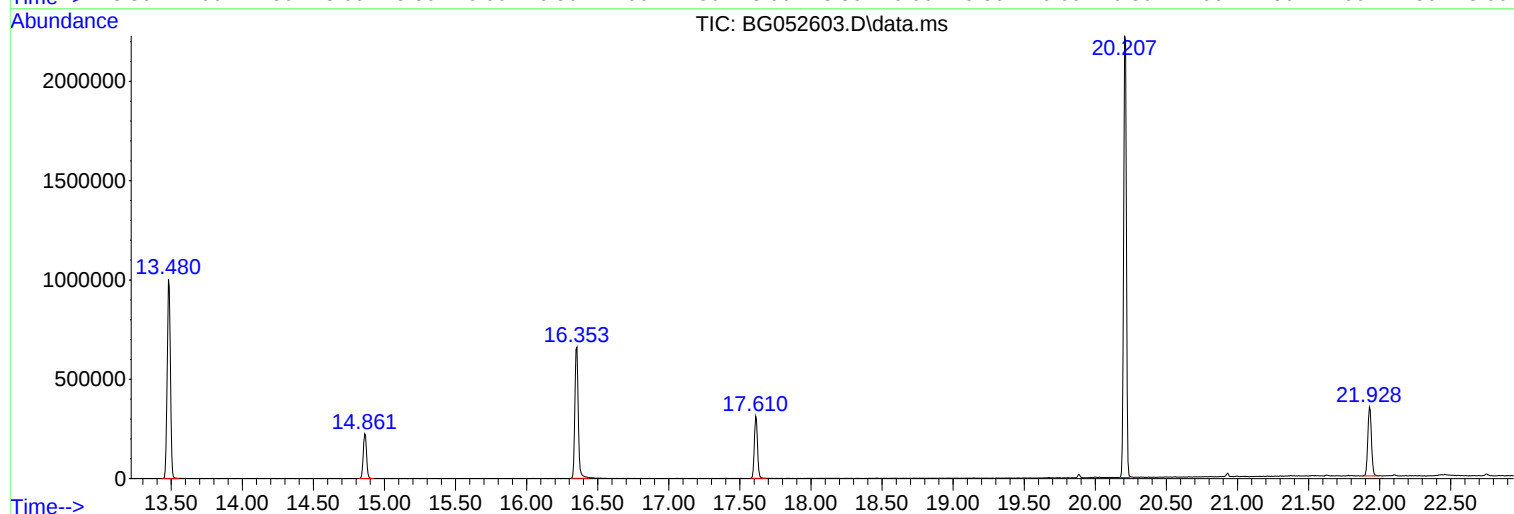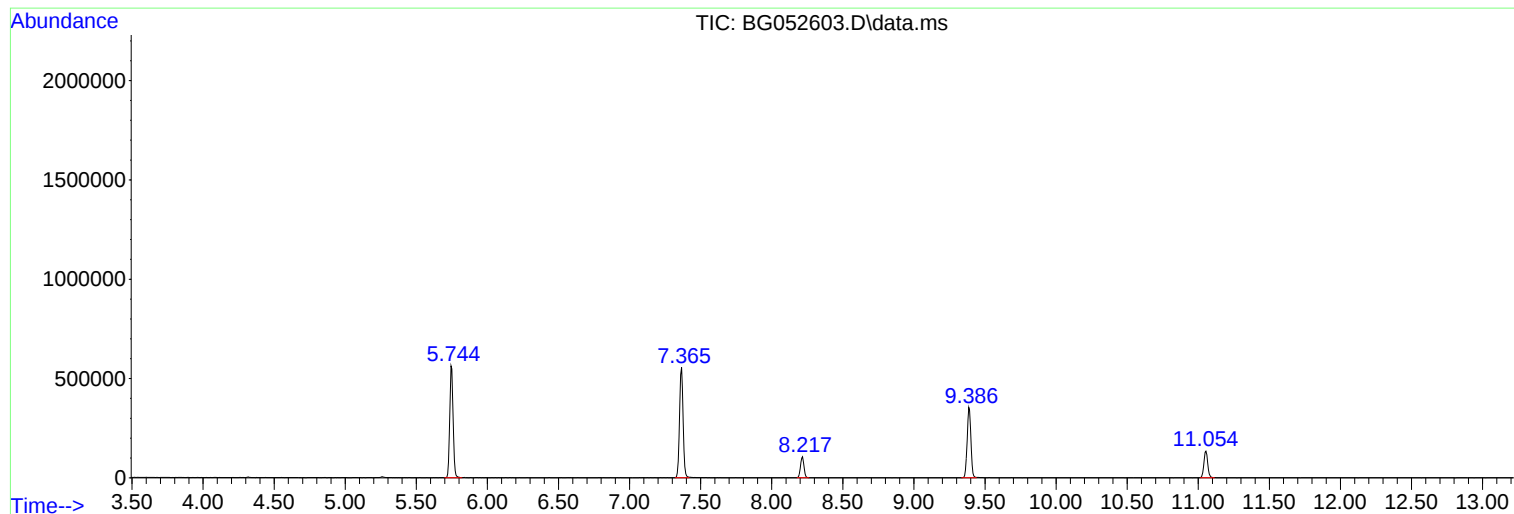

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052603.D
Acq On : 8 Mar 2022 13:20
Operator : CG/JU
Sample : PB143083BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143083BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052603.D
Acq On : 8 Mar 2022 13:20
Operator : CG/JU
Sample : PB143083BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143083BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------