

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
 Data File : BG052612.D
 Acq On : 8 Mar 2022 19:57
 Operator : CG/JU
 Sample : N1825-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DUM-32

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.747	377	384	395	rVB	412395	669350	34.36%	7.994%
2	7.362	651	659	671	rBV	426192	733697	37.66%	8.762%
3	8.214	796	804	810	rBV	96330	162079	8.32%	1.936%
4	9.383	995	1003	1013	rBV	259627	486701	24.98%	5.812%
5	11.051	1278	1287	1295	rBV	129233	239452	12.29%	2.860%
6	13.477	1693	1700	1709	rBV	744970	1156387	59.36%	13.810%
7	14.858	1928	1935	1943	rVB	225030	349094	17.92%	4.169%
8	16.350	2182	2189	2206	rBV	553899	907855	46.60%	10.842%
9	17.613	2396	2404	2409	rBV	298640	471398	24.20%	5.630%
10	19.657	2747	2752	2760	rBV	34089	51812	2.66%	0.619%
11	20.022	2808	2814	2821	rVB	32771	53070	2.72%	0.634%
12	20.204	2839	2845	2851	rBV	1525691	1947992	100.00%	23.264%
13	21.525	3066	3070	3076	rBV6	19827	43246	2.22%	0.516%
14	21.613	3083	3085	3096	rVB5	9708	23099	1.19%	0.276%
15	21.925	3130	3138	3145	rBV	301262	555634	28.52%	6.636%
16	25.385	3716	3727	3740	rVB3	169199	522638	26.83%	6.242%




Sum of corrected areas: 8373504

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052612.D
Acq On : 8 Mar 2022 19:57
Operator : CG/JU
Sample : N1825-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DUM-32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

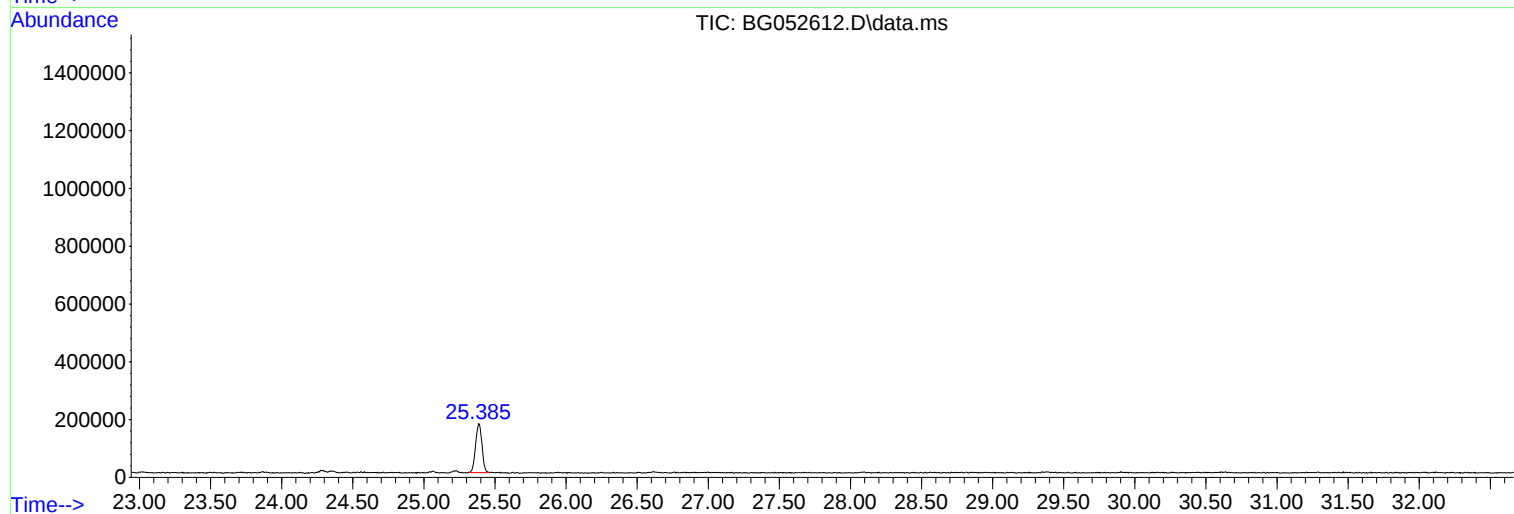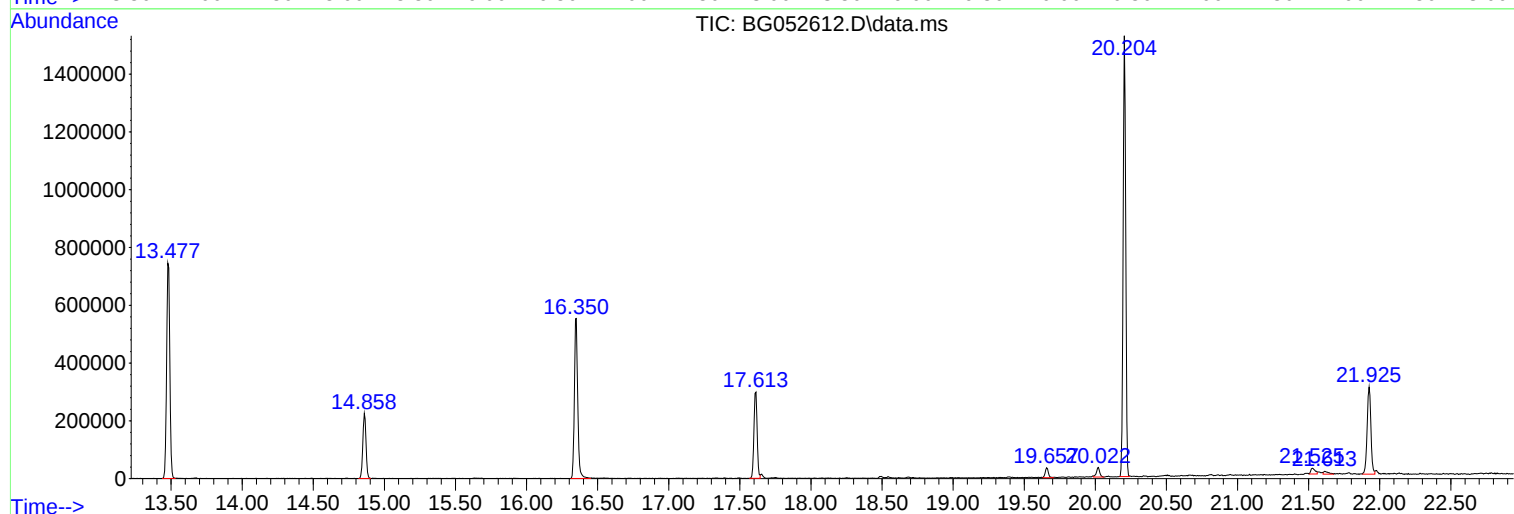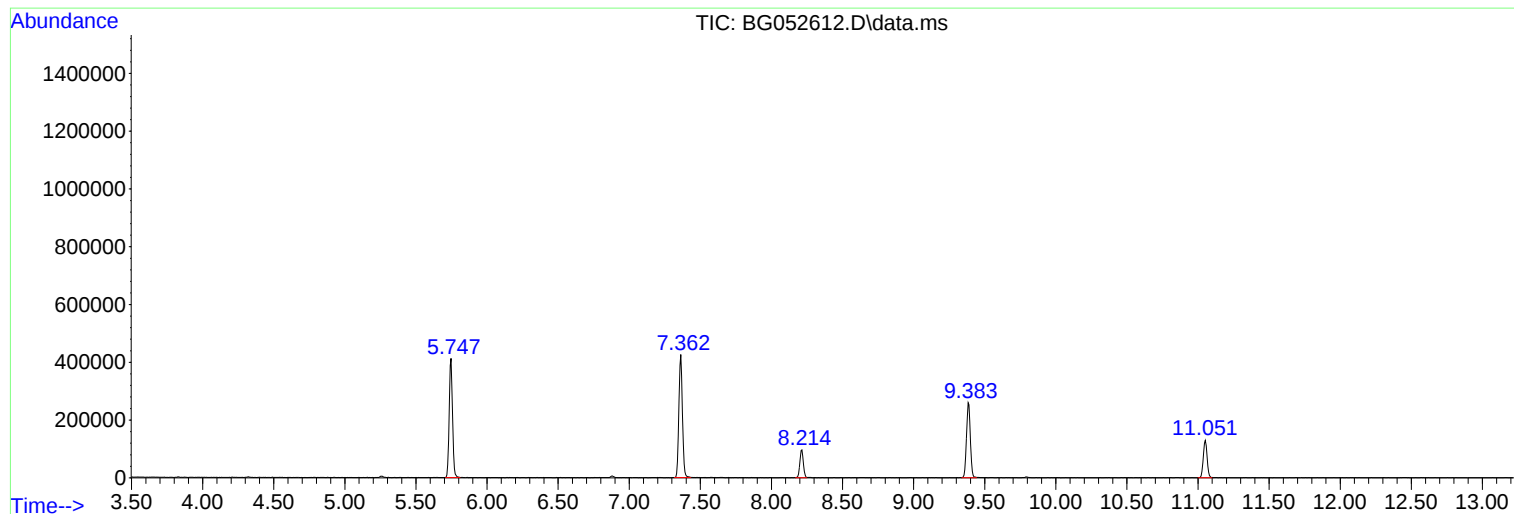

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052612.D
Acq On : 8 Mar 2022 19:57
Operator : CG/JU
Sample : N1825-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DUM-32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052612.D
Acq On : 8 Mar 2022 19:57
Operator : CG/JU
Sample : N1825-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DUM-32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------