


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
 Data File : BG052601.D
 Acq On : 8 Mar 2022 12:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 08 01:09:10 2022

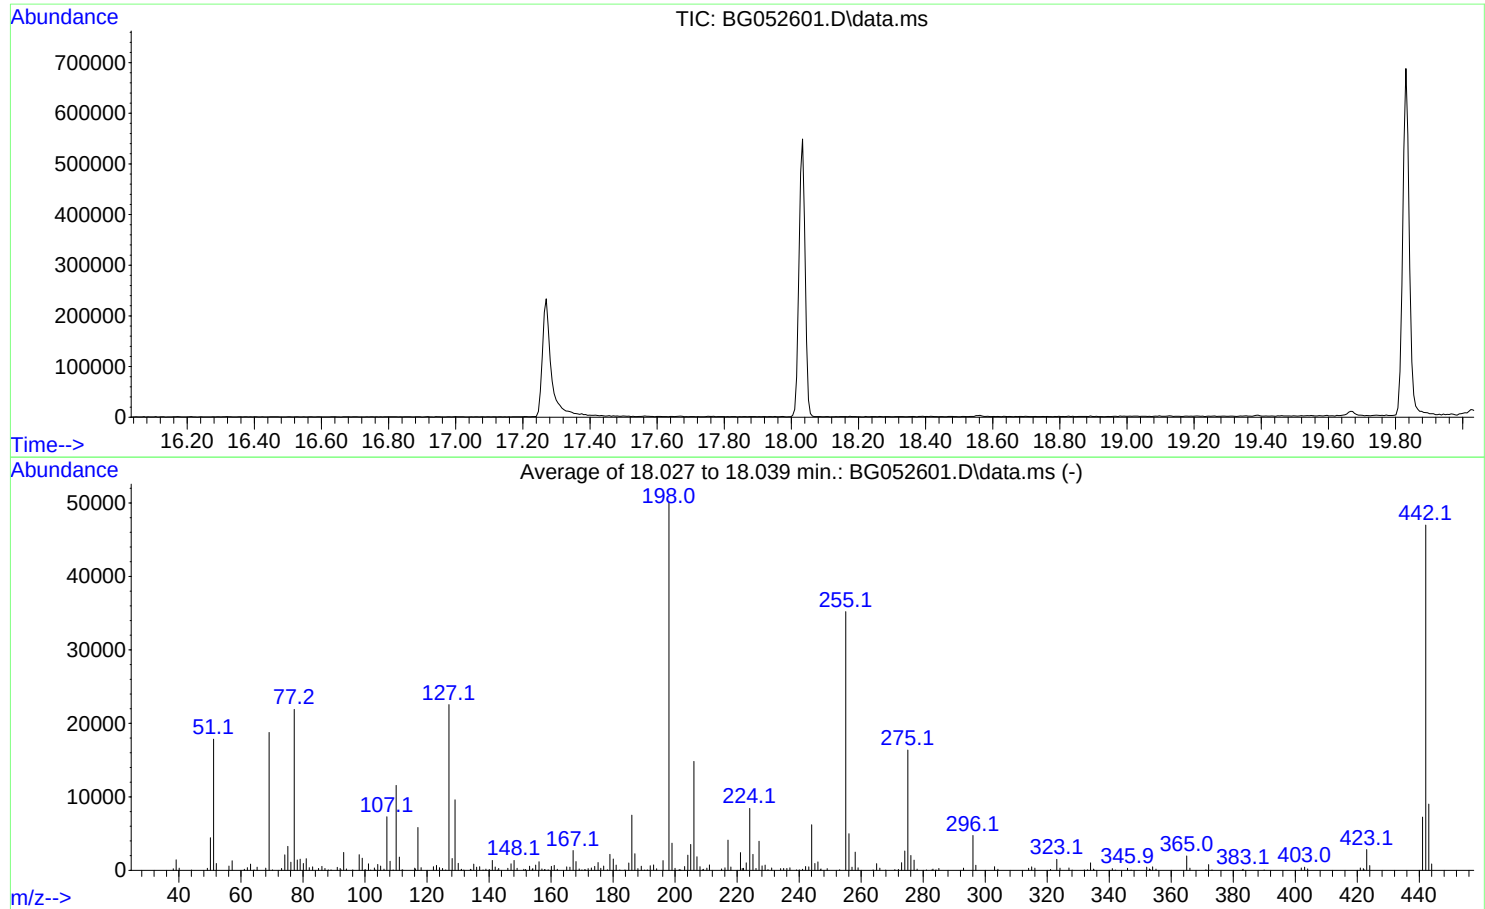




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	17853	PASS
68	69	0.00	2	1.6	303	PASS
69	198	0.00	100	37.5	18775	PASS
70	69	0.00	2	0.3	57	PASS
127	198	10	80	45.1	22563	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50059	PASS
199	198	5	9	7.4	3712	PASS
275	198	10	60	32.7	16371	PASS
365	198	1	100	3.9	1953	PASS
441	198	0.01	100	14.5	7261	PASS
442	442	50	100	100.0	46997	PASS
443	442	15	24	19.2	9013	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
Data File : BG052601.D
Acq On : 8 Mar 2022 12:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 09 05:02:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 08 01:09:10 2022
Response via : Initial Calibration

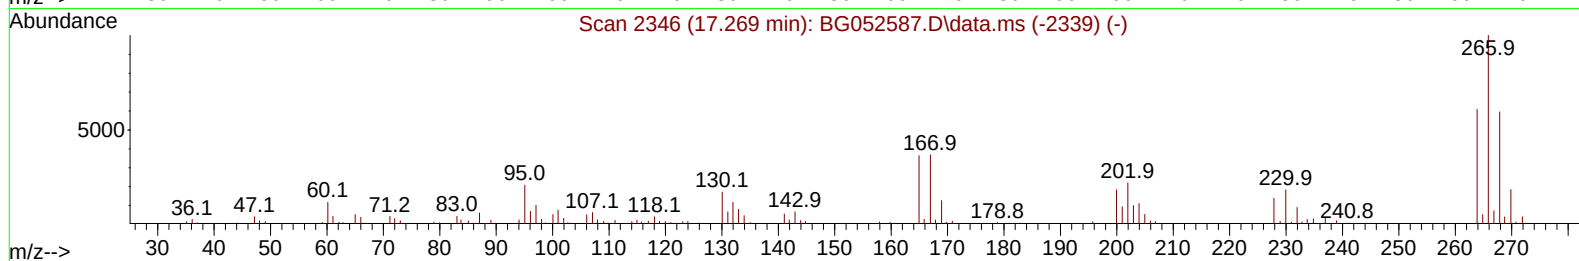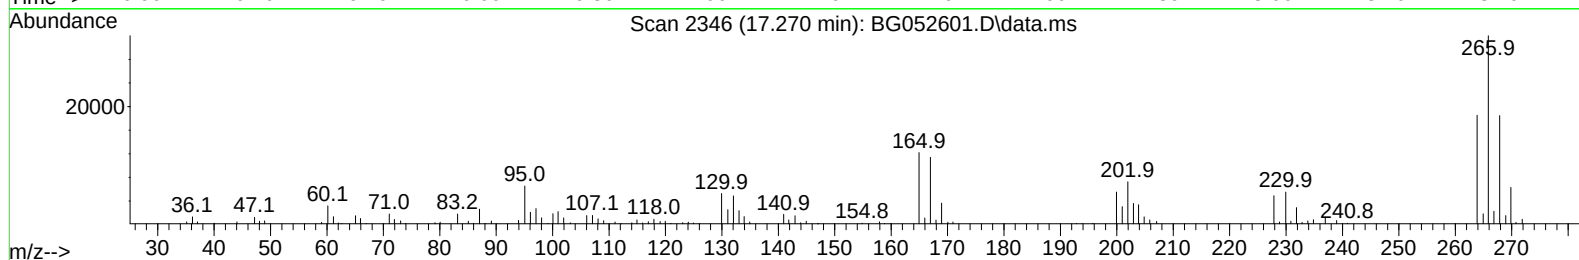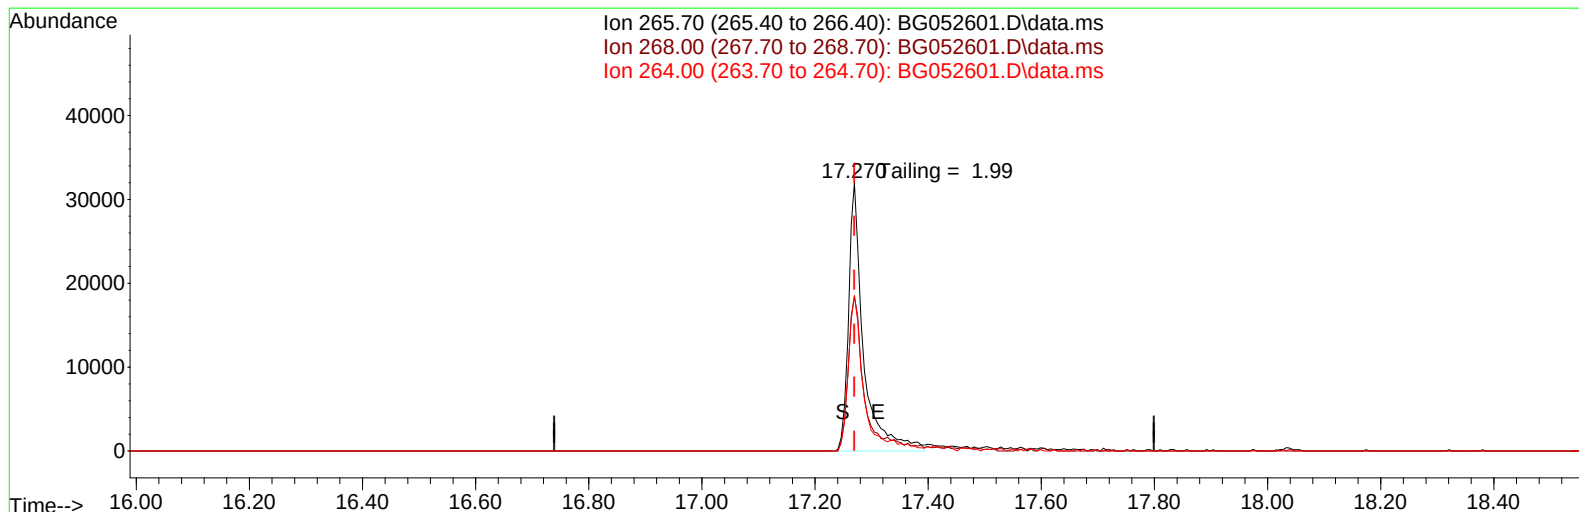

TIC: BG052601.D\data.ms

(70) Pentachlorophenol (C)

17.270min (+ 0.001) 120019.68 ng




response 59115

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	57.70
264.00	65.20	57.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030822\
 Data File : BG052601.D
 Acq On : 8 Mar 2022 12:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 09 05:02:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 08 01:09:10 2022
 Response via : Initial Calibration

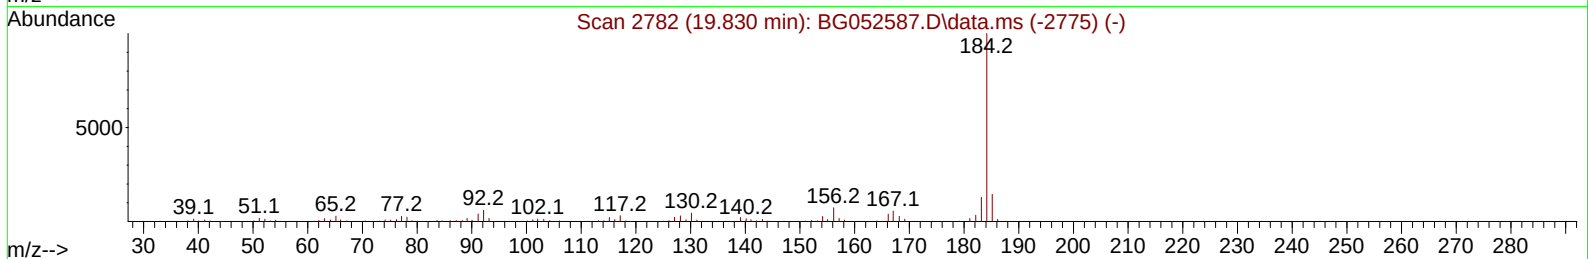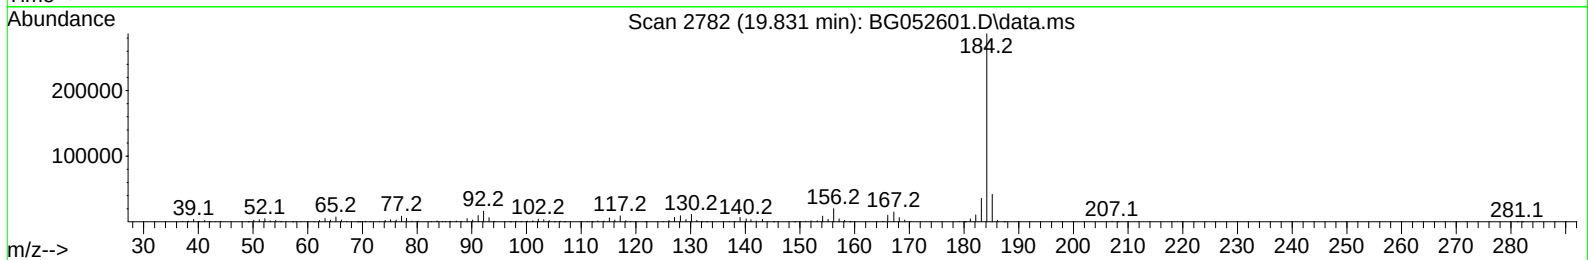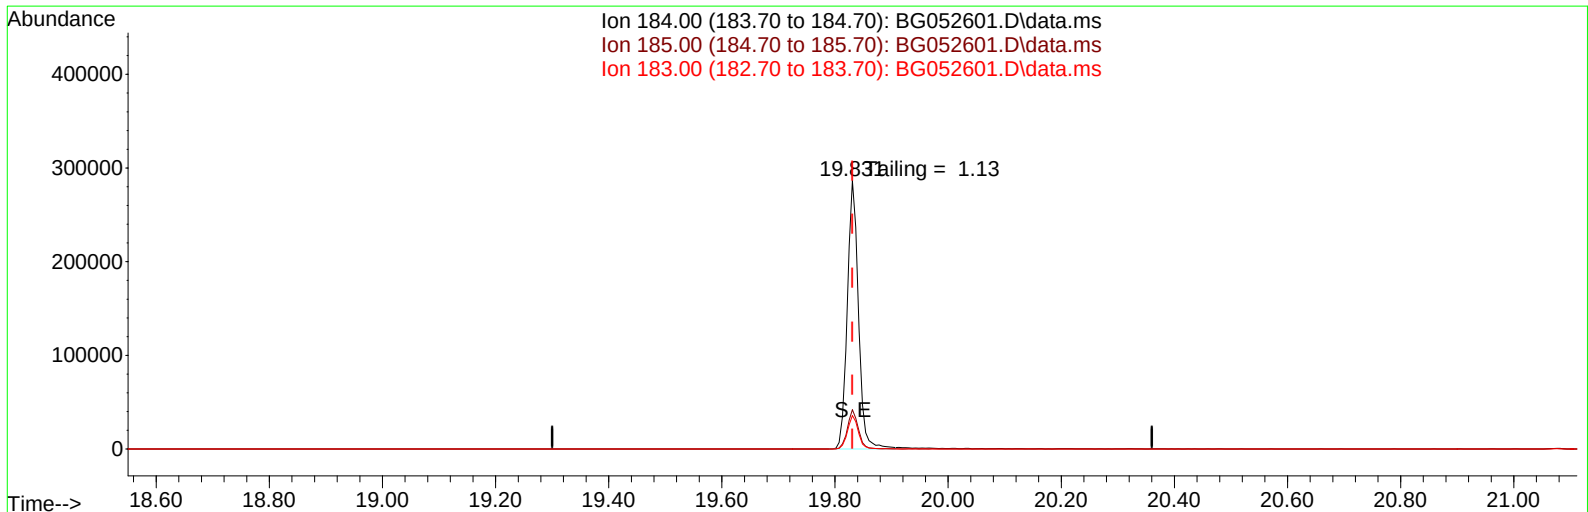

TIC: BG052601.D\data.ms

(77) Benzidine

19.831min (+ 0.001) 22563.44 ng

response 395618

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.66
183.00	12.20	12.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/8/2022	BNA_G	<u>BG052601.D</u>
Compound Name	Response	Retention Time
DDT	206697	21.076
DDD	2181	20.671
DDE	63	20.125
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2244	208941	1.07

Instrument :
BNA_G
ClientSampleId :
DFTPP