

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056909.D
 Acq On : 9 Mar 2023 11:00
 Operator : CG/JU
 Sample : 01713-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Mar 09 11:49:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 08 23:58:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.414	152	15195	20.000	ng/ul	0.00
20) Naphthalene-d8	11.258	136	62370	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.030	164	51851	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.774	188	146997	20.000	ng/ul	0.00
79) Chrysene-d12	22.092	240	145122	20.000	ng/ul	0.00
88) Perylene-d12	25.647	264	154746	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.690	96	862	2.200	ng/uL	0.00
4) Pyridine-d5	4.113	84	145	0.114	ng/ul	-0.02
7) Phenol-d5	7.539	99	17659	11.339	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.715	67	11473	11.728	ng/ul	0.00
11) 2-Chlorophenol-d4	7.938	132	12026	12.338	ng/ul	0.00
15) 4-Methylphenol-d8	9.107	113	9262	7.882	ng/ul	0.00
21) Nitrobenzene-d5	9.589	128	6448	12.465	ng/ul	0.00
24) 2-Nitrophenol-d4	10.324	143	8080	13.203	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.864	165	13779	11.624	ng/ul	0.00
31) 4-Chloroaniline-d4	11.381	131	13394	8.575	ng/ul	0.00
46) Dimethylphthalate-d6	14.413	166	56419	12.721	ng/ul	0.00
49) Acenaphthylene-d8	14.724	160	61002	12.527	ng/ul	0.00
54) 4-Nitrophenol-d4	15.189	143	6098	8.114	ng/ul	0.00
60) Fluorene-d10	16.017	176	52576	12.784	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.117	200	10166	9.569	ng/ul	0.00
73) Anthracene-d10	17.868	188	88100	12.401	ng/ul	0.00
81) Pyrene-d10	20.130	212	121059	13.695	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.394	264	111185	13.122	ng/ul	-0.01
Target Compounds						
					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.934	149	9951	1.990	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056909.D
Acq On : 9 Mar 2023 11:00
Operator : CG/JU
Sample : 01713-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Mar 09 11:49:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 08 23:58:51 2023
Response via : Initial Calibration

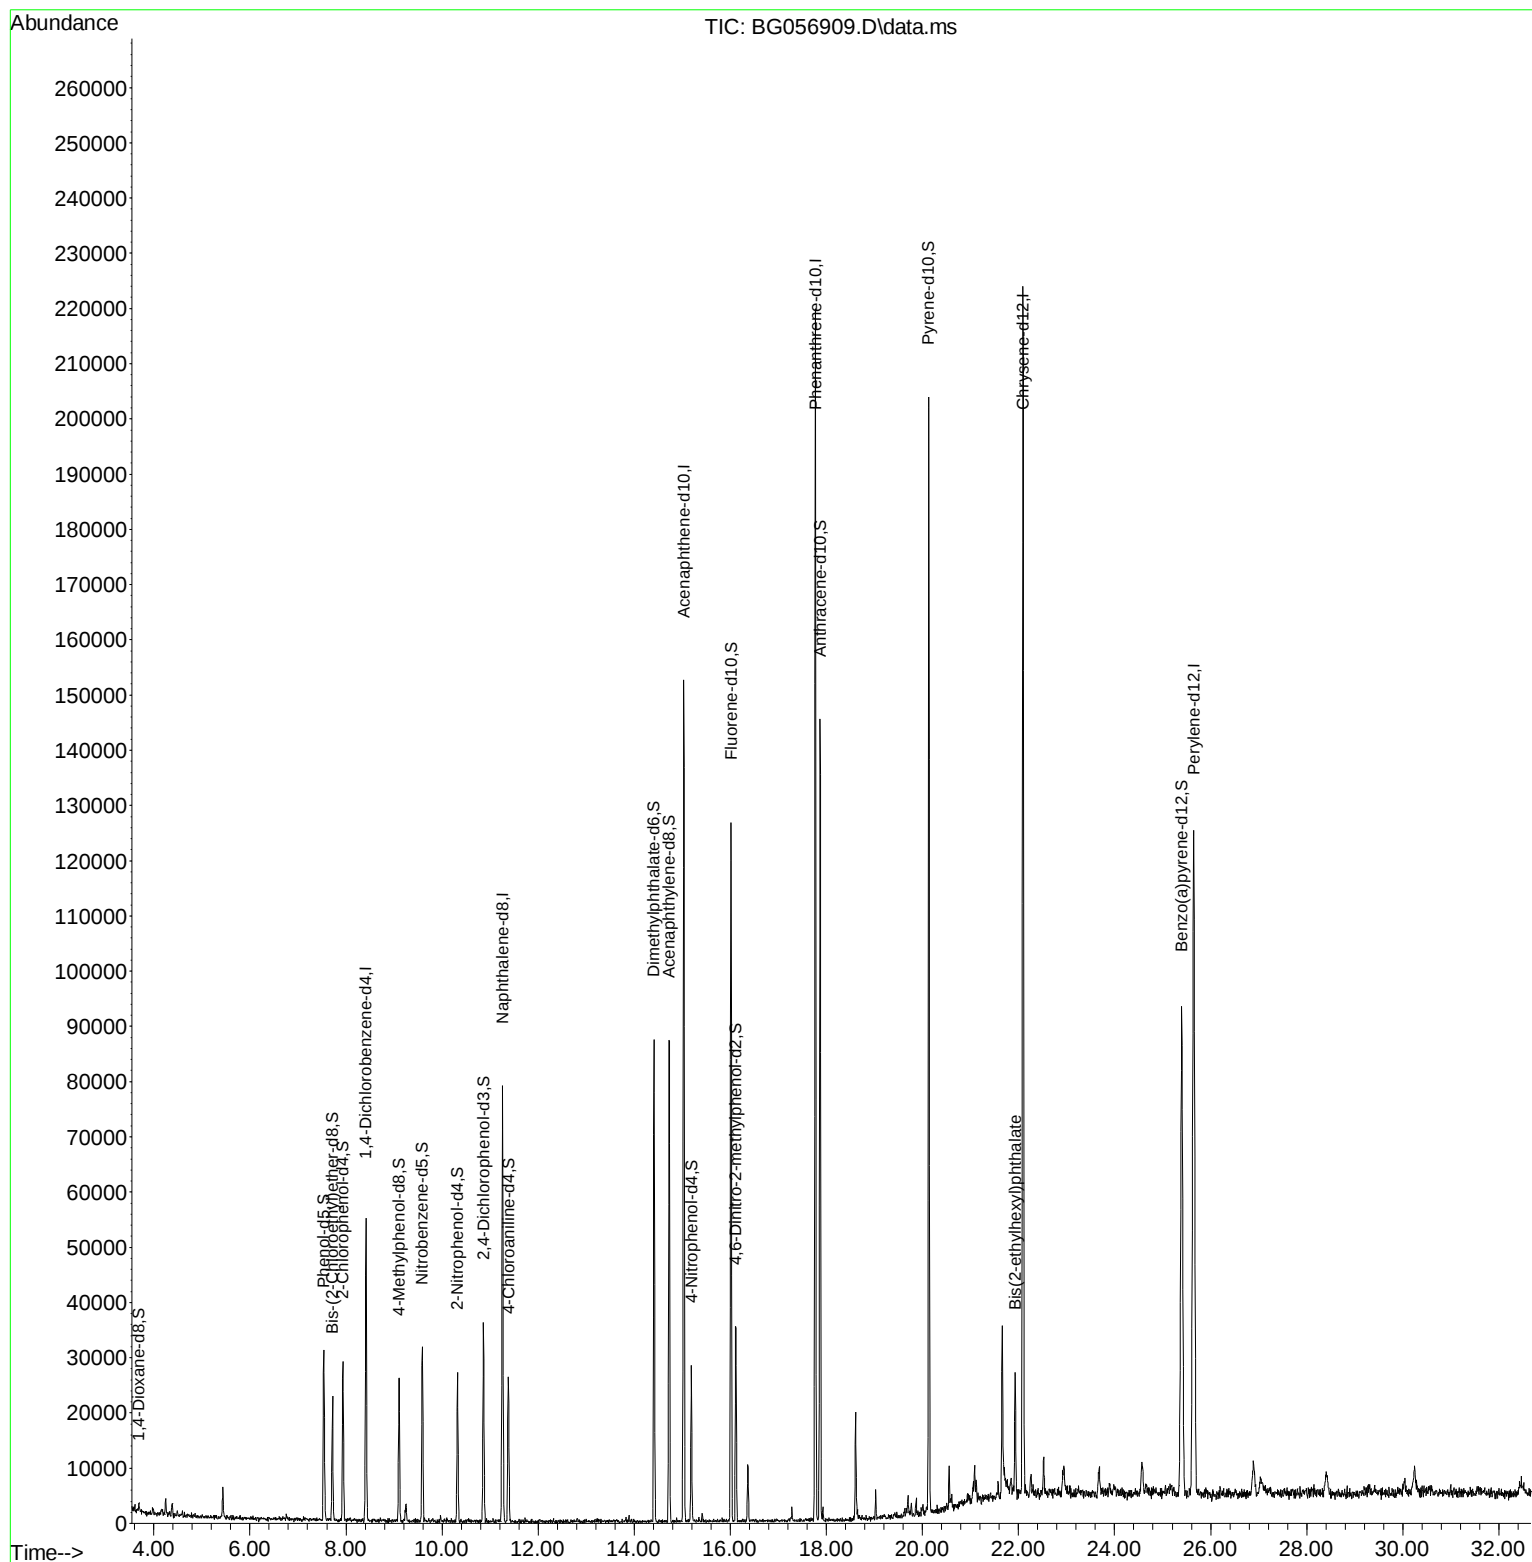

Abundance Scan 3130 (21.928 min): BG056901.D\data.ms (-3126) (-)

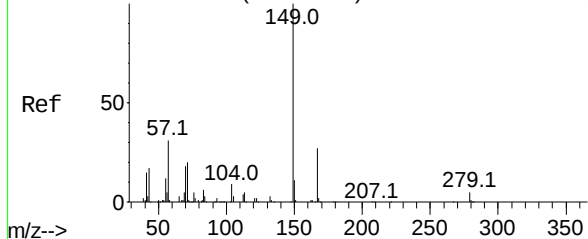

Bis(2-ethylhexyl)phthalate

Concen: 1.990 ng/ul

RT: 21.934 min Scan# 3131

Delta R.T. -0.006 min

Lab File: BG056909.D


Acq: 9 Mar 2023 11:00

Instrument :

BNA_G

ClientSampleId :

Abundance Scan 3131 (21.934 min): BG056909.D\data.ms

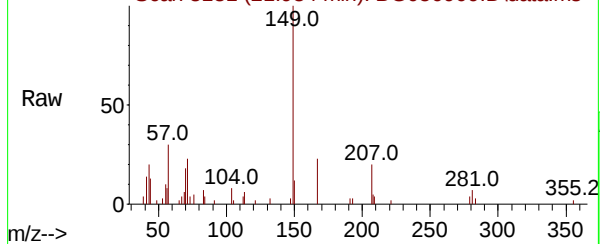


Tgt Ion:149 Resp: 9951

Ion Ratio Lower Upper

149 100

167 23.4 20.3 30.5

279 4.3 4.0 6.0

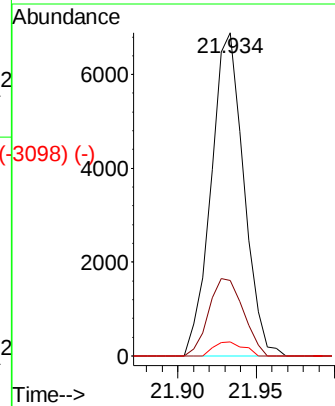

Abundance Scan 3131 (21.934 min): BG056909.D\data.ms (-3098) (-)

