




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056889.D
 Acq On : 8 Mar 2023 20:35
 Operator : CG/JU
 Sample : 01784-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAD8

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:01:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 08 23:58:51 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

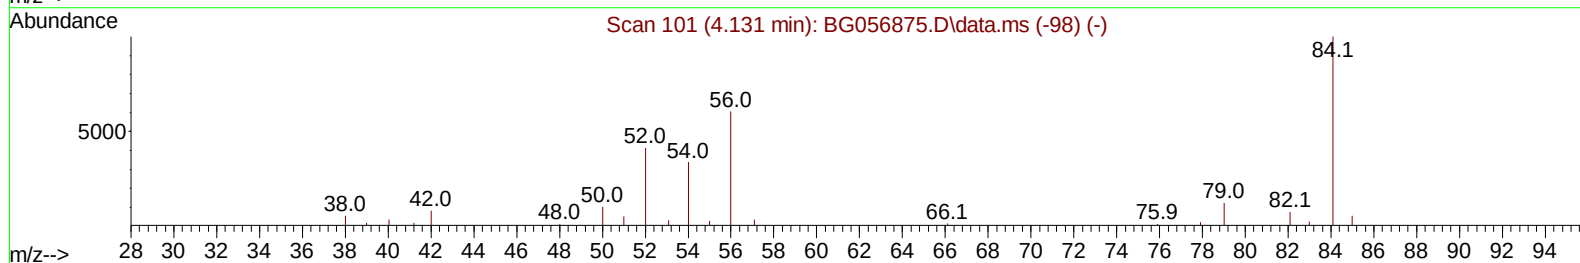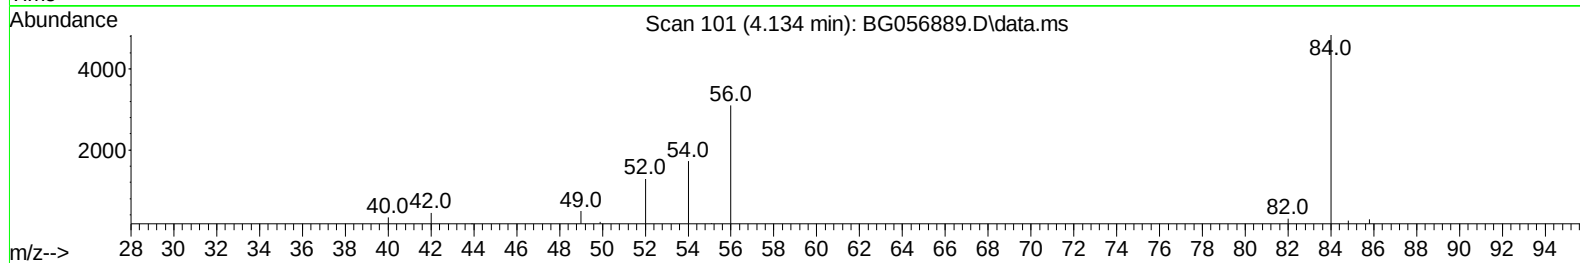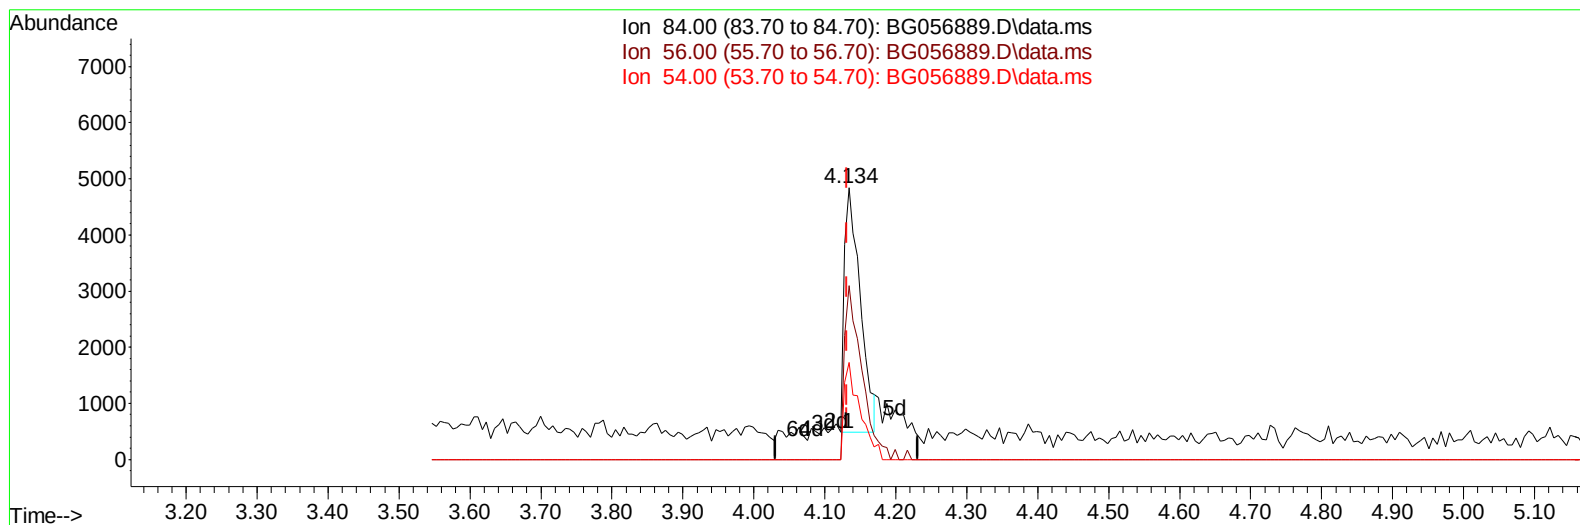

TIC: BG056889.D\data.ms

(4) Pyridine-d5 (S)

4.134min (+ 0.003) 5.79 ng/u1

response 6743

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	69.50	64.06
54.00	34.90	35.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056889.D
 Acq On : 8 Mar 2023 20:35
 Operator : CG/JU
 Sample : 01784-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAD8

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:01:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 08 23:58:51 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

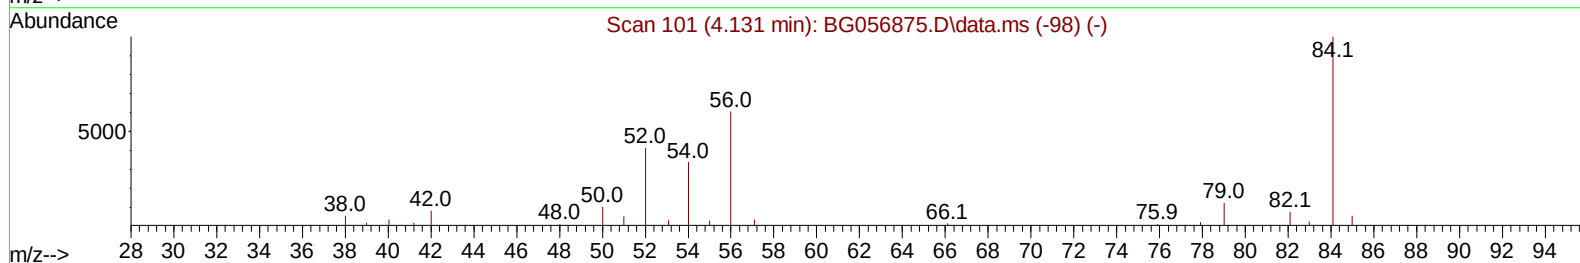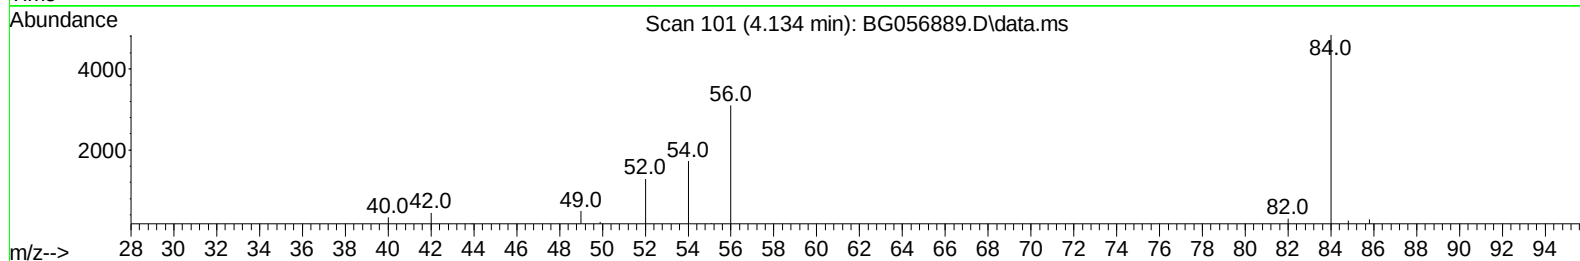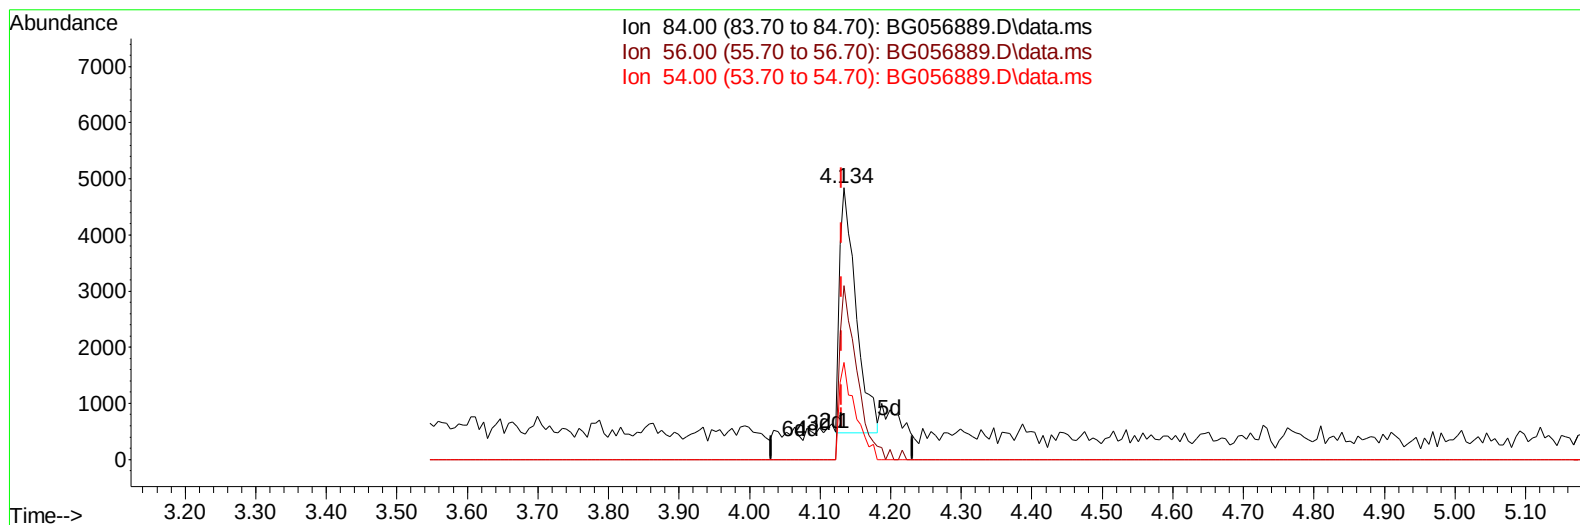

TIC: BG056889.D\data.ms

(4) Pyridine-d5 (S)

4.134min (+ 0.003) 6.06 ng/ul m

response 7060

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	69.50	64.06
54.00	34.90	35.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056889.D
 Acq On : 8 Mar 2023 20:35
 Operator : CG/JU
 Sample : 01784-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

DCAD8

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:01:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 08 23:58:51 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.417	152		13885	20.000	ng/ul	0.00
20) Naphthalene-d8	11.261	136		57514	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	15.033	164		46277	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.771	188		125419	20.000	ng/ul	0.00
79) Chrysene-d12	22.095	240		128960	20.000	ng/ul	0.00
88) Perylene-d12	25.644	264		141215	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.693	96		1129	3.153	ng/uL	0.00
4) Pyridine-d5	4.134	84		7060m	6.061	ng/ul	0.00
7) Phenol-d5	7.542	99		6323	4.443	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.718	67		23973	26.819	ng/ul	0.00
11) 2-Chlorophenol-d4	7.936	132		17947	20.150	ng/ul	0.00
15) 4-Methylphenol-d8	9.105	113		12906	12.019	ng/ul	0.00
21) Nitrobenzene-d5	9.592	128		13345	27.975	ng/ul	0.00
24) 2-Nitrophenol-d4	10.321	143		14452	25.609	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.862	165		27725	25.364	ng/ul	0.00
31) 4-Chloroaniline-d4	11.379	131		23824	16.541	ng/ul	0.00
46) Dimethylphthalate-d6	14.416	166		128338	32.422	ng/ul	0.00
49) Acenaphthylene-d8	14.728	160		125356	28.842	ng/ul	0.00
54) 4-Nitrophenol-d4	15.192	143		3921	5.846	ng/ul	0.00
60) Fluorene-d10	16.014	176		111863	30.476	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.120	200		29053	32.053	ng/ul	0.00
73) Anthracene-d10	17.871	188		203533	33.577	ng/ul	0.00
81) Pyrene-d10	20.133	212		264471	33.669	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.403	264		263437	34.069	ng/ul	0.00
Target Compounds							
						Qvalue	
30) Naphthalene	11.314	128		342606	107.840	ng/ul	98
36) 2-Methylnaphthalene	12.883	142		22508	9.849	ng/ul	89
37) 1-Methylnaphthalene	13.100	142		35670	15.622	ng/ul	94
42) 2,4,5-Trichlorophenol	13.547	196		2862	2.309	ng/ul#	90
43) 1,1'-Biphenyl	13.870	154		30077	8.678	ng/ul	98
50) Acenaphthylene	14.757	152		8844	2.014	ng/ul	97
52) Acenaphthene	15.098	153		96881	31.537	ng/ul	95
56) Dibenzofuran	15.427	168		54761	11.661	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.644	232		7777	6.510	ng/ul#	98
61) Fluorene	16.073	166		9388	2.510	ng/ul#	93
71) Pentachlorophenol	17.413	266		30334	30.496	ng/ul	98
72) Phenanthrene	17.812	178		59116	8.759	ng/ul	98
74) Anthracene	17.906	178		8149	1.185	ng/ul	98
77) Carbazole	18.165	167		147532	25.284	ng/ul	100
80) Fluoranthene	19.798	202		16164	1.726	ng/ul	97
82) Pyrene	20.162	202		10015	1.068	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056889.D
Acq On : 8 Mar 2023 20:35
Operator : CG/JU
Sample : 01784-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAD8

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:01:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 08 23:58:51 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

