




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056902.D
Acq On : 9 Mar 2023 6:11
Operator : CG/JU
Sample : PB151262BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK262

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

Quant Time: Mar 09 06:51:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 08 23:58:51 2023
Response via : Initial Calibration

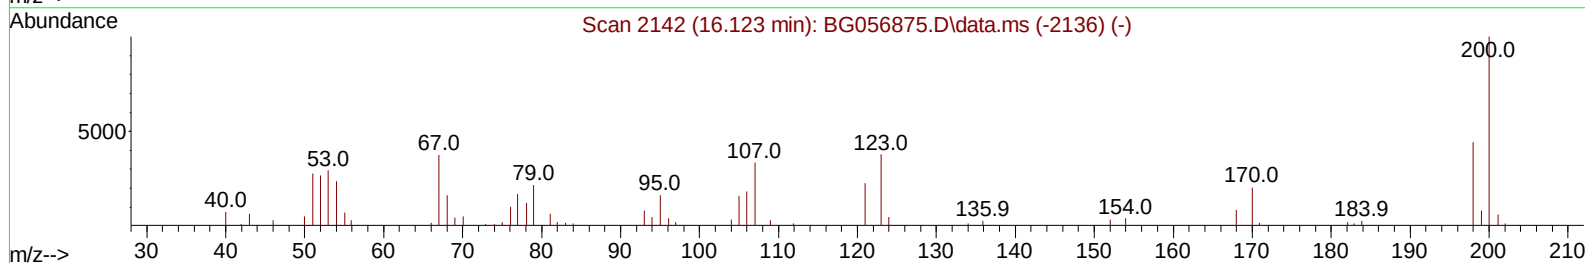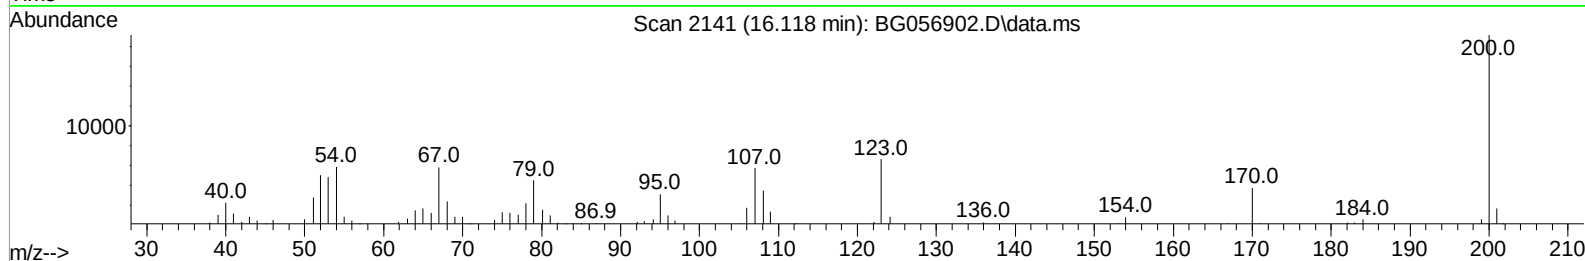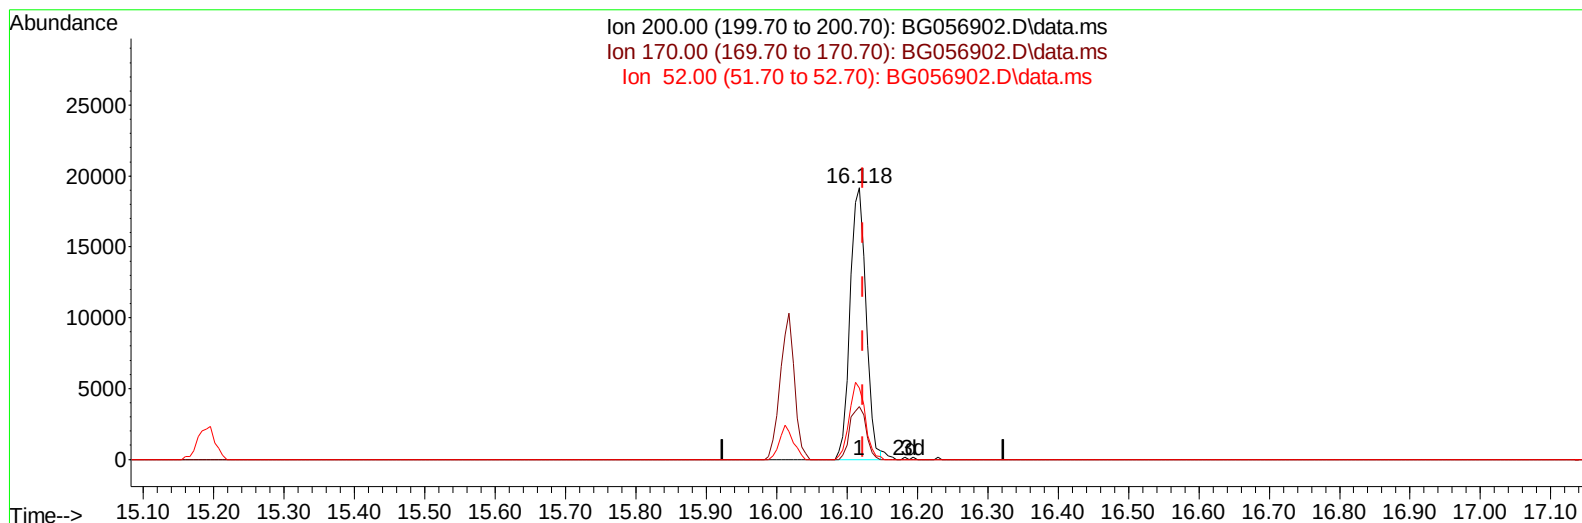

TIC: BG056902.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

16.118min (-0.005) 31.67 ng/uI

response 29917

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.70	19.56
52.00	37.80	26.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056902.D
Acq On : 9 Mar 2023 6:11
Operator : CG/JU
Sample : PB151262BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK262

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

Quant Time: Mar 09 06:51:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 08 23:58:51 2023
Response via : Initial Calibration

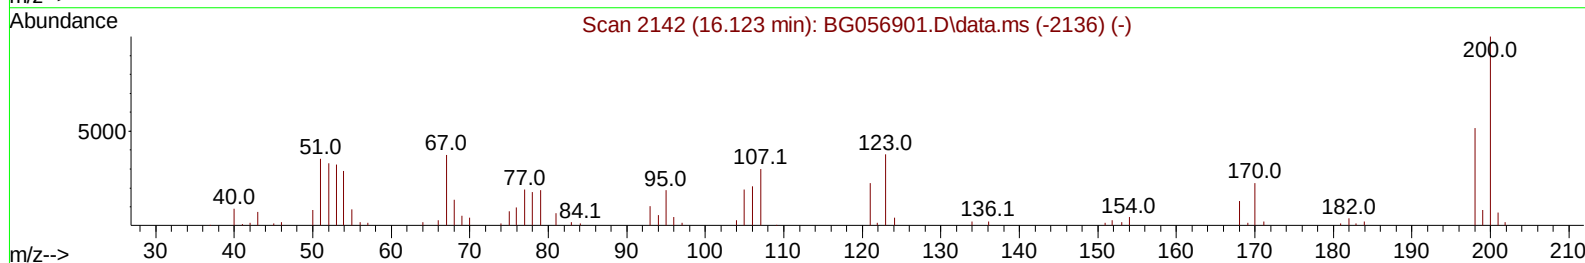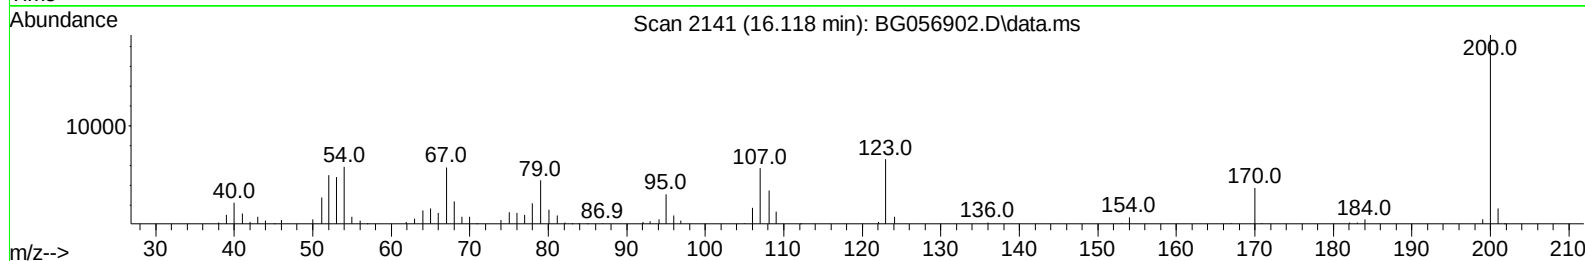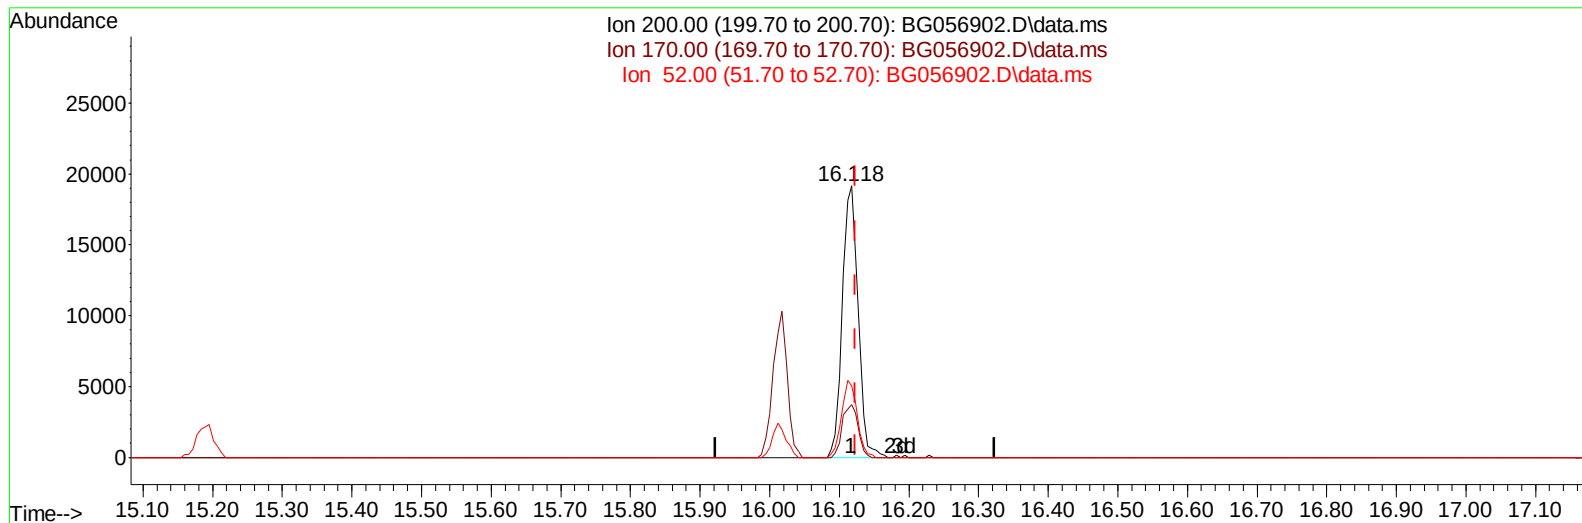

TIC: BG056902.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

16.118min (-0.005) 32.02 ng/ul m

response 30246

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.70	19.56
52.00	37.80	26.41#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056902.D
 Acq On : 9 Mar 2023 6:11
 Operator : CG/JU
 Sample : PB151262BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK262

Manual IntegrationsAPPROVED

Quant Time: Mar 09 06:51:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 08 23:58:51 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.415	152	12511	20.000	ng/ul	0.00
20) Naphthalene-d8	11.259	136	52098	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.031	164	44124	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.769	188	130710	20.000	ng/ul	0.00
79) Chrysene-d12	22.093	240	134441	20.000	ng/ul	# 0.00
88) Perylene-d12	25.642	264	141708	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.691	96	2709	8.397	ng/uL	0.00
4) Pyridine-d5	4.126	84	39456	37.595	ng/ul	0.00
7) Phenol-d5	7.539	99	44907	35.021	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.716	67	29002	36.008	ng/ul	0.00
11) 2-Chlorophenol-d4	7.939	132	30191	37.620	ng/ul	0.00
15) 4-Methylphenol-d8	9.102	113	32526	33.617	ng/ul	0.00
21) Nitrobenzene-d5	9.590	128	15598	36.098	ng/ul	0.00
24) 2-Nitrophenol-d4	10.319	143	19831	38.794	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.859	165	33781	34.117	ng/ul	0.00
31) 4-Chloroaniline-d4	11.376	131	46639	35.747	ng/ul	0.00
46) Dimethylphthalate-d6	14.414	166	143973	38.147	ng/ul	0.00
49) Acenaphthylene-d8	14.725	160	147603	35.618	ng/ul	0.00
54) 4-Nitrophenol-d4	15.189	143	26183	40.941	ng/ul	0.00
60) Fluorene-d10	16.018	176	127020	36.293	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.118	200	30246m	32.018	ng/ul	0.00
73) Anthracene-d10	17.869	188	238314	37.724	ng/ul	0.00
81) Pyrene-d10	20.131	212	305088	37.256	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.395	264	295492	38.082	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056902.D
Acq On : 9 Mar 2023 6:11
Operator : CG/JU
Sample : PB151262BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK262

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

Quant Time: Mar 09 06:51:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 08 23:58:51 2023
Response via : Initial Calibration

