




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056910.D
Acq On : 9 Mar 2023 11:41
Operator : CG/JU
Sample : 01713-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZY7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 01:25:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 08 23:58:51 2023
Response via : Initial Calibration

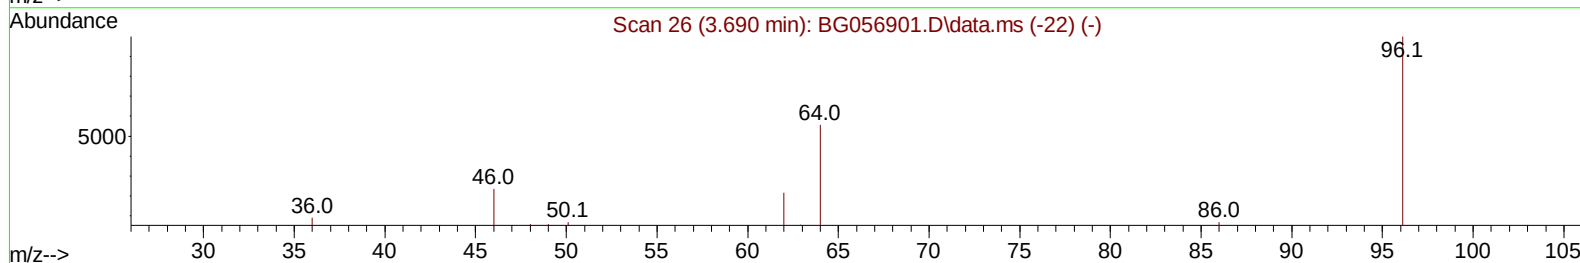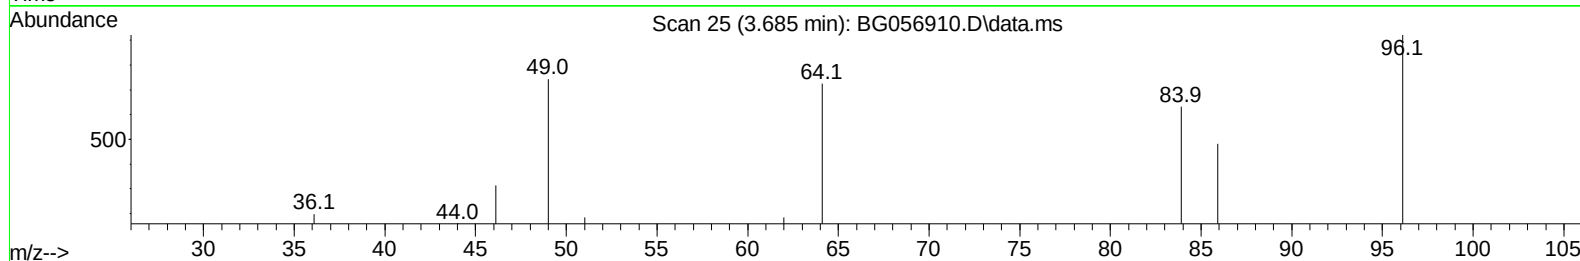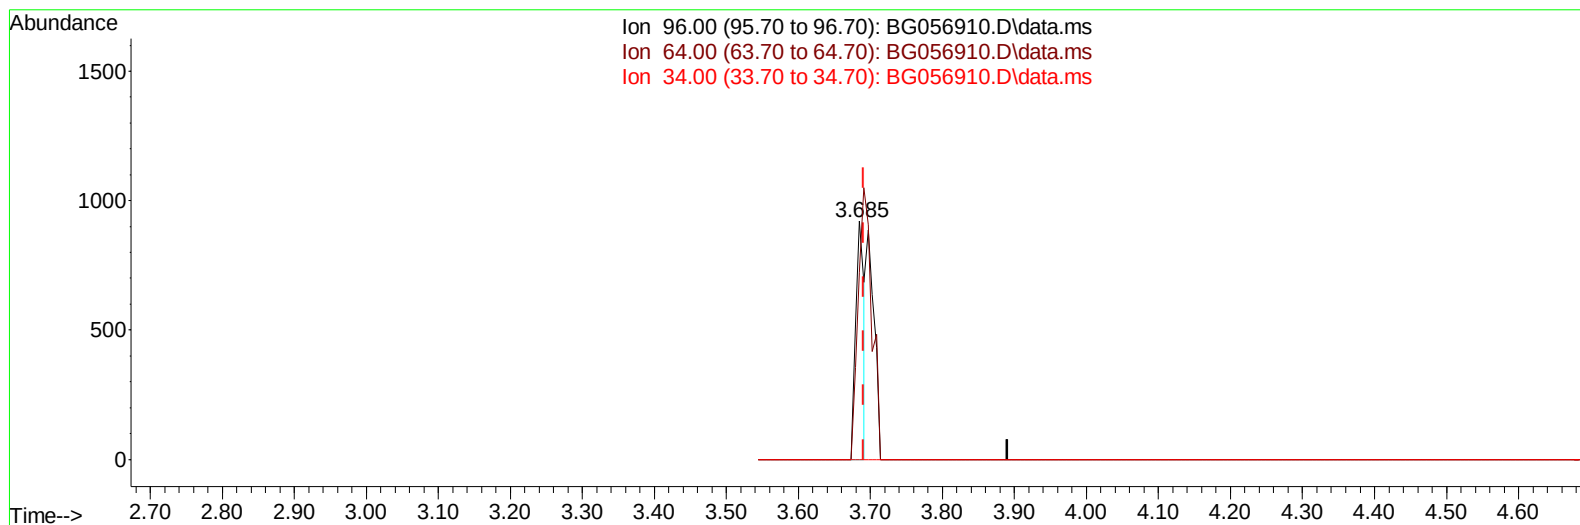

TIC: BG056910.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.685min (-0.006) 2.08 ng/uL****response 750**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.00	78.61
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056910.D
 Acq On : 9 Mar 2023 11:41
 Operator : CG/JU
 Sample : 01713-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZY7

Manual IntegrationsAPPROVED

Quant Time: Mar 10 01:25:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 08 23:58:51 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

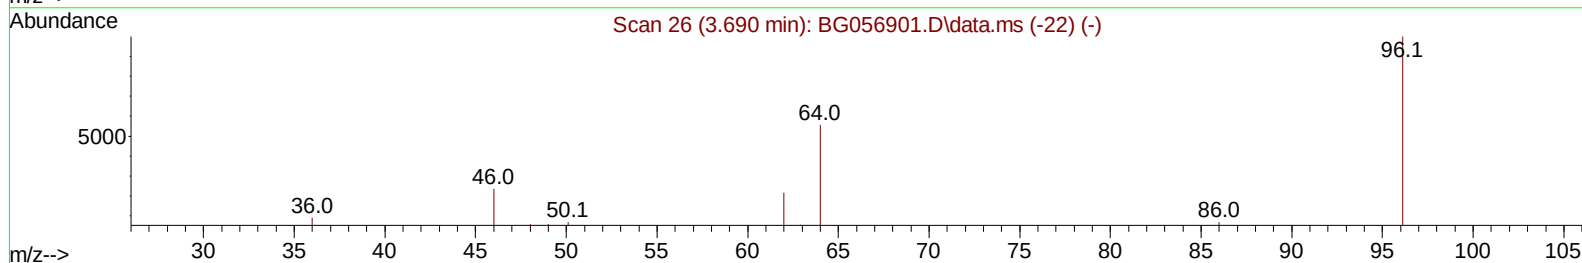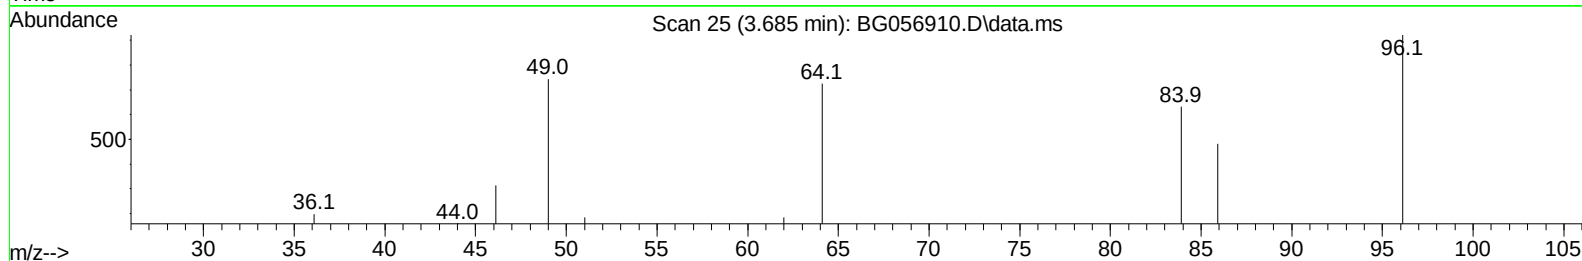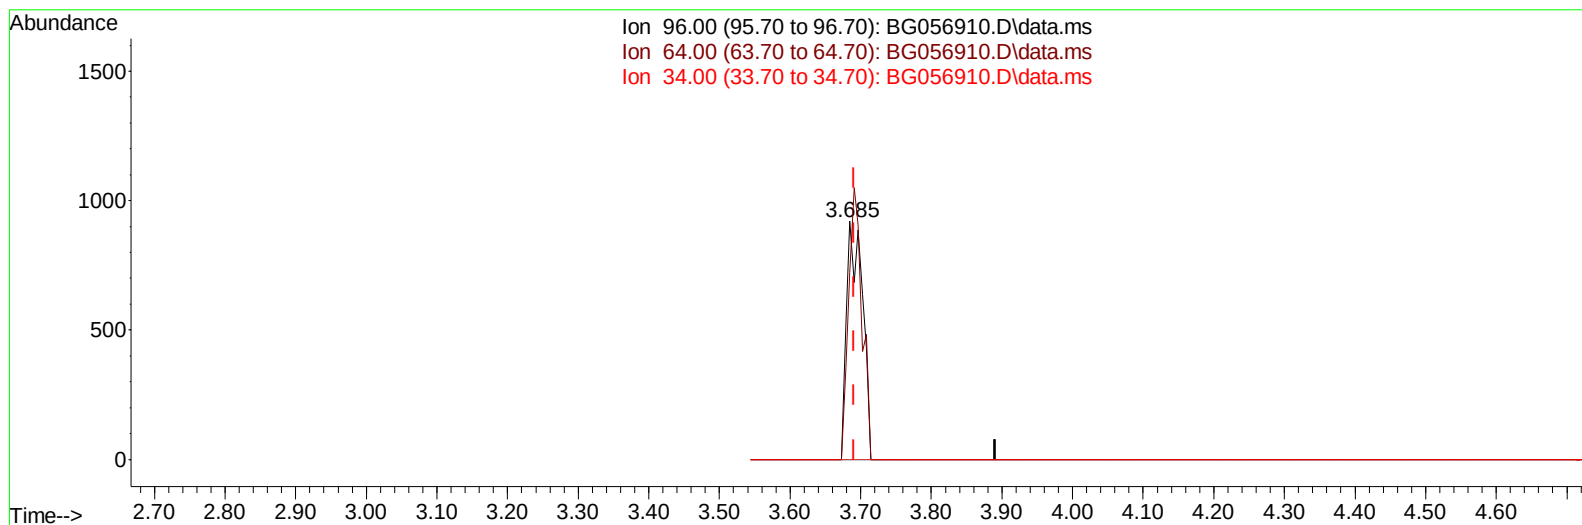

TIC: BG056910.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.685min (-0.006) 4.00 ng/uL m

response 1440

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.00	78.61
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056910.D
 Acq On : 9 Mar 2023 11:41
 Operator : CG/JU
 Sample : 01713-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZY7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 01:25:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 08 23:58:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.420	152	13972	20.000	ng/ul	0.00
20) Naphthalene-d8	11.258	136	60044	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.030	164	50351	20.000	ng/ul	# 0.00
64) Phenanthrene-d10	17.768	188	139449	20.000	ng/ul	0.00
79) Chrysene-d12	22.093	240	137925	20.000	ng/ul	0.00
88) Perylene-d12	25.641	264	151439	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.685	96	1440m	3.997	ng/uL	0.00
4) Pyridine-d5	4.131	84	27241	23.242	ng/ul	0.00
7) Phenol-d5	7.539	99	33825	23.620	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.715	67	21077	23.432	ng/ul	0.00
11) 2-Chlorophenol-d4	7.939	132	21536	24.029	ng/ul	0.00
15) 4-Methylphenol-d8	9.102	113	25336	23.447	ng/ul	0.00
21) Nitrobenzene-d5	9.590	128	12279	24.656	ng/ul	0.00
24) 2-Nitrophenol-d4	10.324	143	13977	23.724	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.865	165	27619	24.202	ng/ul	0.00
31) 4-Chloroaniline-d4	11.382	131	34416	22.888	ng/ul	0.00
46) Dimethylphthalate-d6	14.413	166	102128	23.713	ng/ul	0.00
49) Acenaphthylene-d8	14.731	160	110405	23.347	ng/ul	0.00
54) 4-Nitrophenol-d4	15.189	143	19109	26.184	ng/ul	0.00
60) Fluorene-d10	16.017	176	95135	23.821	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.117	200	21760	21.591	ng/ul	0.00
73) Anthracene-d10	17.868	188	164319	24.381	ng/ul	0.00
81) Pyrene-d10	20.136	212	208205	24.783	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.395	264	201232	24.268	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056910.D
Acq On : 9 Mar 2023 11:41
Operator : CG/JU
Sample : 01713-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZY7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 01:25:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 08 23:58:51 2023
Response via : Initial Calibration

