

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056881.D
 Acq On : 8 Mar 2023 14:18
 Operator : CG/JU
 Sample : 01784-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAD6

Quant Time: Mar 08 14:58:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 07 23:54:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.414	152	13407	20.000	ng/u1	0.00
20) Naphthalene-d8	11.258	136	54005	20.000	ng/u1	0.00
38) Acenaphthene-d10	15.036	164	44429	20.000	ng/u1	# 0.00
64) Phenanthrene-d10	17.774	188	125252	20.000	ng/u1	0.00
79) Chrysene-d12	22.098	240	127658	20.000	ng/u1	-0.01
88) Perylene-d12	25.647	264	137216	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.690	96	1508	4.362	ng/uL	0.00
4) Pyridine-d5	4.142	84	6505	5.784	ng/u1	0.01
7) Phenol-d5	7.544	99	7807	5.681	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.721	67	23605	27.349	ng/u1	0.00
11) 2-Chlorophenol-d4	7.938	132	18820	21.884	ng/u1	0.00
15) 4-Methylphenol-d8	9.107	113	13711	13.224	ng/u1	0.00
21) Nitrobenzene-d5	9.595	128	13588	30.336	ng/u1	0.00
24) 2-Nitrophenol-d4	10.323	143	15499	29.249	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.864	165	25199	24.551	ng/u1	0.00
31) 4-Chloroaniline-d4	11.381	131	25311	18.715	ng/u1	0.00
46) Dimethylphthalate-d6	14.419	166	114811	30.211	ng/u1	0.00
49) Acenaphthylene-d8	14.730	160	119705	28.688	ng/u1	0.00
54) 4-Nitrophenol-d4	15.188	143	4333	6.729	ng/u1	-0.01
60) Fluorene-d10	16.017	176	104928	29.775	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.117	200	26355	29.115	ng/u1	0.00
73) Anthracene-d10	17.873	188	206404	34.096	ng/u1	0.00
81) Pyrene-d10	20.135	212	266106	34.222	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.400	264	253965	33.802	ng/u1	-0.02
Target Compounds						
30) Naphthalene	11.311	128	9534	3.196	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056881.D
Acq On : 8 Mar 2023 14:18
Operator : CG/JU
Sample : 01784-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAD6

Quant Time: Mar 08 14:58:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 07 23:54:44 2023
Response via : Initial Calibration

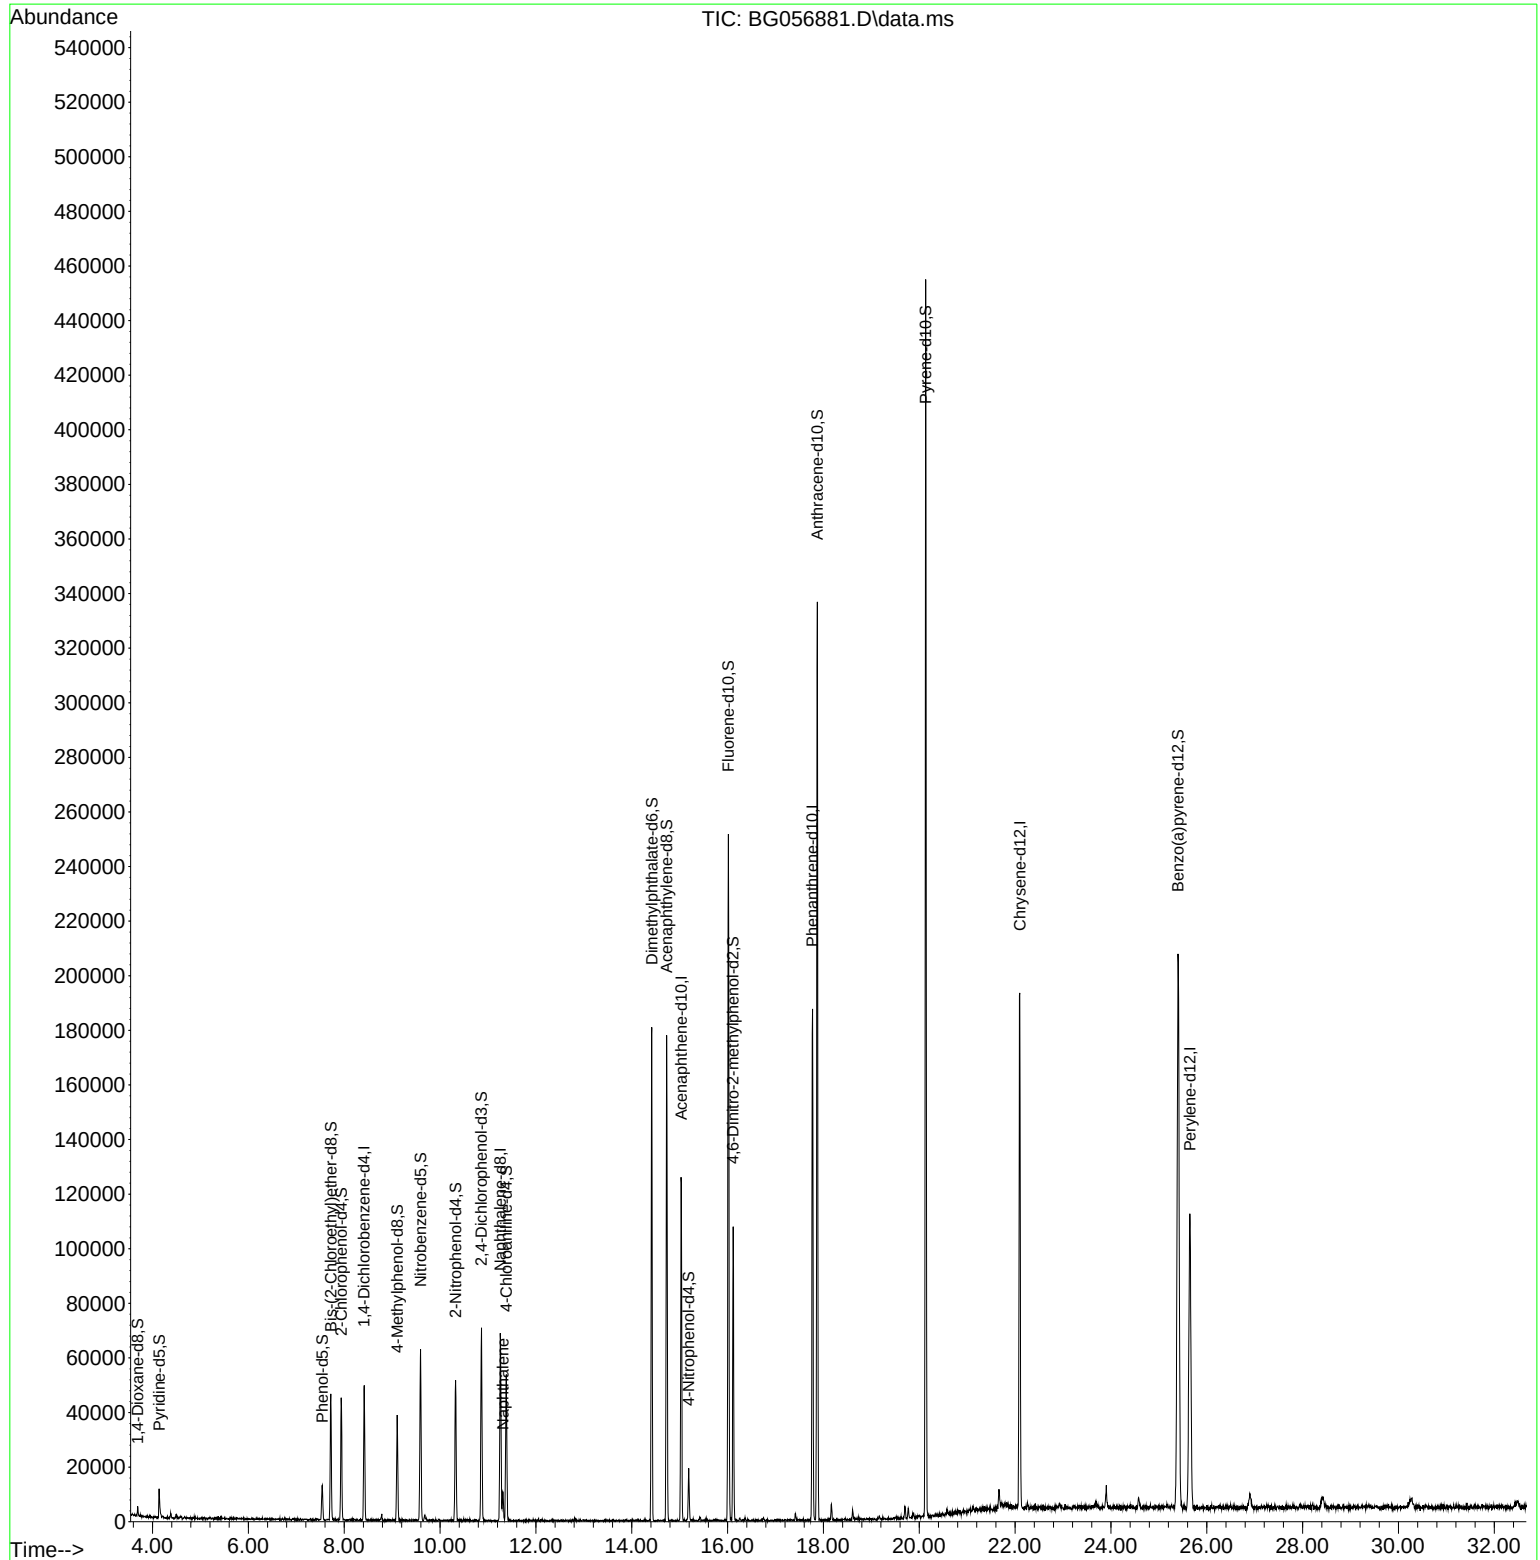

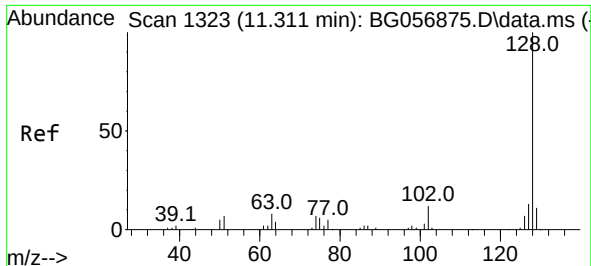

#30

Naphthalene

Concen: 3.196 ng/ul

RT: 11.311 min Scan# 11

Delta R.T. -0.007 min

Lab File: BG056881.D


Acq: 8 Mar 2023 14:18

Instrument :

BNA_G

ClientSampleId :

DCAD6

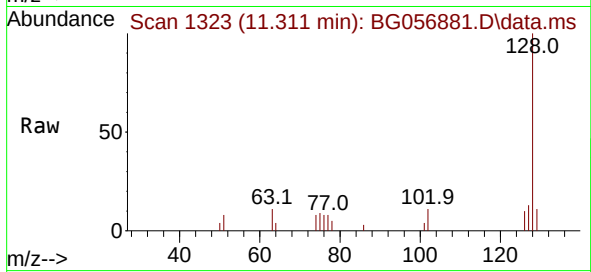

Tgt Ion:128 Resp: 9534

Ion Ratio Lower Upper

128 100

129 10.9 9.4 14.0

127 13.3 11.8 17.6

