

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056876.D
 Acq On : 8 Mar 2023 10:50
 Operator : CG/JU
 Sample : PB151256BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	22	26	34	rVB3	4503	7555	1.34%	0.143%
2	3.957	67	71	72	rBV3	662	842	0.15%	0.016%
3	4.087	91	93	97	rBV3	761	905	0.16%	0.017%
4	4.128	97	100	112	rBV	54993	93716	16.59%	1.779%
5	4.351	134	138	139	rBV2	692	853	0.15%	0.016%
6	4.486	159	161	166	rVV3	872	996	0.18%	0.019%
7	4.563	168	174	176	rBV3	521	970	0.17%	0.018%
8	5.039	252	255	257	rBV2	905	1046	0.19%	0.020%
9	5.291	296	298	301	rBV	847	986	0.17%	0.019%
10	5.644	356	358	362	rVB2	837	833	0.15%	0.016%
11	5.749	373	376	378	rBV2	758	829	0.15%	0.016%
12	5.932	406	407	412	rBV3	644	873	0.15%	0.017%
13	6.325	472	474	477	rVB	880	926	0.16%	0.018%
14	6.760	543	548	549	rBV	524	802	0.14%	0.015%
15	7.542	674	681	688	rBV	64121	113570	20.11%	2.156%
16	7.653	698	700	703	rVB	730	784	0.14%	0.015%
17	7.718	703	711	720	rBV	47416	79889	14.14%	1.517%
18	7.935	742	748	756	rBV	60315	104274	18.46%	1.979%
19	8.417	824	830	839	rVB2	53146	90933	16.10%	1.726%
20	9.104	940	947	955	rBV	75457	129985	23.01%	2.467%
21	9.592	1023	1030	1038	rVB	63380	113510	20.10%	2.155%
22	9.715	1049	1051	1055	rVB	551	772	0.14%	0.015%
23	10.326	1148	1155	1163	rVB	55642	97197	17.21%	1.845%
24	10.867	1240	1247	1254	rBV	75861	134598	23.83%	2.555%
25	11.261	1306	1314	1322	rBB	75701	131935	23.36%	2.505%
26	11.384	1328	1335	1341	rBV	77532	140095	24.80%	2.659%
27	12.806	1574	1577	1582	rBV3	1124	1663	0.29%	0.032%
28	14.416	1845	1851	1858	rBV	182445	257612	45.61%	4.890%
29	14.733	1898	1905	1912	rBV	178538	273493	48.42%	5.192%
30	15.033	1950	1956	1964	rBV	137752	215564	38.17%	4.092%
31	15.191	1977	1983	1994	rBV	97774	153626	27.20%	2.916%
32	16.020	2117	2124	2130	rVB	234765	359351	63.63%	6.822%
33	16.120	2135	2141	2149	rVB2	98327	143017	25.32%	2.715%
34	17.777	2416	2423	2430	rVB	210542	322377	57.08%	6.120%
35	17.871	2433	2439	2449	rVV2	284073	440359	77.97%	8.359%
36	18.587	2557	2561	2564	rBV2	754	1235	0.22%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056876.D
 Acq On : 8 Mar 2023 10:50
 Operator : CG/JU
 Sample : PB151256BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	19.151	2655	2657	2661	rBV2	809	1008	0.18%	0.019%
38	19.281	2677	2679	2683	rVB2	741	875	0.15%	0.017%
39	19.704	2748	2751	2754	rBV3	3615	4892	0.87%	0.093%
40	19.774	2758	2763	2766	rBV3	3753	5726	1.01%	0.109%
41	19.862	2776	2778	2784	rVB	1600	1554	0.28%	0.029%
42	20.009	2801	2803	2806	rBV3	1037	1005	0.18%	0.019%
43	20.139	2818	2825	2832	rBV	401623	564793	100.00%	10.721%
44	20.585	2899	2901	2904	rBV	1388	1480	0.26%	0.028%
45	20.609	2904	2905	2909	rVV2	1097	1426	0.25%	0.027%
46	20.650	2909	2912	2915	rVV2	3672	3814	0.68%	0.072%
47	20.844	2942	2945	2947	rBV3	1307	1411	0.25%	0.027%
48	21.425	3042	3044	3047	rBV3	1957	2309	0.41%	0.044%
49	22.101	3152	3159	3171	rVB2	209154	371282	65.74%	7.048%
50	22.794	3275	3277	3279	rBV3	1915	1272	0.23%	0.024%
51	22.818	3279	3281	3284	rVV4	1897	1188	0.21%	0.023%
52	23.341	3368	3370	3372	rBV2	2393	1671	0.30%	0.032%
53	23.617	3416	3417	3419	rBV	2327	1299	0.23%	0.025%
54	24.874	3629	3631	3632	rBV2	2387	1674	0.30%	0.032%
55	24.945	3642	3643	3644	rVB	2957	1042	0.18%	0.020%
56	25.409	3710	3722	3733	rVB2	179428	520277	92.12%	9.876%
57	25.656	3753	3764	3776	rVB2	117346	351434	62.22%	6.671%
58	25.949	3812	3814	3818	rBV3	2311	3323	0.59%	0.063%
59	27.477	4073	4074	4077	rBV3	2729	1468	0.26%	0.028%
60	29.598	4433	4435	4437	rBV3	1892	1776	0.31%	0.034%
61	32.553	4937	4938	4942	rVB2	2837	1941	0.34%	0.037%




Sum of corrected areas: 5267911

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056876.D
Acq On : 8 Mar 2023 10:50
Operator : CG/JU
Sample : PB151256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

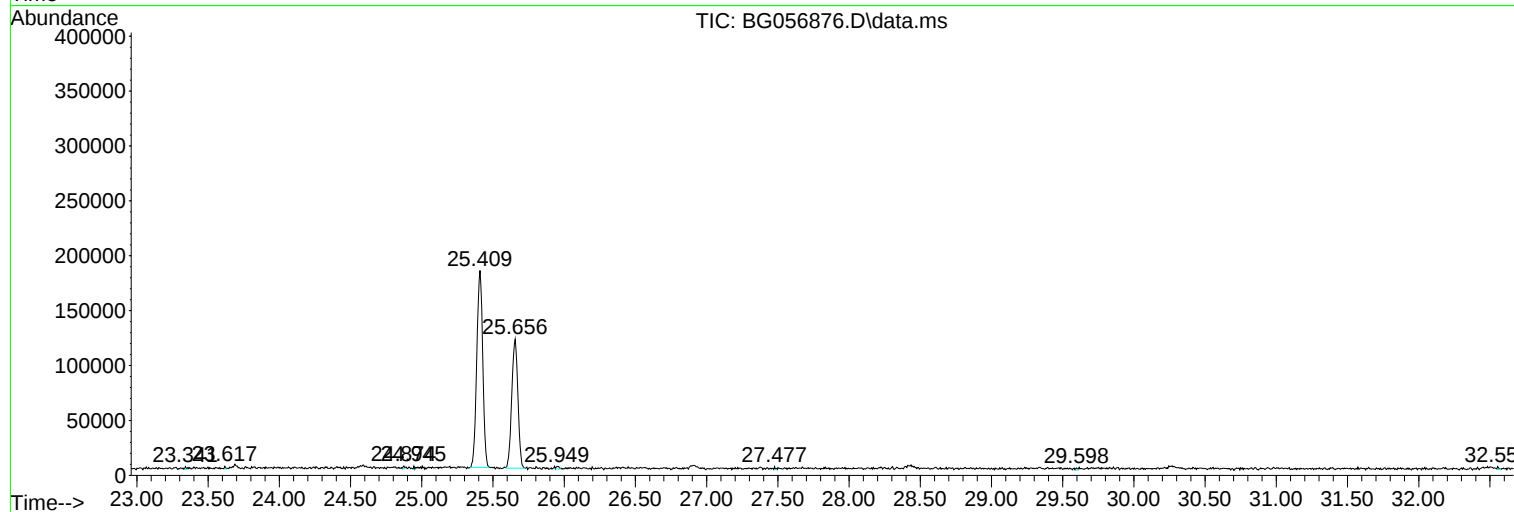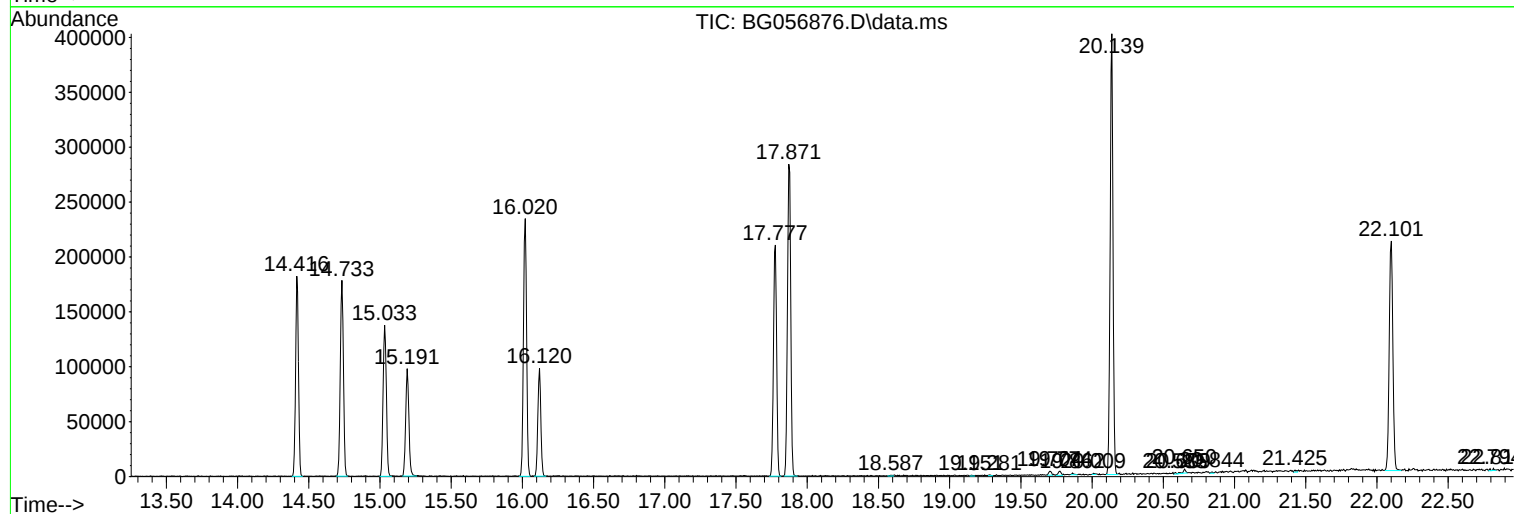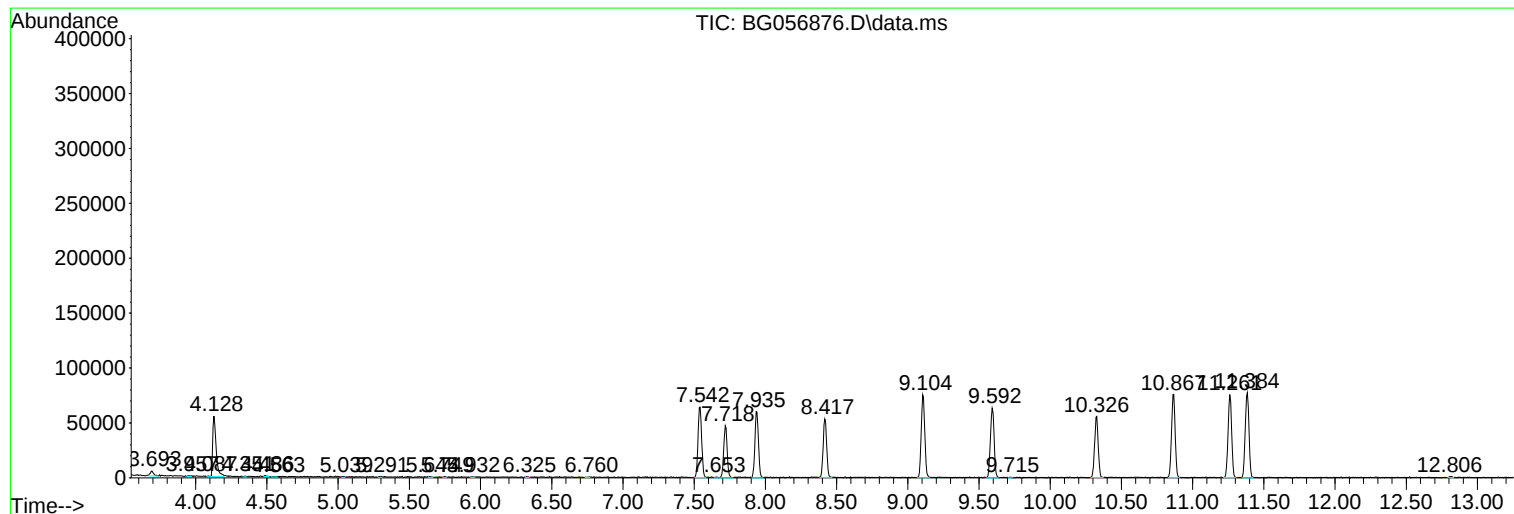

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056876.D
Acq On : 8 Mar 2023 10:50
Operator : CG/JU
Sample : PB151256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056876.D
Acq On : 8 Mar 2023 10:50
Operator : CG/JU
Sample : PB151256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc