

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056877.D
 Acq On : 8 Mar 2023 11:32
 Operator : CG/JU
 Sample : 01746-24
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	22	25	31	rBV3	3565	5974	0.92%	0.117%
2	3.845	49	52	54	rVB	1170	1009	0.16%	0.020%
3	4.133	99	101	114	rVB	15906	25278	3.89%	0.495%
4	4.380	142	143	148	rVB3	1333	1553	0.24%	0.030%
5	4.492	158	162	167	rBV5	1268	1646	0.25%	0.032%
6	5.414	315	319	320	rBV	681	941	0.14%	0.018%
7	5.438	320	323	326	rVB2	851	1214	0.19%	0.024%
8	6.677	530	534	537	rBV	587	952	0.15%	0.019%
9	7.535	674	680	690	rBV2	13415	22423	3.45%	0.439%
10	7.717	705	711	719	rVB	46039	74725	11.51%	1.462%
11	7.941	742	749	757	rBV	44227	75282	11.59%	1.473%
12	8.422	824	831	842	rVB	49576	85977	13.24%	1.682%
13	9.104	941	947	955	rBV	35054	61961	9.54%	1.212%
14	9.592	1023	1030	1038	rBV	62221	110521	17.02%	2.162%
15	10.326	1148	1155	1161	rVB	50479	88182	13.58%	1.725%
16	10.861	1240	1246	1254	rBV	65734	117795	18.14%	2.305%
17	11.119	1286	1290	1295	rVB	1895	2860	0.44%	0.056%
18	11.260	1307	1314	1321	rVB	70462	123602	19.03%	2.418%
19	11.384	1327	1335	1341	rBV	50354	92056	14.18%	1.801%
20	12.811	1575	1578	1583	rVB2	782	1376	0.21%	0.027%
21	13.246	1647	1652	1655	rVB4	1593	2400	0.37%	0.047%
22	13.869	1753	1758	1764	rVB2	10994	15624	2.41%	0.306%
23	14.316	1829	1834	1837	rBV	489	945	0.15%	0.018%
24	14.415	1845	1851	1858	rBV	180044	260878	40.17%	5.104%
25	14.733	1898	1905	1917	rVB	178438	277813	42.78%	5.436%
26	15.032	1949	1956	1963	rBV	128410	202124	31.12%	3.955%
27	15.191	1978	1983	1991	rVB2	17336	30429	4.69%	0.595%
28	15.350	2004	2010	2015	rBV3	1260	2209	0.34%	0.043%
29	15.426	2015	2023	2028	rBV	9802	14876	2.29%	0.291%
30	15.561	2044	2046	2049	rBV2	912	999	0.15%	0.020%
31	16.019	2117	2124	2130	rBV	259356	390360	60.11%	7.638%
32	16.072	2130	2133	2136	rVV2	4691	6412	0.99%	0.125%
33	16.119	2136	2141	2149	rVB	108052	153639	23.66%	3.006%
34	16.254	2161	2164	2167	rBV	1158	1087	0.17%	0.021%
35	17.224	2326	2329	2333	rVB2	974	1041	0.16%	0.020%
36	17.418	2358	2362	2367	rVB2	4638	6560	1.01%	0.128%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056877.D
 Acq On : 8 Mar 2023 11:32
 Operator : CG/JU
 Sample : 01746-24
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	17.776	2416	2423	2429	rBV	200790	301583	46.44%	5.901%
38	17.870	2433	2439	2447	rVB2	334908	508285	78.27%	9.945%
39	18.611	2563	2565	2569	rBV2	2328	2877	0.44%	0.056%
40	18.693	2577	2579	2585	rVV3	810	1425	0.22%	0.028%

41	18.746	2585	2588	2593	rVB2	1073	1361	0.21%	0.027%
42	18.840	2601	2604	2606	rBV2	1121	1152	0.18%	0.023%
43	19.169	2656	2660	2661	rBV2	984	939	0.14%	0.018%
44	19.415	2701	2702	2707	rBV2	640	951	0.15%	0.019%
45	19.457	2707	2709	2716	rVB3	920	1683	0.26%	0.033%

46	19.703	2747	2751	2756	rVB3	4653	6287	0.97%	0.123%
47	19.774	2758	2763	2767	rVV	4185	5477	0.84%	0.107%
48	19.821	2770	2771	2775	rBV2	821	908	0.14%	0.018%
49	19.868	2775	2779	2782	rBV2	1783	2106	0.32%	0.041%
50	19.903	2783	2785	2788	rVB2	1654	1631	0.25%	0.032%

51	19.933	2788	2790	2791	rBV2	1401	1130	0.17%	0.022%
52	20.009	2801	2803	2807	rBV3	1208	1502	0.23%	0.029%
53	20.138	2818	2825	2834	rVB	448769	649396	100.00%	12.706%
54	20.514	2886	2889	2890	rBV2	1226	1289	0.20%	0.025%
55	20.573	2898	2899	2903	rVB2	2633	2344	0.36%	0.046%

56	20.614	2903	2906	2908	rBV3	1733	1397	0.22%	0.027%
57	20.732	2924	2926	2929	rVB3	1788	1450	0.22%	0.028%
58	20.761	2929	2931	2933	rBV2	1131	1388	0.21%	0.027%
59	22.095	3152	3158	3171	rVB2	203039	356187	54.85%	6.969%
60	22.341	3198	3200	3203	rVV4	1899	1895	0.29%	0.037%

61	22.371	3203	3205	3206	rVB2	1830	922	0.14%	0.018%
62	23.205	3345	3347	3348	rBV	1571	1093	0.17%	0.021%
63	24.351	3540	3542	3546	rBV3	2393	2119	0.33%	0.041%
64	24.586	3576	3582	3585	rBV6	2911	6197	0.95%	0.121%
65	24.933	3639	3641	3642	rBV	1904	908	0.14%	0.018%

66	24.950	3642	3644	3647	rVV3	1869	1378	0.21%	0.027%
67	25.326	3706	3708	3710	rBV2	1858	1320	0.20%	0.026%
68	25.408	3710	3722	3734	rVB2	210827	621717	95.74%	12.165%
69	25.649	3752	3763	3774	rVB2	111437	342046	52.67%	6.693%
70	27.200	4025	4027	4030	rBV3	1658	2145	0.33%	0.042%

71	27.306	4043	4045	4046	rBV2	1773	1222	0.19%	0.024%
72	28.393	4228	4230	4231	rBV	3037	2275	0.35%	0.045%
73	28.581	4260	4262	4263	rBV2	1839	951	0.15%	0.019%
74	28.622	4267	4269	4272	rBV3	1939	2816	0.43%	0.055%
75	29.574	4429	4431	4433	rBV2	2335	2166	0.33%	0.042%

76	29.627	4438	4440	4441	rBV	1903	995	0.15%	0.019%
----	--------	------	------	------	-----	------	-----	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056877.D
Acq On : 8 Mar 2023 11:32
Operator : CG/JU
Sample : 01746-24
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAC9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Title : SVOA CALIBRATION

77	29.844	4475	4477	4478	rBV2	1959	1601	0.25%	0.031%
78	31.807	4809	4811	4812	rBV	3162	1643	0.25%	0.032%




Sum of corrected areas: 5110880

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056877.D
Acq On : 8 Mar 2023 11:32
Operator : CG/JU
Sample : 01746-24
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

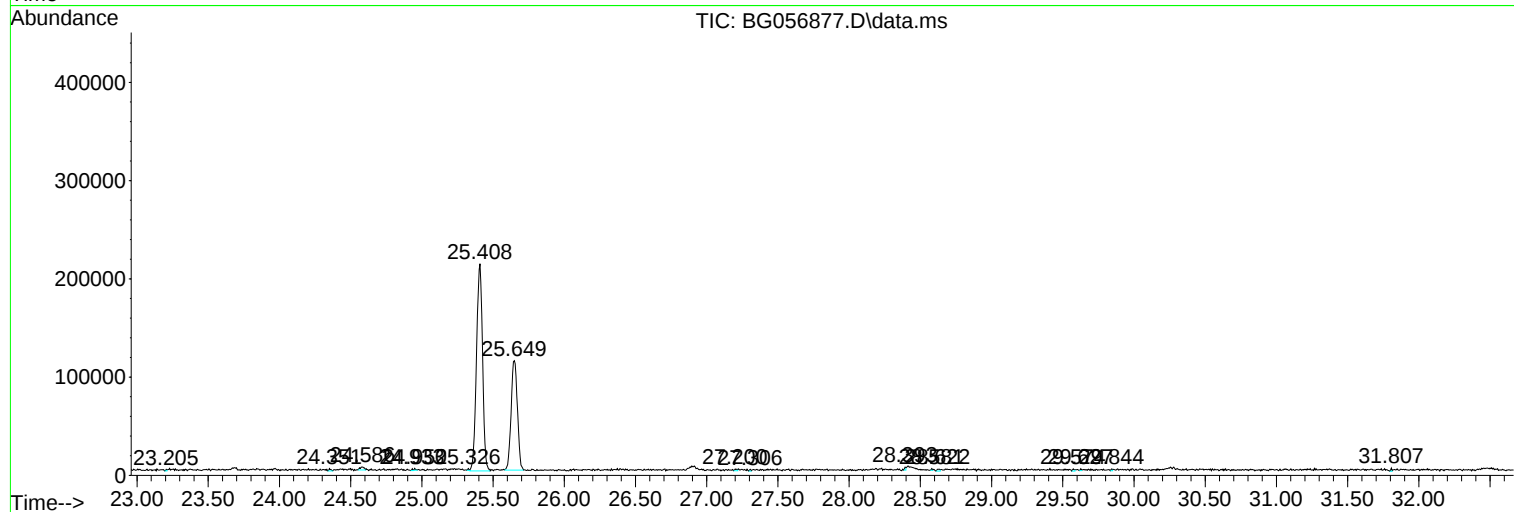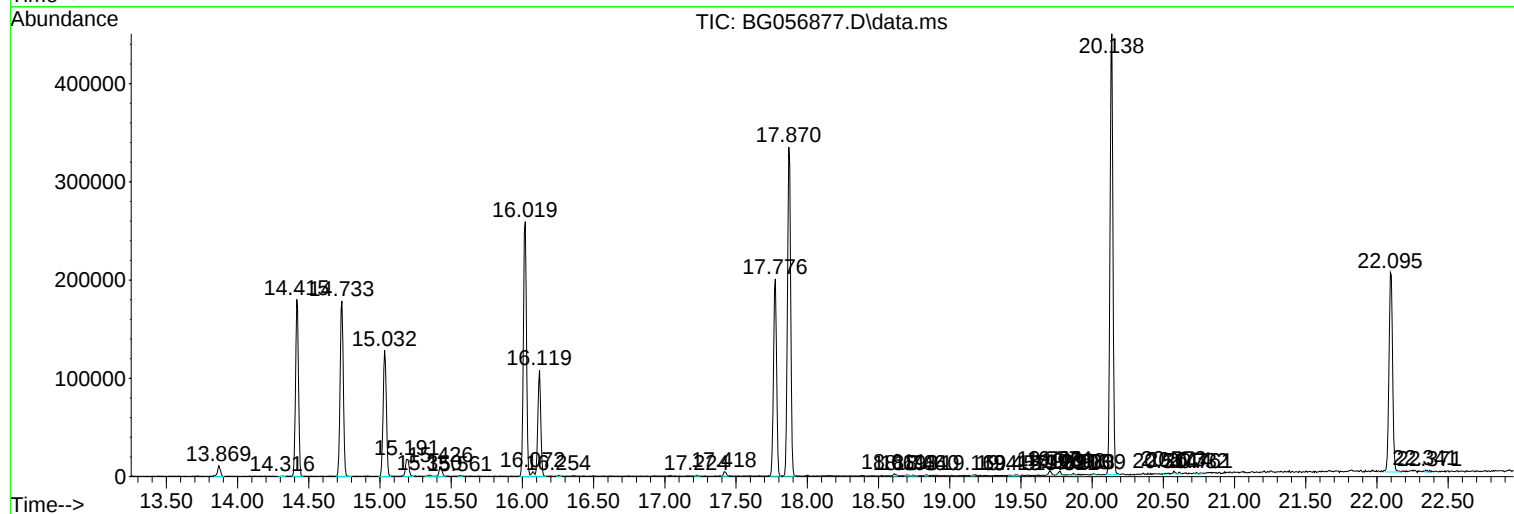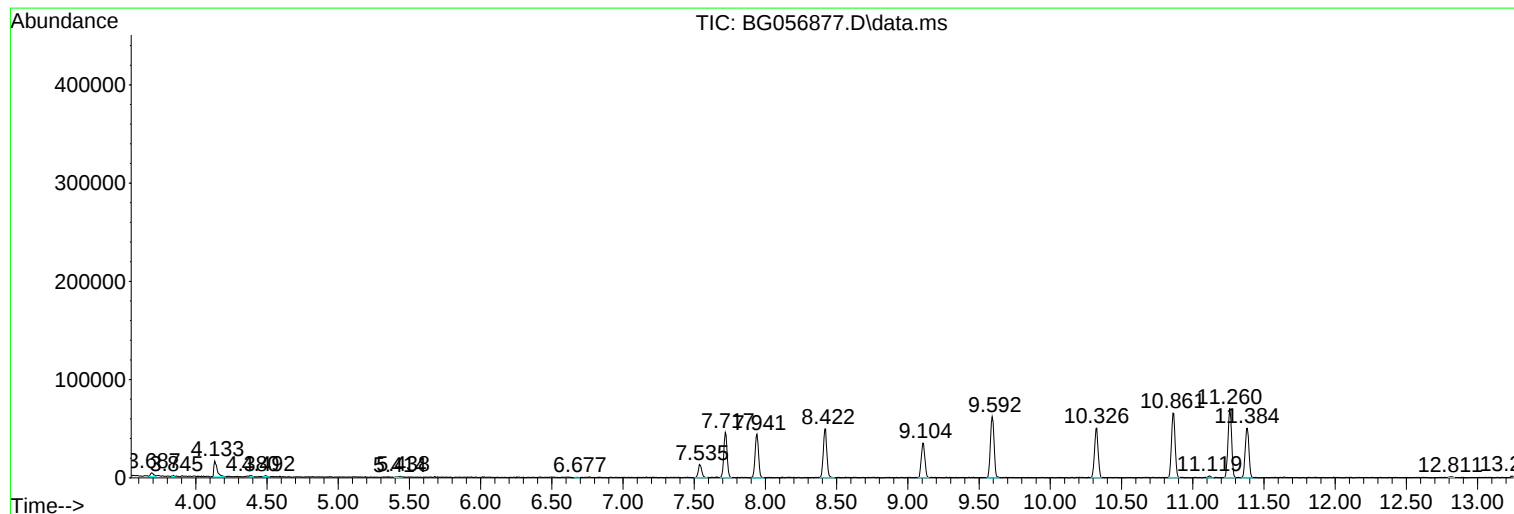

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056877.D
Acq On : 8 Mar 2023 11:32
Operator : CG/JU
Sample : 01746-24
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056877.D
Acq On : 8 Mar 2023 11:32
Operator : CG/JU
Sample : 01746-24
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc