

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056879.D
 Acq On : 8 Mar 2023 12:55
 Operator : CG/JU
 Sample : 01784-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056879.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.690	22	26	31	rVB3	3140	4776	0.73%	0.093%
2	4.136	99	102	110	rVB2	8084	12397	1.91%	0.241%
3	4.377	139	143	146	rBV2	1257	1454	0.22%	0.028%
4	4.595	178	180	184	rVB3	1176	1249	0.19%	0.024%
5	5.435	320	323	328	rVB3	1203	1895	0.29%	0.037%
6	5.981	413	416	418	rBV2	788	1038	0.16%	0.020%
7	6.974	578	585	588	rBB	702	1363	0.21%	0.027%
8	7.538	676	681	688	rBV	15809	25231	3.88%	0.491%
9	7.720	705	712	718	rBV	50236	82315	12.67%	1.602%
10	7.938	743	749	755	rVB2	50118	83385	12.83%	1.622%
11	8.414	824	830	837	rBV	46436	78467	12.07%	1.527%
12	9.060	937	940	942	rBV	616	907	0.14%	0.018%
13	9.107	942	948	956	rVB	41362	72933	11.22%	1.419%
14	9.595	1024	1031	1039	rVB	64905	115604	17.79%	2.249%
15	9.718	1048	1052	1055	rBB2	669	910	0.14%	0.018%
16	9.971	1092	1095	1098	rVB	1442	1857	0.29%	0.036%
17	10.323	1148	1155	1163	rVB	58377	98919	15.22%	1.925%
18	10.864	1240	1247	1255	rVB	77199	133208	20.50%	2.592%
19	11.258	1305	1314	1322	rBV	64642	117544	18.09%	2.287%
20	11.381	1328	1335	1342	rBV	57772	102225	15.73%	1.989%
21	12.456	1513	1518	1522	rVB2	3388	4341	0.67%	0.084%
22	12.815	1574	1579	1584	rBV	1568	2029	0.31%	0.039%
23	14.419	1845	1852	1858	rVB	197640	282017	43.40%	5.487%
24	14.730	1898	1905	1913	rVB2	194637	301471	46.39%	5.866%
25	15.035	1950	1957	1964	rVB	124626	190818	29.36%	3.713%
26	15.188	1978	1983	1990	rBV3	22225	34679	5.34%	0.675%
27	15.265	1990	1996	2000	rVB2	599	1006	0.15%	0.020%
28	15.787	2082	2085	2090	rBV2	2785	3938	0.61%	0.077%
29	15.940	2108	2111	2114	rBV	713	1111	0.17%	0.022%
30	16.017	2118	2124	2131	rBV	270265	411211	63.28%	8.001%
31	16.117	2134	2141	2147	rBV	111142	159149	24.49%	3.097%
32	16.369	2181	2184	2187	rVB3	1151	1362	0.21%	0.027%
33	16.598	2218	2223	2228	rBV3	7934	8562	1.32%	0.167%
34	16.745	2243	2248	2252	rBV3	3074	3908	0.60%	0.076%
35	17.350	2345	2351	2355	rBV2	5625	8212	1.26%	0.160%
36	17.391	2355	2358	2362	rVB2	3105	3690	0.57%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056879.D
 Acq On : 8 Mar 2023 12:55
 Operator : CG/JU
 Sample : 01784-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	17.773	2417	2423	2431	rVB	194172	287889	44.30%	5.601%
38	17.873	2433	2440	2448	rBV2	348253	524622	80.73%	10.208%
39	18.608	2561	2565	2570	rBV3	5838	8203	1.26%	0.160%
40	18.702	2576	2581	2584	rBV3	2122	2825	0.43%	0.055%
41	18.890	2611	2613	2616	rBV3	1155	1373	0.21%	0.027%
42	19.701	2747	2751	2756	rVB5	5209	7151	1.10%	0.139%
43	19.777	2756	2764	2767	rBV4	4267	7132	1.10%	0.139%
44	19.812	2767	2770	2774	rVB3	790	921	0.14%	0.018%
45	19.865	2777	2779	2783	rVB2	1550	1675	0.26%	0.033%
46	20.006	2801	2803	2808	rVB2	1456	1753	0.27%	0.034%
47	20.088	2815	2817	2819	rVB	1957	1466	0.23%	0.029%
48	20.135	2819	2825	2833	rBV	473004	649851	100.00%	12.644%
49	20.329	2856	2858	2859	rBV2	935	913	0.14%	0.018%
50	20.376	2865	2866	2870	rBV3	768	984	0.15%	0.019%
51	20.517	2888	2890	2891	rBV	1273	1036	0.16%	0.020%
52	20.658	2912	2914	2917	rVB3	1460	1466	0.23%	0.029%
53	21.028	2975	2977	2979	rVB2	1771	1230	0.19%	0.024%
54	21.111	2988	2991	2992	rBV2	2296	1978	0.30%	0.038%
55	21.305	3021	3024	3025	rBV2	1943	1611	0.25%	0.031%
56	21.381	3035	3037	3039	rBV3	1516	1187	0.18%	0.023%
57	21.663	3082	3085	3091	rBV6	5084	8193	1.26%	0.159%
58	21.775	3102	3104	3105	rBV2	1909	1322	0.20%	0.026%
59	21.822	3110	3112	3113	rBV2	2253	1143	0.18%	0.022%
60	21.933	3129	3131	3135	rVB	6206	7575	1.17%	0.147%
61	22.098	3152	3159	3166	rVB2	186131	316208	48.66%	6.152%
62	22.991	3309	3311	3313	rVB3	1564	1122	0.17%	0.022%
63	23.014	3313	3315	3318	rBV3	1970	2048	0.32%	0.040%
64	23.584	3410	3412	3420	rVB6	4481	5276	0.81%	0.103%
65	23.896	3463	3465	3473	rVB7	4009	7043	1.08%	0.137%
66	24.577	3577	3581	3586	rVB7	2266	3917	0.60%	0.076%
67	25.406	3711	3722	3733	rVB2	205718	602699	92.74%	11.727%
68	25.647	3753	3763	3777	rVB2	102467	311375	47.91%	6.058%
69	26.880	3971	3973	3974	rBV2	2889	1749	0.27%	0.034%
70	29.313	4385	4387	4388	rBV	1834	1388	0.21%	0.027%
71	29.589	4431	4434	4436	rBV3	1736	2213	0.34%	0.043%
72	29.936	4491	4493	4496	rBV3	2115	2407	0.37%	0.047%
73	31.193	4705	4707	4708	rBV2	1722	904	0.14%	0.018%
74	31.963	4836	4838	4839	rBV2	1930	1383	0.21%	0.027%
75	32.356	4903	4905	4907	rBV2	1957	1133	0.17%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056879.D
Acq On : 8 Mar 2023 12:55
Operator : CG/JU
Sample : 01784-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAD1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 5139545

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056879.D
Acq On : 8 Mar 2023 12:55
Operator : CG/JU
Sample : 01784-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

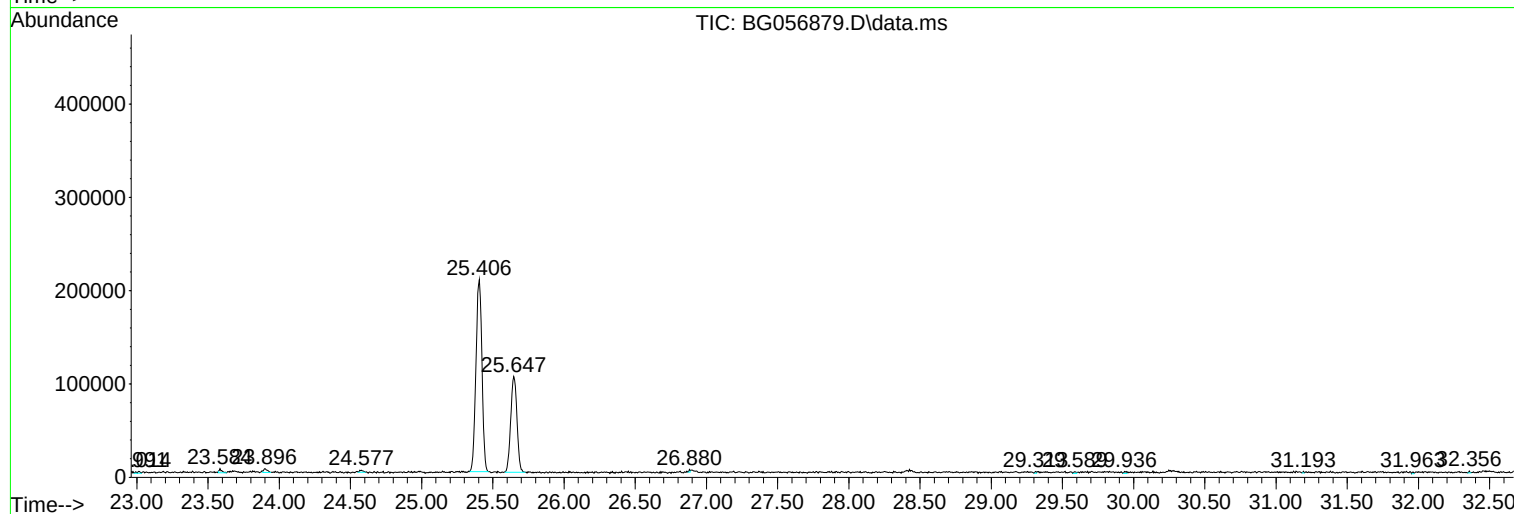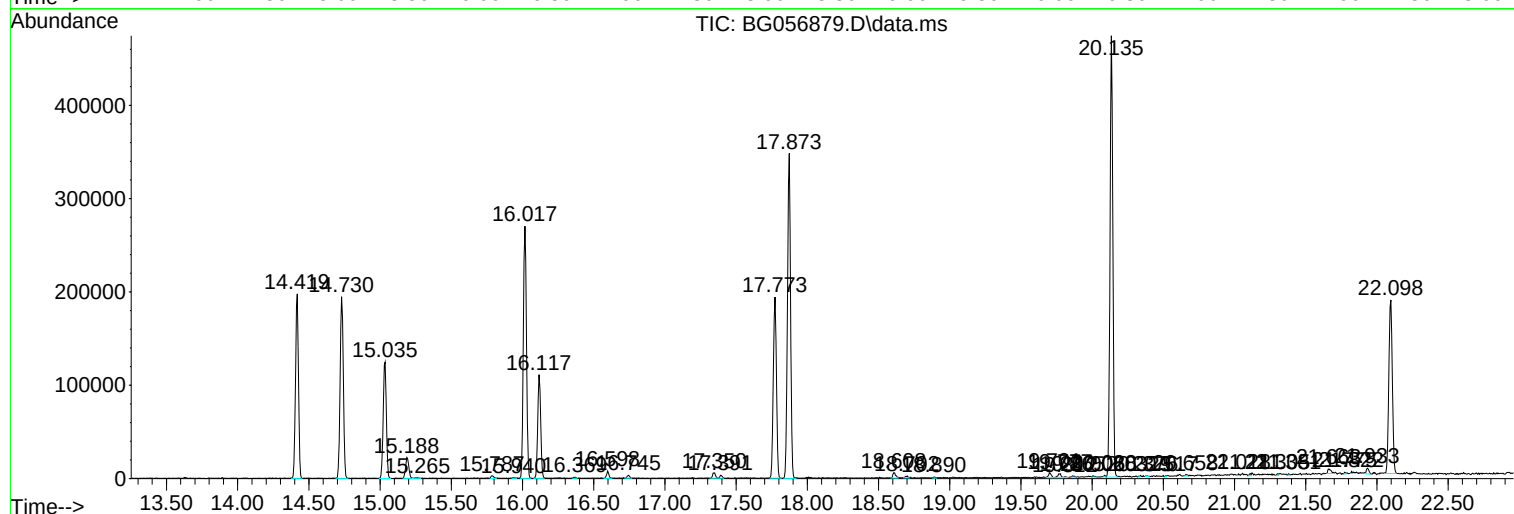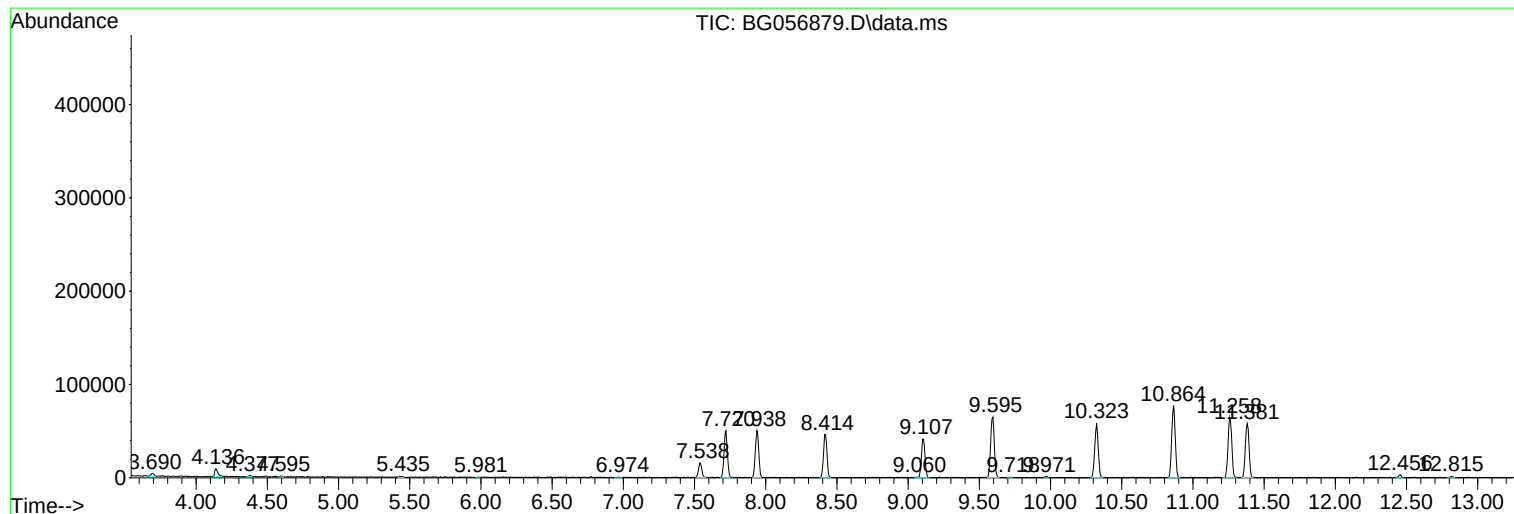

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056879.D
Acq On : 8 Mar 2023 12:55
Operator : CG/JU
Sample : 01784-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056879.D
Acq On : 8 Mar 2023 12:55
Operator : CG/JU
Sample : 01784-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc