

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056880.D
 Acq On : 8 Mar 2023 13:36
 Operator : CG/JU
 Sample : 01784-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.691	22	26	31	rVB3	3631	4755	0.71%	0.092%
2	3.785	39	42	44	rBV2	1321	1265	0.19%	0.025%
3	3.979	72	75	76	rBV	973	899	0.13%	0.017%
4	4.137	100	102	108	rBV	8057	12766	1.91%	0.247%
5	4.378	141	143	147	rVB3	1669	2007	0.30%	0.039%
6	4.484	159	161	165	rBV2	991	935	0.14%	0.018%
7	4.590	176	179	182	rBV3	1336	1888	0.28%	0.037%
8	5.019	249	252	253	rBV	983	895	0.13%	0.017%
9	5.436	319	323	324	rBV2	1563	1211	0.18%	0.023%
10	7.498	669	674	675	rBV2	797	1228	0.18%	0.024%
11	7.539	675	681	689	rVB	14798	26595	3.98%	0.515%
12	7.721	704	712	718	rVB	46967	80123	11.98%	1.553%
13	7.939	743	749	757	rBV	46816	80331	12.01%	1.557%
14	8.421	823	831	837	rBV	46957	79391	11.87%	1.539%
15	8.961	921	923	926	rBV	1498	1428	0.21%	0.028%
16	9.102	942	947	955	rVB	43056	71975	10.76%	1.395%
17	9.414	998	1000	1005	rBV2	635	1064	0.16%	0.021%
18	9.590	1023	1030	1037	rBV	66749	116682	17.45%	2.261%
19	10.001	1097	1100	1102	rBV	873	915	0.14%	0.018%
20	10.324	1148	1155	1162	rBV	55838	98686	14.76%	1.913%
21	10.865	1239	1247	1257	rBV	76669	133825	20.01%	2.594%
22	11.258	1305	1314	1321	rBV	65573	116049	17.36%	2.249%
23	11.382	1329	1335	1342	rBV	57353	102224	15.29%	1.981%
24	11.435	1342	1344	1350	rVB	948	1324	0.20%	0.026%
25	11.958	1428	1433	1437	rVB2	784	1278	0.19%	0.025%
26	12.216	1474	1477	1481	rBV	852	1132	0.17%	0.022%
27	12.815	1575	1579	1583	rBV4	1045	1956	0.29%	0.038%
28	13.620	1712	1716	1720	rBV	515	1039	0.16%	0.020%
29	13.867	1752	1758	1761	rBV2	1198	2333	0.35%	0.045%
30	14.414	1845	1851	1858	rBV	198661	286759	42.89%	5.558%
31	14.731	1898	1905	1911	rBV	194635	301395	45.07%	5.841%
32	15.031	1950	1956	1963	rBV	123610	193851	28.99%	3.757%
33	15.101	1963	1968	1972	rVV2	2627	3981	0.60%	0.077%
34	15.189	1976	1983	1991	rVB2	23176	35881	5.37%	0.695%
35	15.424	2019	2023	2028	rBV	3124	3866	0.58%	0.075%
36	16.018	2117	2124	2131	rBV	277718	415255	62.10%	8.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056880.D
 Acq On : 8 Mar 2023 13:36
 Operator : CG/JU
 Sample : 01784-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	16.118	2136	2141	2149	rVB	111905	161881	24.21%	3.137%
38	16.253	2162	2164	2167	rBV2	1038	1157	0.17%	0.022%
39	16.740	2243	2247	2252	rBV4	1137	1879	0.28%	0.036%
40	17.069	2298	2303	2306	rBV3	800	1449	0.22%	0.028%
41	17.774	2415	2423	2430	rBV	183622	282038	42.18%	5.466%
42	17.874	2432	2440	2447	rBV2	340467	533934	79.85%	10.348%
43	18.168	2486	2490	2495	rVB2	2027	2775	0.42%	0.054%
44	18.403	2528	2530	2532	rVB	901	927	0.14%	0.018%
45	18.609	2560	2565	2570	rBV4	4506	6962	1.04%	0.135%
46	18.897	2612	2614	2617	rBV2	1282	1120	0.17%	0.022%
47	19.026	2633	2636	2639	rBV2	685	1122	0.17%	0.022%
48	19.384	2695	2697	2700	rVB2	1265	911	0.14%	0.018%
49	19.414	2700	2702	2705	rBV2	1022	1357	0.20%	0.026%
50	19.637	2735	2740	2741	rBV2	930	1188	0.18%	0.023%
51	19.707	2744	2752	2755	rBV5	5301	8130	1.22%	0.158%
52	19.772	2759	2763	2768	rVB2	4155	6016	0.90%	0.117%
53	19.860	2776	2778	2783	rVB2	2192	2871	0.43%	0.056%
54	20.007	2800	2803	2805	rBV3	1147	1278	0.19%	0.025%
55	20.042	2808	2809	2812	rBV2	1147	922	0.14%	0.018%
56	20.095	2815	2818	2819	rBV2	880	1049	0.16%	0.020%
57	20.136	2819	2825	2832	rVB	467791	668663	100.00%	12.959%
58	20.818	2939	2941	2946	rVB3	2377	2824	0.42%	0.055%
59	20.935	2959	2961	2962	rBV2	1328	1246	0.19%	0.024%
60	20.965	2965	2966	2969	rVV2	1355	985	0.15%	0.019%
61	21.864	3118	3119	3120	rBV	2333	978	0.15%	0.019%
62	22.034	3146	3148	3151	rBV4	1873	2674	0.40%	0.052%
63	22.099	3152	3159	3169	rVB2	188161	324549	48.54%	6.290%
64	22.798	3276	3278	3279	rBV2	2266	1283	0.19%	0.025%
65	25.013	3654	3655	3657	rVB2	2467	1023	0.15%	0.020%
66	25.401	3711	3721	3734	rVB2	208874	620717	92.83%	12.030%
67	25.648	3752	3763	3777	rVB2	103526	317439	47.47%	6.152%
68	25.877	3800	3802	3805	rVB3	2493	1949	0.29%	0.038%
69	25.965	3815	3817	3819	rBV3	1771	1867	0.28%	0.036%
70	27.792	4126	4128	4129	rBV2	1713	1253	0.19%	0.024%
71	28.791	4297	4298	4301	rBV3	1963	1979	0.30%	0.038%
72	28.920	4318	4320	4322	rBV2	1848	1428	0.21%	0.028%
73	31.664	4785	4787	4790	rBV3	1667	1518	0.23%	0.029%
74	32.610	4946	4948	4950	rBV3	1895	1209	0.18%	0.023%

Sum of corrected areas: 5159737




Instrument :
BNA_G
ClientSampleId :
DCAD2

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056880.D
Acq On : 8 Mar 2023 13:36
Operator : CG/JU
Sample : 01784-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

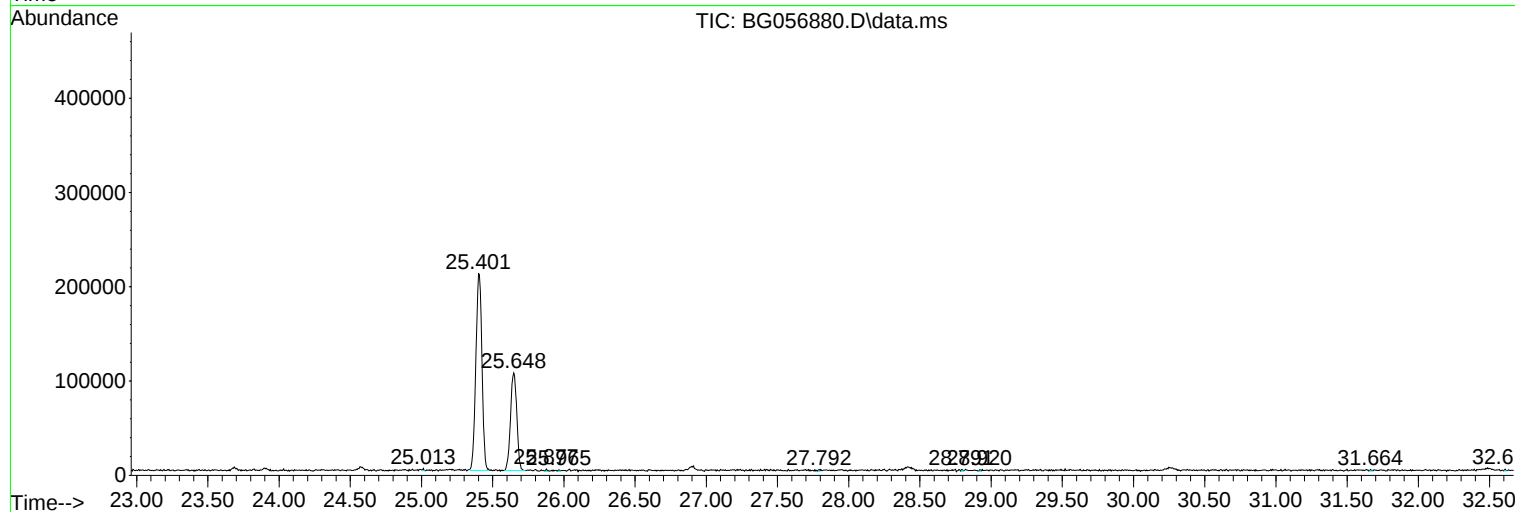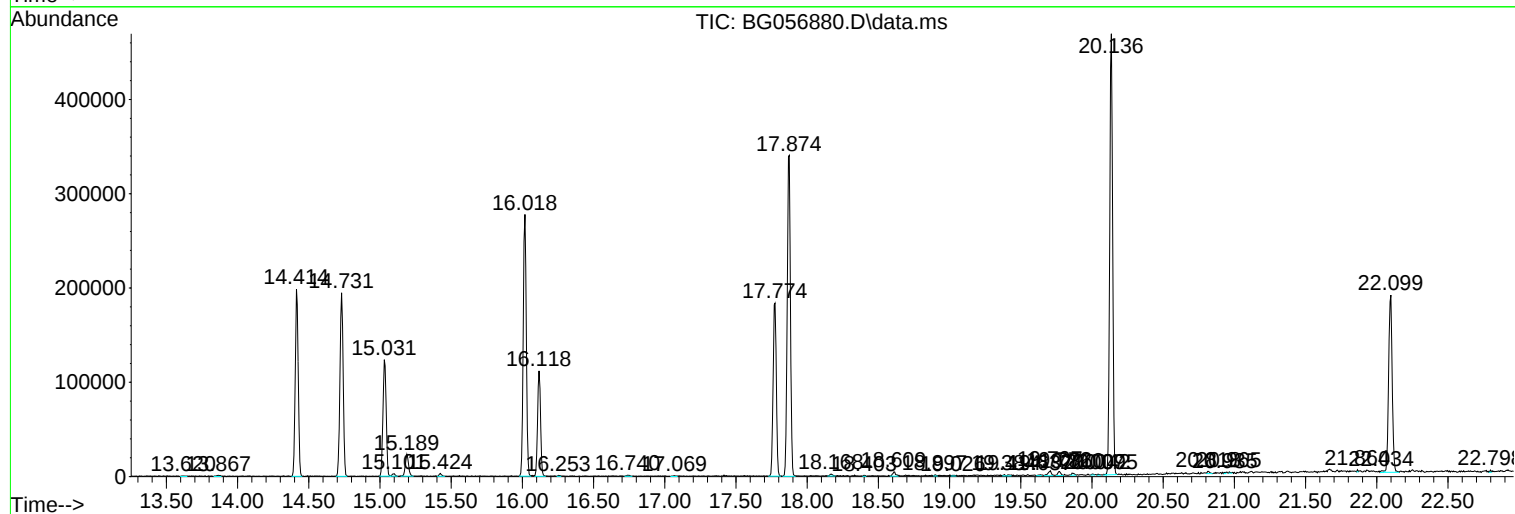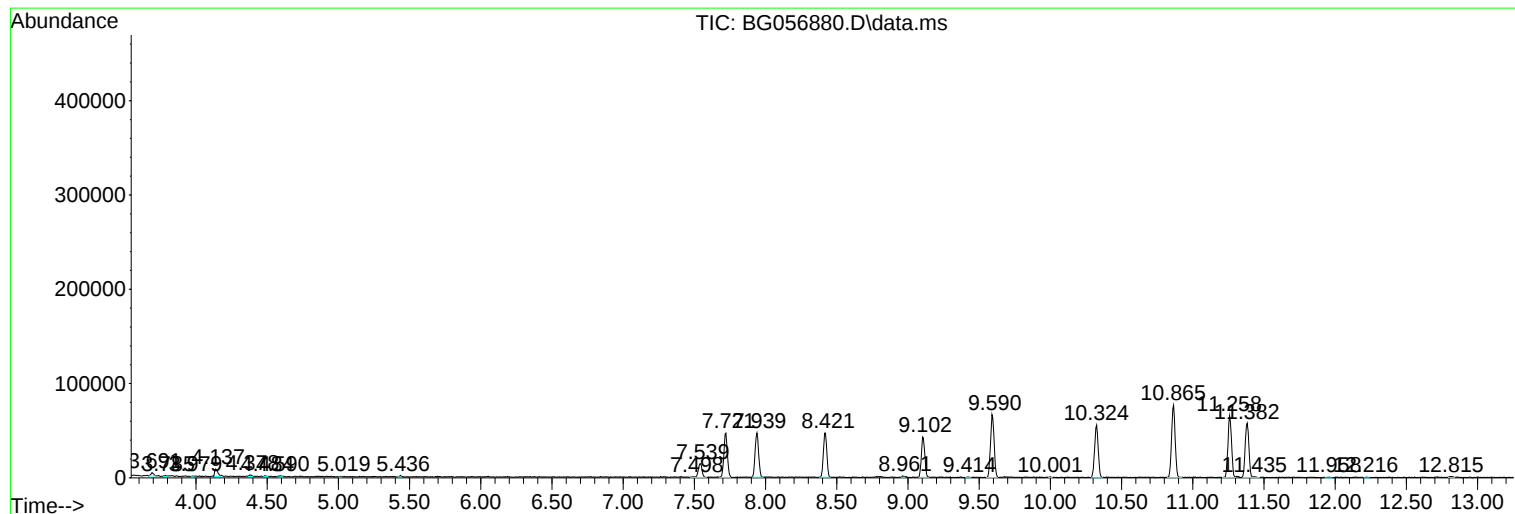

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056880.D
Acq On : 8 Mar 2023 13:36
Operator : CG/JU
Sample : 01784-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056880.D
Acq On : 8 Mar 2023 13:36
Operator : CG/JU
Sample : 01784-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc