

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056884.D
 Acq On : 8 Mar 2023 16:24
 Operator : CG/JU
 Sample : 01784-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.691	23	26	30	rVB3	2628	3457	0.55%	0.069%
2	4.131	99	101	113	rVB	15243	24904	4.00%	0.499%
3	4.378	140	143	149	rVB3	1506	2432	0.39%	0.049%
4	4.454	153	156	158	rBV	1009	1124	0.18%	0.023%
5	4.484	158	161	168	rBV4	1517	2803	0.45%	0.056%
6	4.584	177	178	182	rBV	649	812	0.13%	0.016%
7	5.183	278	280	283	rBV3	784	920	0.15%	0.018%
8	5.436	317	323	329	rVB4	1070	2252	0.36%	0.045%
9	5.665	359	362	367	rVB3	976	1510	0.24%	0.030%
10	7.539	676	681	687	rVB	12570	20539	3.30%	0.412%
11	7.721	705	712	720	rBV	43004	72137	11.58%	1.447%
12	7.939	743	749	756	rBV	41527	72612	11.66%	1.456%
13	8.414	824	830	838	rVB	50657	83950	13.48%	1.683%
14	9.102	942	947	959	rVB2	32175	56326	9.04%	1.130%
15	9.419	999	1001	1004	rBV	675	890	0.14%	0.018%
16	9.595	1022	1031	1037	rBV	59517	104856	16.83%	2.103%
17	9.819	1066	1069	1072	rBV	683	1034	0.17%	0.021%
18	10.007	1098	1101	1104	rVB	688	878	0.14%	0.018%
19	10.324	1147	1155	1163	rVB2	47838	86368	13.87%	1.732%
20	10.865	1239	1247	1254	rBV	65043	115600	18.56%	2.318%
21	11.258	1308	1314	1322	rVB2	69156	123946	19.90%	2.486%
22	11.382	1328	1335	1344	rBV2	57599	103413	16.60%	2.074%
23	11.946	1427	1431	1434	rBV	581	964	0.15%	0.019%
24	12.063	1447	1451	1456	rVB3	973	1671	0.27%	0.034%
25	12.204	1474	1475	1482	rVB	471	825	0.13%	0.017%
26	12.662	1551	1553	1558	rVB2	711	1031	0.17%	0.021%
27	12.815	1575	1579	1582	rBV2	1069	1672	0.27%	0.034%
28	14.419	1845	1852	1858	rBV	175117	258070	41.43%	5.175%
29	14.543	1870	1873	1877	rVB2	822	1067	0.17%	0.021%
30	14.731	1898	1905	1915	rVB	180370	272924	43.81%	5.473%
31	15.030	1950	1956	1963	rVB	134996	205919	33.06%	4.129%
32	15.189	1978	1983	1988	rBV3	15382	23576	3.78%	0.473%
33	16.017	2118	2124	2132	rVB	253920	379104	60.86%	7.602%
34	16.117	2136	2141	2148	rVB	103478	146490	23.52%	2.938%
35	16.252	2161	2164	2168	rBV2	985	1106	0.18%	0.022%
36	16.364	2178	2183	2188	rVB3	2717	4447	0.71%	0.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056884.D
 Acq On : 8 Mar 2023 16:24
 Operator : CG/JU
 Sample : 01784-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	17.774	2416	2423	2429	rBV	199048	307865	49.42%	6.174%
38	17.868	2433	2439	2446	rBV2	327000	494428	79.37%	9.915%
39	18.168	2487	2490	2493	rBV2	979	1394	0.22%	0.028%
40	18.614	2561	2566	2568	rBV3	3232	4254	0.68%	0.085%

41	18.691	2577	2579	2586	rVB2	987	1592	0.26%	0.032%
42	19.701	2747	2751	2755	rVV3	3826	5312	0.85%	0.107%
43	19.766	2759	2762	2767	rVB2	3803	5269	0.85%	0.106%
44	19.819	2767	2771	2774	rBV2	811	1076	0.17%	0.022%
45	20.013	2800	2804	2806	rBV2	821	1244	0.20%	0.025%

46	20.083	2812	2816	2818	rBV3	1201	1278	0.21%	0.026%
47	20.136	2818	2825	2833	rVV	425244	622913	100.00%	12.492%
48	20.389	2866	2868	2871	rVB3	1197	1114	0.18%	0.022%
49	20.418	2871	2873	2877	rBV2	922	1267	0.20%	0.025%
50	20.494	2884	2886	2888	rBV3	1133	1050	0.17%	0.021%

51	20.518	2888	2890	2893	rVV2	978	1126	0.18%	0.023%
52	20.841	2943	2945	2949	rBV4	1224	1817	0.29%	0.036%
53	20.888	2951	2953	2957	rBV3	1569	1822	0.29%	0.037%
54	21.006	2971	2973	2977	rBV5	1614	2039	0.33%	0.041%
55	21.058	2977	2982	2986	rVV5	2499	4378	0.70%	0.088%

56	21.664	3080	3085	3088	rBV5	10389	17344	2.78%	0.348%
57	21.934	3127	3131	3132	rBV4	1713	1748	0.28%	0.035%
58	22.098	3152	3159	3169	rVB	201009	349112	56.05%	7.001%
59	22.921	3297	3299	3302	rVB3	2902	2308	0.37%	0.046%
60	23.667	3424	3426	3428	rBV3	2230	2763	0.44%	0.055%

61	23.802	3447	3449	3452	rVB4	1761	1068	0.17%	0.021%
62	23.902	3460	3466	3471	rVB2	8689	16569	2.66%	0.332%
63	24.219	3518	3520	3522	rBV3	1977	1252	0.20%	0.025%
64	24.519	3569	3571	3573	rBV2	1708	874	0.14%	0.018%
65	24.684	3597	3599	3600	rBV2	1519	811	0.13%	0.016%

66	25.124	3672	3674	3677	rBV3	1433	1835	0.29%	0.037%
67	25.400	3710	3721	3735	rVB2	202859	588163	94.42%	11.795%
68	25.647	3752	3763	3776	rVB	117880	346987	55.70%	6.958%
69	26.217	3858	3860	3862	rBV3	1839	1353	0.22%	0.027%
70	26.587	3921	3923	3926	rBV2	1704	1484	0.24%	0.030%

71	27.269	4037	4039	4040	rBV2	1636	1364	0.22%	0.027%
72	28.385	4227	4229	4230	rBV2	2230	1184	0.19%	0.024%
73	29.607	4435	4437	4439	rBV3	1719	1296	0.21%	0.026%
74	30.207	4537	4539	4541	rBV3	1790	2040	0.33%	0.041%
75	30.818	4641	4643	4648	rBV3	1646	2301	0.37%	0.046%

76	31.158	4699	4701	4702	rBV2	2200	1919	0.31%	0.038%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056884.D
Acq On : 8 Mar 2023 16:24
Operator : CG/JU
Sample : 01784-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAF2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 4986642

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056884.D
Acq On : 8 Mar 2023 16:24
Operator : CG/JU
Sample : 01784-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

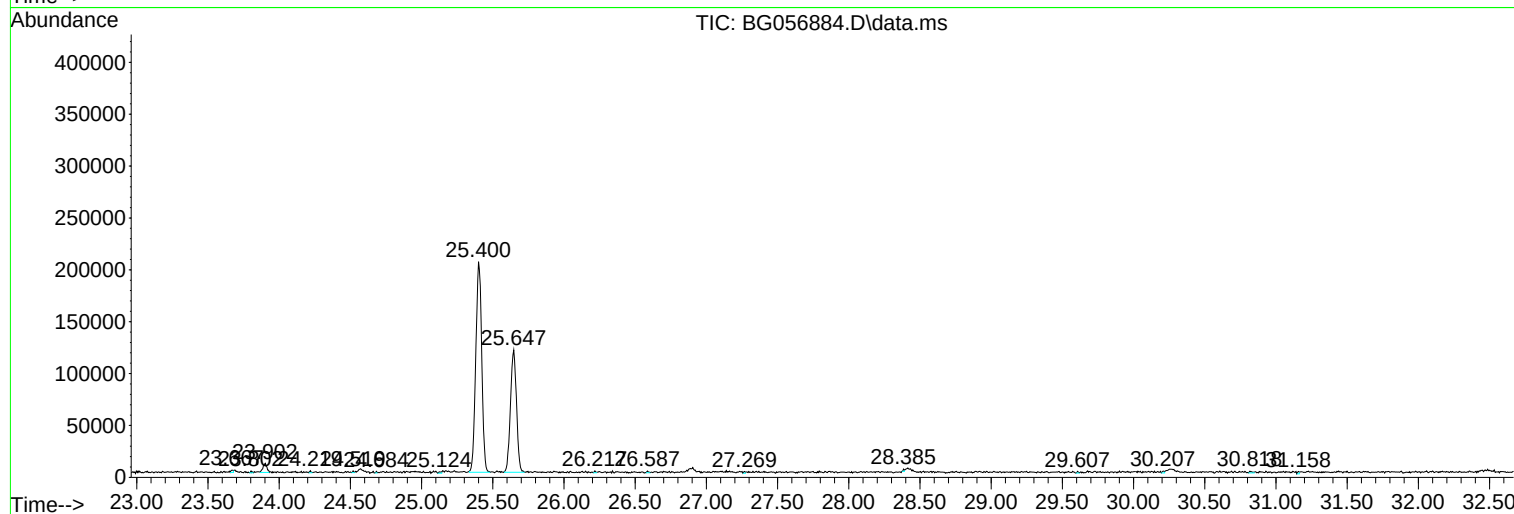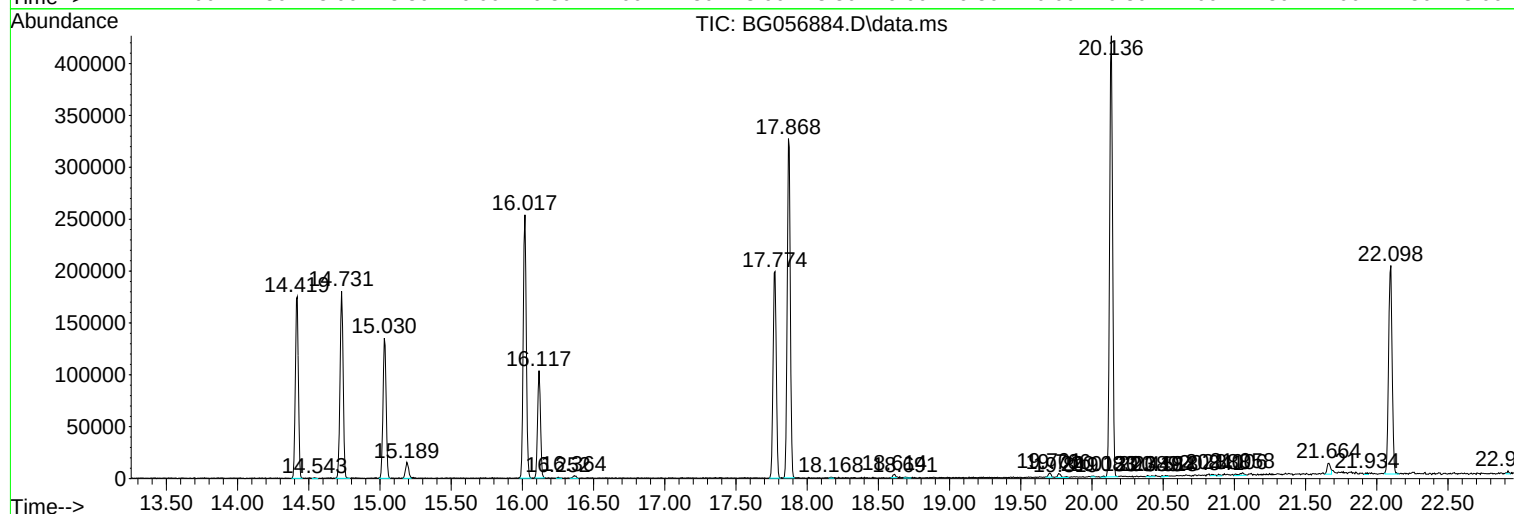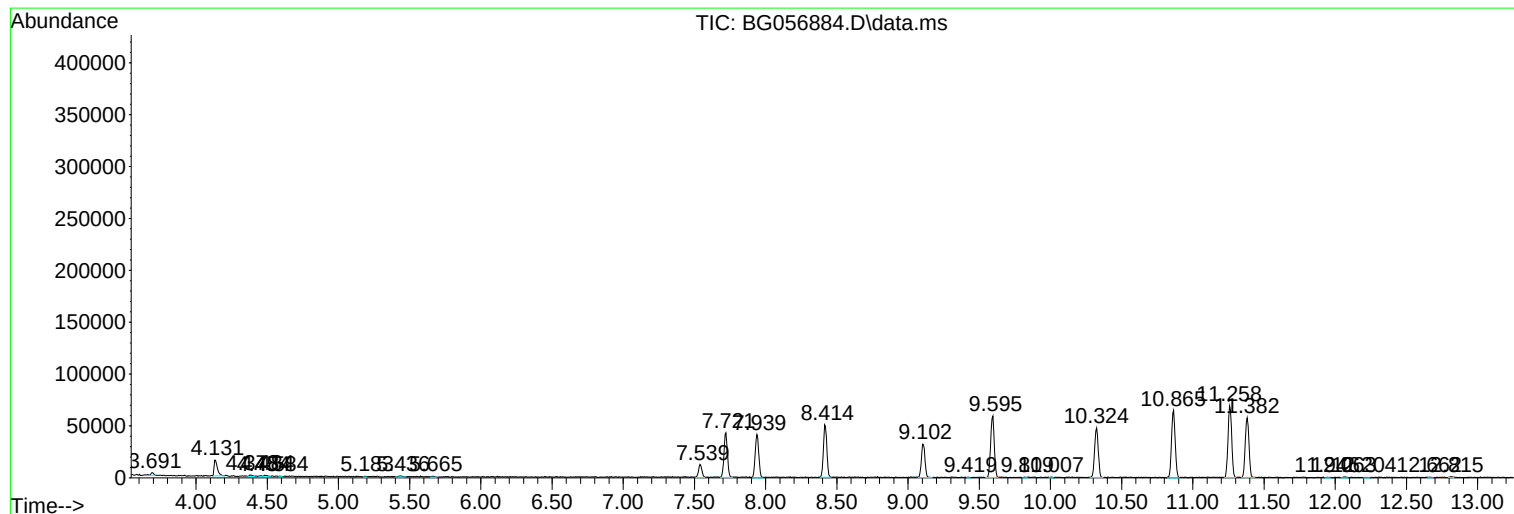

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056884.D
Acq On : 8 Mar 2023 16:24
Operator : CG/JU
Sample : 01784-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056884.D
Acq On : 8 Mar 2023 16:24
Operator : CG/JU
Sample : 01784-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc