

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056888.D
 Acq On : 8 Mar 2023 19:54
 Operator : CG/JU
 Sample : PB151260BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.685	22	25	31	rBV4	3644	5165	0.95%	0.104%
2	3.803	42	45	48	rBV3	648	866	0.16%	0.017%
3	3.920	63	65	68	rBV	855	924	0.17%	0.019%
4	4.132	98	101	112	rBV	46852	79029	14.50%	1.589%
5	4.367	137	141	146	rVB3	722	1197	0.22%	0.024%
6	4.690	192	196	198	rBV2	627	887	0.16%	0.018%
7	4.843	221	222	225	rBV2	728	779	0.14%	0.016%
8	4.937	236	238	241	rBV	716	761	0.14%	0.015%
9	5.360	305	310	313	rBV2	552	934	0.17%	0.019%
10	5.542	337	341	342	rBV2	744	963	0.18%	0.019%
11	6.458	494	497	502	rBV3	537	893	0.16%	0.018%
12	6.670	532	533	536	rBV	1003	783	0.14%	0.016%
13	7.393	654	656	662	rBV2	413	731	0.13%	0.015%
14	7.539	675	681	689	rBV	58341	97731	17.93%	1.964%
15	7.716	705	711	719	rVB	41596	70551	12.94%	1.418%
16	7.822	727	729	732	rBV	822	744	0.14%	0.015%
17	7.939	742	749	756	rBV	51711	91120	16.71%	1.832%
18	8.415	824	830	837	rBV	50916	84571	15.51%	1.700%
19	8.785	891	893	896	rBV	465	727	0.13%	0.015%
20	9.108	941	948	957	rVB	66631	115122	21.12%	2.314%
21	9.590	1023	1030	1037	rBV	56386	99144	18.19%	1.993%
22	10.324	1147	1155	1163	rBV2	48379	85563	15.69%	1.720%
23	10.865	1239	1247	1255	rBV	66184	119499	21.92%	2.402%
24	11.035	1272	1276	1279	rBV2	857	1226	0.22%	0.025%
25	11.259	1306	1314	1320	rBV	70862	125673	23.05%	2.526%
26	11.382	1328	1335	1343	rBV	70180	123962	22.74%	2.492%
27	12.816	1576	1579	1582	rVB	1225	1507	0.28%	0.030%
28	14.414	1845	1851	1857	rBV	167005	240746	44.16%	4.839%
29	14.731	1897	1905	1912	rBV2	161476	251487	46.13%	5.055%
30	15.031	1949	1956	1963	rBV	137205	213002	39.07%	4.281%
31	15.189	1976	1983	1994	rBV	84120	135530	24.86%	2.724%
32	16.018	2117	2124	2132	rVB	225018	342942	62.91%	6.893%
33	16.118	2135	2141	2147	rVV	85681	122180	22.41%	2.456%
34	17.769	2416	2422	2430	rVB	212850	319444	58.60%	6.421%
35	17.869	2432	2439	2446	rVB2	279042	423254	77.64%	8.508%
36	18.462	2537	2540	2544	rVB	661	850	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056888.D
 Acq On : 8 Mar 2023 19:54
 Operator : CG/JU
 Sample : PB151260BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	18.756	2587	2590	2593	rVB	524	753	0.14%	0.015%
38	18.903	2612	2615	2616	rBV	956	963	0.18%	0.019%
39	19.702	2747	2751	2755	rBV4	3490	5232	0.96%	0.105%
40	19.772	2759	2763	2767	rVB4	2785	4431	0.81%	0.089%
41	20.048	2808	2810	2814	rVB2	742	738	0.14%	0.015%
42	20.131	2818	2824	2831	rBV	380113	545172	100.00%	10.958%
43	21.047	2978	2980	2987	rVB5	1799	2254	0.41%	0.045%
44	21.176	3000	3002	3005	rVB	1611	1511	0.28%	0.030%
45	21.200	3005	3006	3009	rBV3	1641	1517	0.28%	0.030%
46	21.270	3016	3018	3021	rBV3	1647	1411	0.26%	0.028%
47	21.470	3050	3052	3055	rVB3	1425	930	0.17%	0.019%
48	22.093	3151	3158	3165	rBV2	216570	369952	67.86%	7.436%
49	22.916	3296	3298	3301	rBV2	1621	1274	0.23%	0.026%
50	24.567	3576	3579	3581	rBV2	2421	2946	0.54%	0.059%
51	24.614	3585	3587	3591	rBV4	1666	1551	0.28%	0.031%
52	24.772	3612	3614	3616	rBV	1480	1115	0.20%	0.022%
53	25.154	3678	3679	3683	rVB4	2157	1303	0.24%	0.026%
54	25.401	3710	3721	3733	rVB2	166282	502278	92.13%	10.096%
55	25.648	3751	3763	3774	rBV2	119077	363751	66.72%	7.312%
56	27.874	4139	4142	4143	rVB2	1507	1316	0.24%	0.026%
57	29.813	4470	4472	4475	rBV3	1545	1555	0.29%	0.031%
58	31.558	4768	4769	4770	rBV	1856	734	0.13%	0.015%
59	32.046	4850	4852	4855	rBV4	1691	1864	0.34%	0.037%




Sum of corrected areas: 4975038

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056888.D
Acq On : 8 Mar 2023 19:54
Operator : CG/JU
Sample : PB151260BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

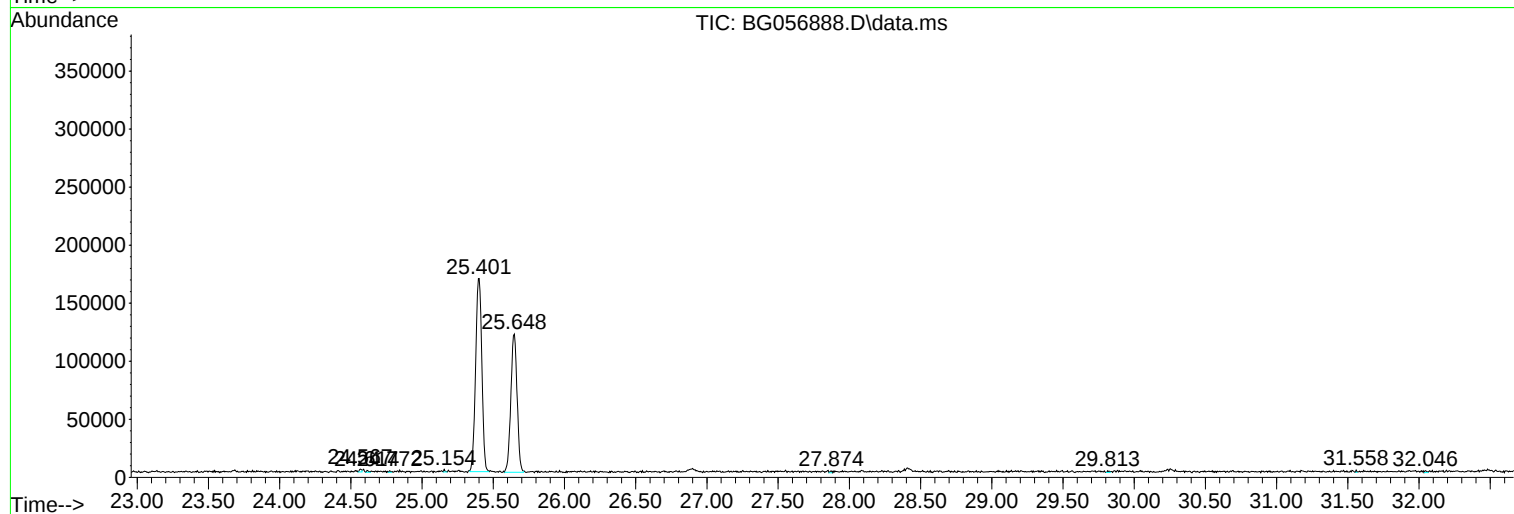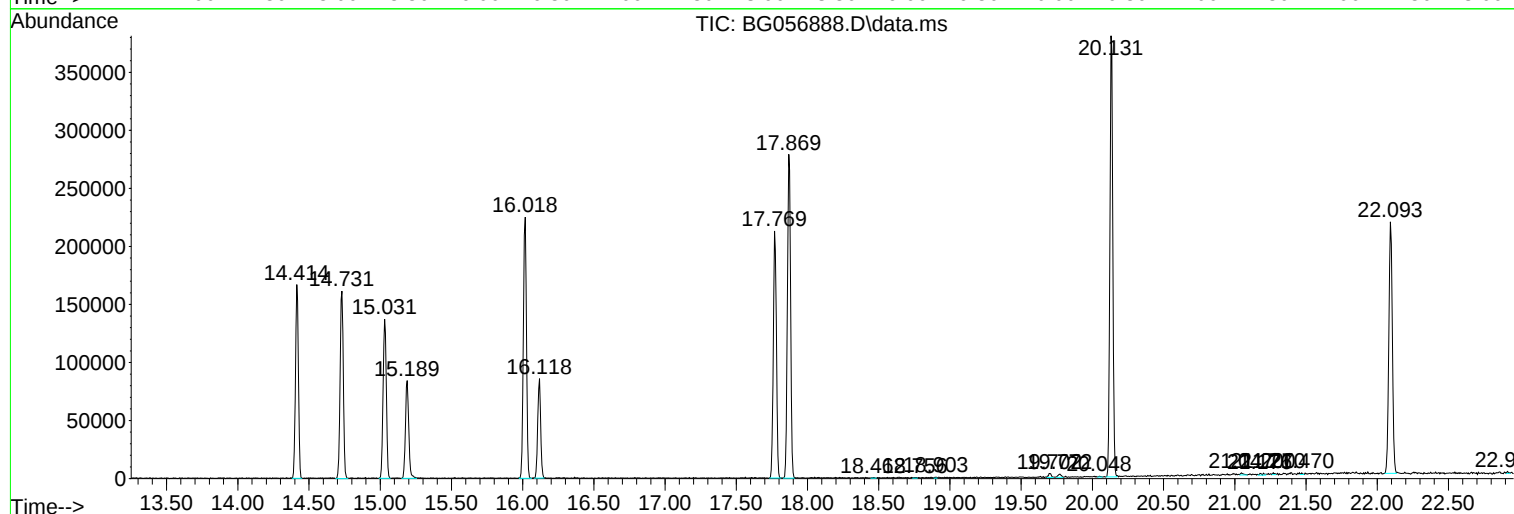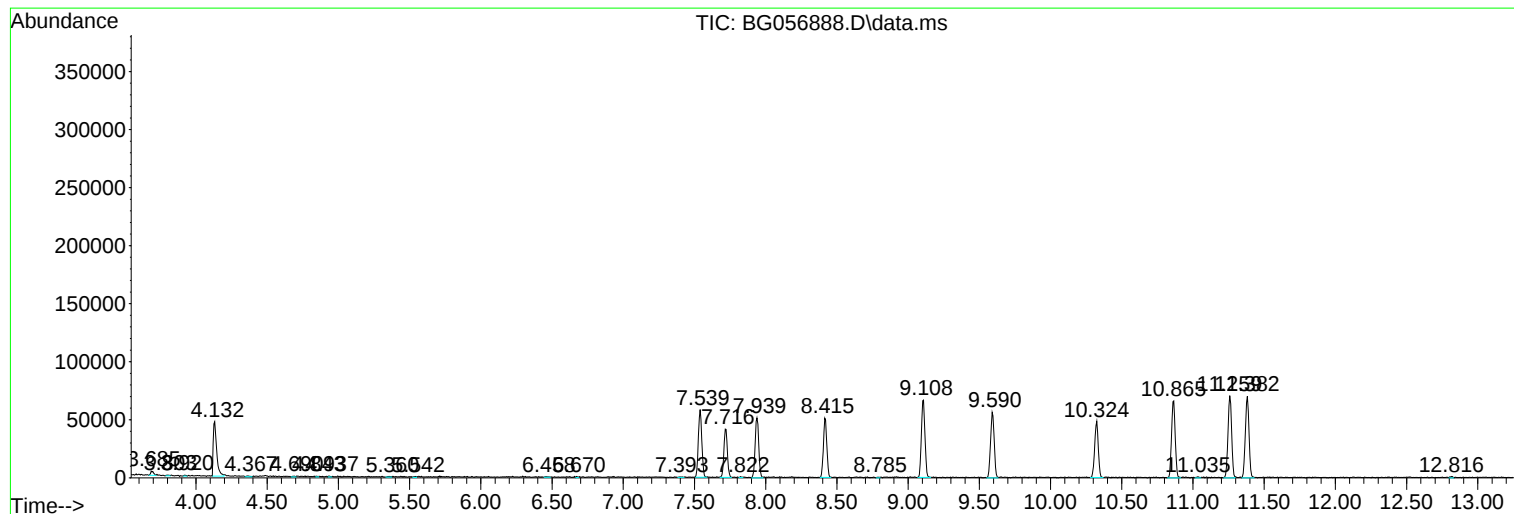

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056888.D
Acq On : 8 Mar 2023 19:54
Operator : CG/JU
Sample : PB151260BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056888.D
Acq On : 8 Mar 2023 19:54
Operator : CG/JU
Sample : PB151260BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc