

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056896.D
 Acq On : 9 Mar 2023 1:24
 Operator : CG/JU
 Sample : 01784-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056896.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.690	22	26	35	rVB2	5130	7233	0.96%	0.122%
2	4.137	98	102	108	rBV	11356	17215	2.27%	0.289%
3	4.384	139	144	147	rBV2	1820	2716	0.36%	0.046%
4	4.495	156	163	166	rVB3	1172	2095	0.28%	0.035%
5	7.539	674	681	687	rBB2	14411	24244	3.20%	0.408%
6	7.715	705	711	719	rBB	54455	90935	12.02%	1.529%
7	7.938	743	749	756	rVB	52196	87401	11.55%	1.470%
8	8.414	824	830	837	rBV	50020	85992	11.36%	1.446%
9	9.102	939	947	955	rBB2	45076	74924	9.90%	1.260%
10	9.589	1023	1030	1038	rBV	74262	135110	17.85%	2.272%
11	9.965	1091	1094	1098	rBB	1034	1144	0.15%	0.019%
12	10.318	1148	1154	1162	rBV	62344	112008	14.80%	1.883%
13	10.864	1238	1247	1254	rBV	87065	152264	20.12%	2.560%
14	11.258	1307	1314	1322	rBB	70839	130749	17.28%	2.198%
15	11.381	1328	1335	1342	rBV2	72166	126093	16.66%	2.120%
16	12.451	1512	1517	1521	rBB	2282	3047	0.40%	0.051%
17	12.809	1574	1578	1584	rVB2	1505	2162	0.29%	0.036%
18	13.397	1673	1678	1684	rBB2	1544	2319	0.31%	0.039%
19	13.626	1714	1717	1721	rVB3	1541	2087	0.28%	0.035%
20	13.890	1758	1762	1768	rVB3	2790	3771	0.50%	0.063%
21	14.413	1845	1851	1858	rVB	227494	330316	43.65%	5.554%
22	14.654	1888	1892	1898	rBV	433	1034	0.14%	0.017%
23	14.730	1898	1905	1913	rVB2	232797	355549	46.98%	5.978%
24	15.030	1950	1956	1962	rBV	139151	219157	28.96%	3.685%
25	15.189	1978	1983	1989	rVB2	21230	32179	4.25%	0.541%
26	15.788	2080	2085	2091	rVB	3004	4282	0.57%	0.072%
27	16.017	2117	2124	2131	rBV	316734	483591	63.90%	8.131%
28	16.117	2134	2141	2148	rBV	130339	180559	23.86%	3.036%
29	16.252	2161	2164	2168	rBV2	717	1140	0.15%	0.019%
30	16.364	2180	2183	2189	rVB3	1994	2624	0.35%	0.044%
31	17.392	2355	2358	2363	rBV2	3756	3971	0.52%	0.067%
32	17.768	2415	2422	2429	rBV	218700	330855	43.72%	5.563%
33	17.868	2432	2439	2447	rVB	409991	605373	79.99%	10.179%
34	18.015	2460	2464	2468	rVB2	1342	1825	0.24%	0.031%
35	18.608	2560	2565	2570	rBB3	11147	13789	1.82%	0.232%
36	18.690	2576	2579	2584	rVB	3589	3731	0.49%	0.063%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056896.D
 Acq On : 9 Mar 2023 1:24
 Operator : CG/JU
 Sample : 01784-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCAC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	18.890	2609	2613	2619	rBV2	814	1942	0.26%	0.033%
38	19.701	2748	2751	2756	rVV4	5492	6928	0.92%	0.116%
39	19.766	2758	2762	2767	rVB2	4941	6913	0.91%	0.116%
40	20.006	2801	2803	2805	rVB3	2227	1830	0.24%	0.031%
41	20.136	2818	2825	2832	rVB	533493	756767	100.00%	12.725%
42	21.657	3080	3084	3093	rBV5	17751	36984	4.89%	0.622%
43	22.092	3151	3158	3165	rBV	215671	373499	49.35%	6.280%
44	22.239	3181	3183	3184	rBV	2012	1225	0.16%	0.021%
45	22.498	3223	3227	3228	rBV3	1568	1446	0.19%	0.024%
46	22.844	3284	3286	3287	rBV2	1673	1045	0.14%	0.018%
47	23.902	3461	3466	3473	rVB4	13517	25597	3.38%	0.430%
48	24.131	3503	3505	3507	rBV3	2294	1960	0.26%	0.033%
49	25.400	3710	3721	3735	rVB2	238433	714417	94.40%	12.013%
50	25.641	3750	3762	3773	rBV2	120490	367298	48.54%	6.176%
51	25.829	3793	3794	3795	rBV	2230	1035	0.14%	0.017%
52	26.675	3936	3938	3939	rBV2	1667	1210	0.16%	0.020%
53	26.887	3972	3974	3979	rVB5	2690	3596	0.48%	0.060%
54	29.008	4334	4335	4339	rBV4	2149	1897	0.25%	0.032%
55	31.593	4773	4775	4779	rBV3	2073	2160	0.29%	0.036%
56	31.652	4784	4785	4787	rBV	2049	1739	0.23%	0.029%
57	32.439	4915	4919	4922	rBV5	2413	4266	0.56%	0.072%




Sum of corrected areas: 5947238

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056896.D
Acq On : 9 Mar 2023 1:24
Operator : CG/JU
Sample : 01784-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

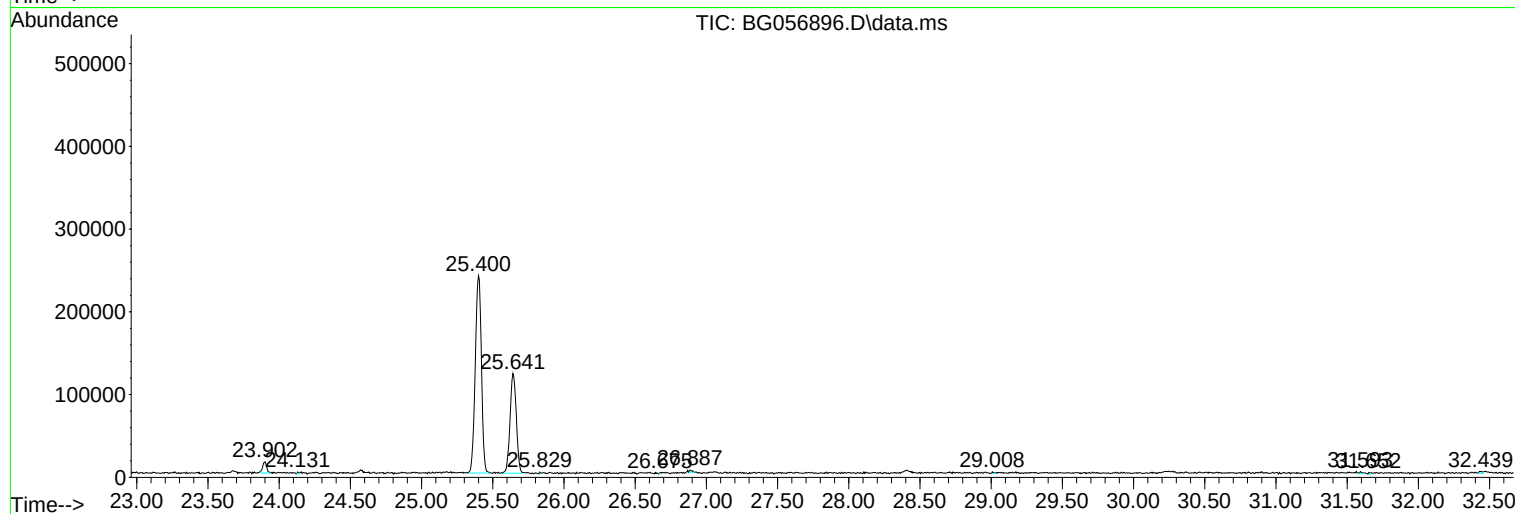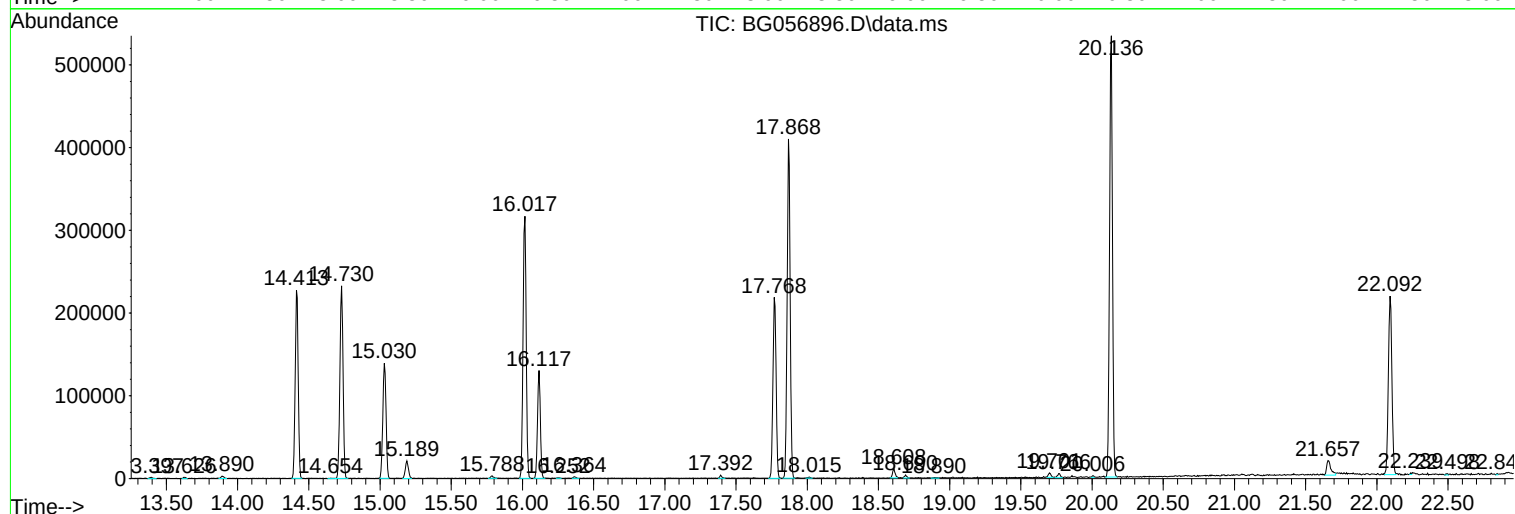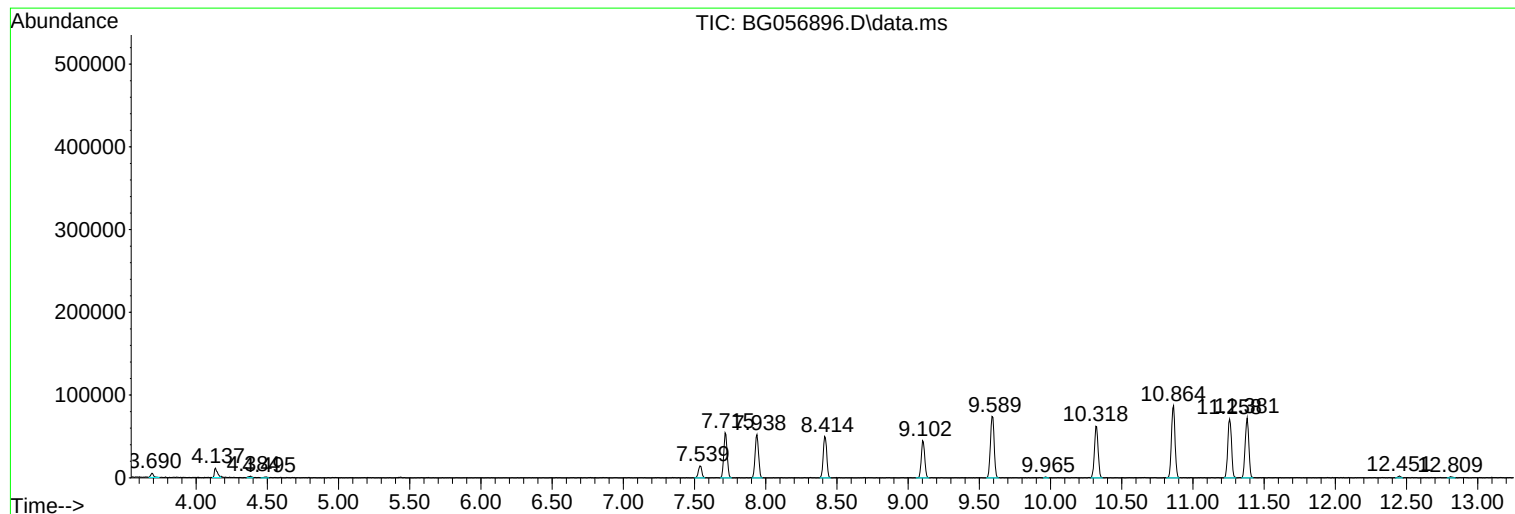

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056896.D
Acq On : 9 Mar 2023 1:24
Operator : CG/JU
Sample : 01784-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056896.D
Acq On : 9 Mar 2023 1:24
Operator : CG/JU
Sample : 01784-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCAC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc