

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056902.D
 Acq On : 9 Mar 2023 6:11
 Operator : CG/JU
 Sample : PB151262BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.691	21	26	31	rVB3	4827	8008	1.09%	0.129%
2	4.126	97	100	113	rBV	64898	109725	14.88%	1.763%
3	7.539	674	681	688	rBB	79345	136486	18.50%	2.192%
4	7.716	705	711	719	rBB	57355	92584	12.55%	1.487%
5	7.939	742	749	756	rBB	70829	121632	16.49%	1.954%
6	8.415	824	830	836	rBV2	47283	77257	10.47%	1.241%
7	9.102	940	947	956	rBB	94273	161363	21.88%	2.592%
8	9.590	1023	1030	1037	rBB	75726	129883	17.61%	2.086%
9	10.319	1148	1154	1161	rBB2	65171	116655	15.81%	1.874%
10	10.859	1240	1246	1254	rBV	94395	165334	22.41%	2.656%
11	11.259	1307	1314	1321	rVB	64523	114143	15.47%	1.834%
12	11.376	1327	1334	1342	rBB	93738	170006	23.05%	2.731%
13	12.816	1574	1579	1584	rBB3	1378	2405	0.33%	0.039%
14	14.414	1845	1851	1858	rVB	229779	325200	44.09%	5.224%
15	14.725	1897	1904	1913	rBV	216316	341666	46.32%	5.488%
16	15.031	1949	1956	1963	rBV	126745	195145	26.46%	3.135%
17	15.189	1976	1983	1996	rBV2	118520	190282	25.80%	3.057%
18	16.018	2116	2124	2130	rBV	310676	466649	63.26%	7.496%
19	16.118	2134	2141	2148	rBV	112638	171899	23.30%	2.761%
20	17.769	2416	2422	2432	rVB	197904	299157	40.56%	4.806%
21	17.869	2432	2439	2446	rBV2	378006	581817	78.88%	9.346%
22	19.702	2745	2751	2756	rBV2	5405	8015	1.09%	0.129%
23	19.766	2756	2762	2768	rBV	4838	7232	0.98%	0.116%
24	19.925	2787	2789	2792	rBV	998	1079	0.15%	0.017%
25	20.131	2815	2824	2832	rBV	527124	737643	100.00%	11.849%
26	20.483	2882	2884	2887	rBV	925	1046	0.14%	0.017%
27	20.548	2891	2895	2897	rBV2	973	1408	0.19%	0.023%
28	20.730	2925	2926	2930	rBV2	1255	1918	0.26%	0.031%
29	20.759	2930	2931	2936	rVB4	1176	1642	0.22%	0.026%
30	21.012	2971	2974	2975	rVB2	1607	1602	0.22%	0.026%
31	21.053	2979	2981	2984	rVB2	1706	1458	0.20%	0.023%
32	21.129	2991	2994	2996	rVB3	1133	1118	0.15%	0.018%
33	21.570	3068	3069	3072	rBV2	1069	1149	0.16%	0.018%
34	21.682	3086	3088	3092	rVB3	1280	1328	0.18%	0.021%
35	21.746	3095	3099	3102	rBV4	2242	3390	0.46%	0.054%
36	21.881	3120	3122	3125	rVB3	1379	1126	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056902.D
 Acq On : 9 Mar 2023 6:11
 Operator : CG/JU
 Sample : PB151262BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	21.928	3129	3130	3134	rBV4	1217	1119	0.15%	0.018%
38	22.093	3151	3158	3165	rVV2	194915	345483	46.84%	5.550%
39	22.816	3276	3281	3282	rBV2	1130	2035	0.28%	0.033%
40	22.851	3285	3287	3288	rVB	2216	1215	0.16%	0.020%
41	22.863	3288	3289	3291	rBV	2071	1298	0.18%	0.021%
42	22.892	3291	3294	3295	rBV3	1117	1157	0.16%	0.019%
43	23.062	3322	3323	3327	rBV2	879	1194	0.16%	0.019%
44	23.256	3352	3356	3359	rVB5	1287	1956	0.27%	0.031%
45	23.438	3385	3387	3388	rBV2	1061	1071	0.15%	0.017%
46	23.603	3413	3415	3418	rVB3	1750	1831	0.25%	0.029%
47	23.644	3420	3422	3425	rVV3	1939	2206	0.30%	0.035%
48	23.673	3425	3427	3429	rVV3	2260	2634	0.36%	0.042%
49	23.691	3429	3430	3435	rVV5	2312	2676	0.36%	0.043%
50	23.750	3439	3440	3444	rVV4	1526	1772	0.24%	0.028%
51	23.791	3444	3447	3451	rVV5	1483	2210	0.30%	0.036%
52	23.820	3451	3452	3455	rVV3	2193	1561	0.21%	0.025%
53	23.985	3478	3480	3482	rVB3	1597	1059	0.14%	0.017%
54	24.214	3517	3519	3522	rBV3	991	1241	0.17%	0.020%
55	24.396	3546	3550	3552	rBV4	2530	3623	0.49%	0.058%
56	24.802	3612	3619	3622	rBV5	1512	2728	0.37%	0.044%
57	24.849	3626	3627	3630	rVV2	2064	1752	0.24%	0.028%
58	24.925	3636	3640	3642	rBV4	1195	1666	0.23%	0.027%
59	25.125	3671	3674	3677	rBV4	1938	2852	0.39%	0.046%
60	25.401	3709	3721	3732	rVV2	233177	691885	93.80%	11.114%
61	25.642	3752	3762	3774	rVV2	110409	333826	45.26%	5.362%
62	25.724	3774	3776	3778	rVB2	1720	1241	0.17%	0.020%
63	26.206	3855	3858	3859	rBV2	1122	1213	0.16%	0.019%
64	26.570	3917	3920	3923	rVV4	1114	1555	0.21%	0.025%
65	26.652	3931	3934	3937	rBV3	1300	2073	0.28%	0.033%
66	26.881	3969	3973	3981	rVV9	3281	8238	1.12%	0.132%
67	26.993	3990	3992	3994	rBV2	1271	1133	0.15%	0.018%
68	27.269	4037	4039	4040	rBV2	1588	1125	0.15%	0.018%
69	27.393	4057	4060	4061	rBV2	1166	1345	0.18%	0.022%
70	27.516	4079	4081	4084	rVB4	1348	1380	0.19%	0.022%
71	27.545	4084	4086	4089	rVB3	1191	1169	0.16%	0.019%
72	27.634	4099	4101	4103	rBV2	1127	1136	0.15%	0.018%
73	27.657	4103	4105	4107	rVB3	1155	1138	0.15%	0.018%
74	27.816	4130	4132	4135	rBV3	1232	1120	0.15%	0.018%
75	27.845	4135	4137	4139	rBV2	1178	1188	0.16%	0.019%
76	28.374	4225	4227	4228	rBV2	2154	2053	0.28%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056902.D
 Acq On : 9 Mar 2023 6:11
 Operator : CG/JU
 Sample : PB151262BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

77	28.397	4229	4231	4232	rVB2	1718	1080	0.15%	0.017%
78	28.756	4289	4292	4295	rBV3	1079	1542	0.21%	0.025%
79	28.862	4309	4310	4314	rBV3	1099	1258	0.17%	0.020%
80	29.008	4332	4335	4336	rBV2	1149	1055	0.14%	0.017%
81	29.126	4353	4355	4358	rBV3	956	1233	0.17%	0.020%
82	29.373	4395	4397	4404	rVB4	1539	2600	0.35%	0.042%
83	29.496	4416	4418	4421	rVB4	1482	1669	0.23%	0.027%
84	29.543	4424	4426	4429	rBV3	1299	1536	0.21%	0.025%
85	30.136	4524	4527	4528	rBV2	993	1060	0.14%	0.017%
86	30.189	4531	4536	4538	rBV3	1533	2104	0.29%	0.034%
87	30.219	4538	4541	4542	rBV3	2158	1838	0.25%	0.030%
88	30.236	4542	4544	4547	rVB4	1430	1472	0.20%	0.024%
89	30.348	4561	4563	4566	rVB3	1150	1096	0.15%	0.018%
90	30.471	4582	4584	4588	rVV4	1699	1890	0.26%	0.030%
91	30.742	4627	4630	4633	rVB4	1450	1483	0.20%	0.024%
92	31.024	4676	4678	4682	rBV4	1756	1876	0.25%	0.030%
93	31.188	4703	4706	4709	rBV4	1336	2132	0.29%	0.034%
94	31.229	4711	4713	4716	rVV3	1207	1430	0.19%	0.023%
95	31.253	4716	4717	4719	rVB2	1618	1079	0.15%	0.017%
96	31.423	4744	4746	4748	rBV3	1993	1972	0.27%	0.032%
97	31.488	4755	4757	4760	rBV2	1167	1270	0.17%	0.020%
98	32.087	4857	4859	4863	rVV5	1410	1563	0.21%	0.025%
99	32.387	4907	4910	4912	rBV3	1386	1803	0.24%	0.029%
100	32.587	4943	4944	4947	rBV2	1773	1570	0.21%	0.025%




Sum of corrected areas: 6225218

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056902.D
Acq On : 9 Mar 2023 6:11
Operator : CG/JU
Sample : PB151262BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK262

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

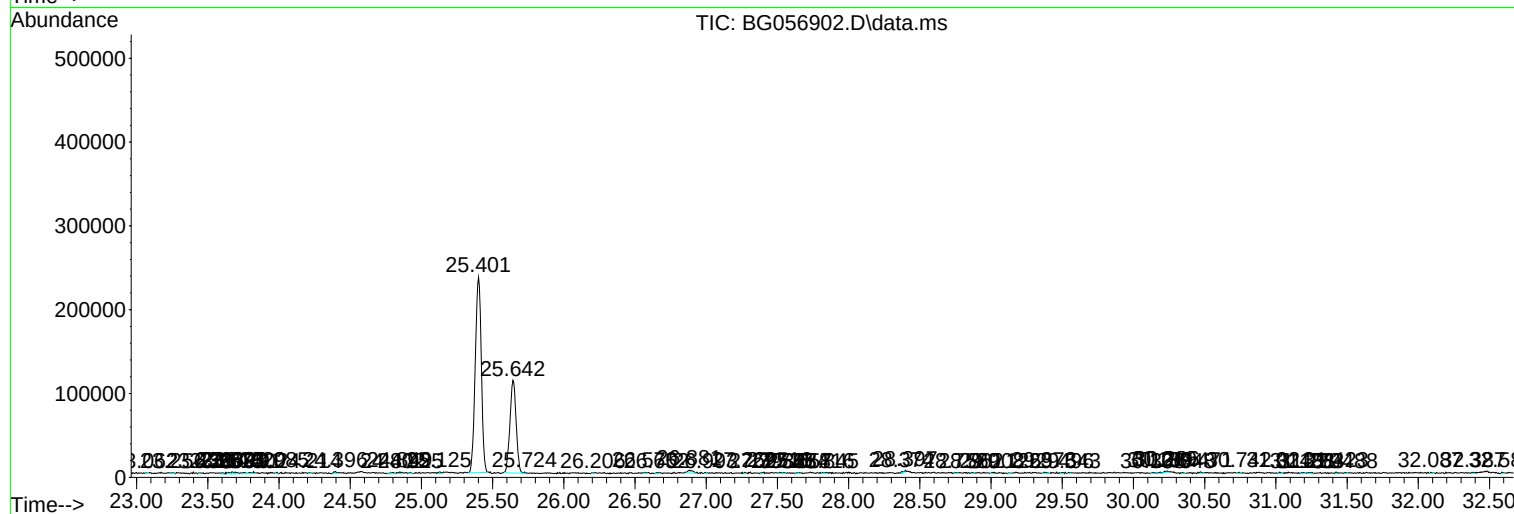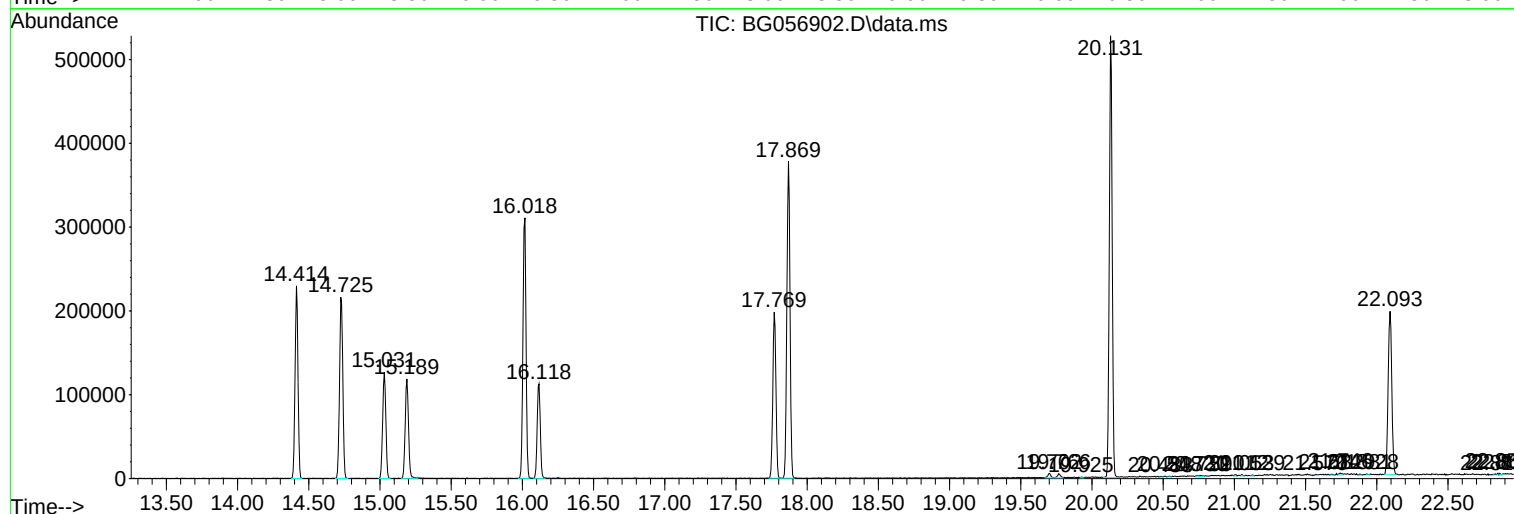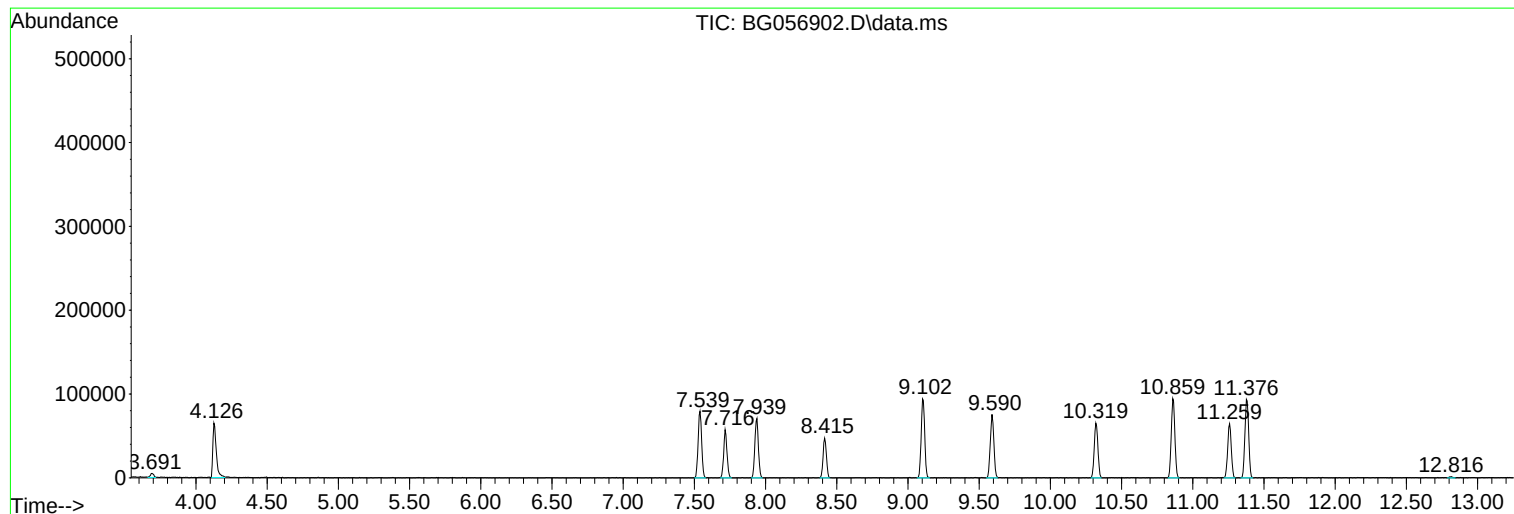

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056902.D
Acq On : 9 Mar 2023 6:11
Operator : CG/JU
Sample : PB151262BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK262

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056902.D
Acq On : 9 Mar 2023 6:11
Operator : CG/JU
Sample : PB151262BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK262

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc